

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
 Data File : FG004595.D
 Signal(s) : FID1A.ch
 Acq On : 04 Apr 2019 17:15
 Operator : AJ\SJ
 Sample : K2240-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 SB-02-(0-2)-DUP

Integration File: autoint1.e
 Quant Time: Apr 05 01:41:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.413	1895105	18.373 ug/ml
Target Compounds			
4) N-TETRADECANE	8.027f	550846	5.084 ug/ml
12) N-OCTACOSANE	16.587	211140	1.825 ug/ml
13) N-TRIACONTANE	17.476	231897	1.955 ug/ml
14) N-DOTRIACONTANE	18.309	207180	1.767 ug/ml
15) N-TETRATRIACONTANE	19.093	62659	0.562 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
Data File : FG004595.D
Signal(s) : FID1A.ch
Acq On : 04 Apr 2019 17:15
Operator : AJ\SJ
Sample : K2240-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-02-(0-2)-DUP

Integration File: autoint1.e
Quant Time: Apr 05 01:41:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

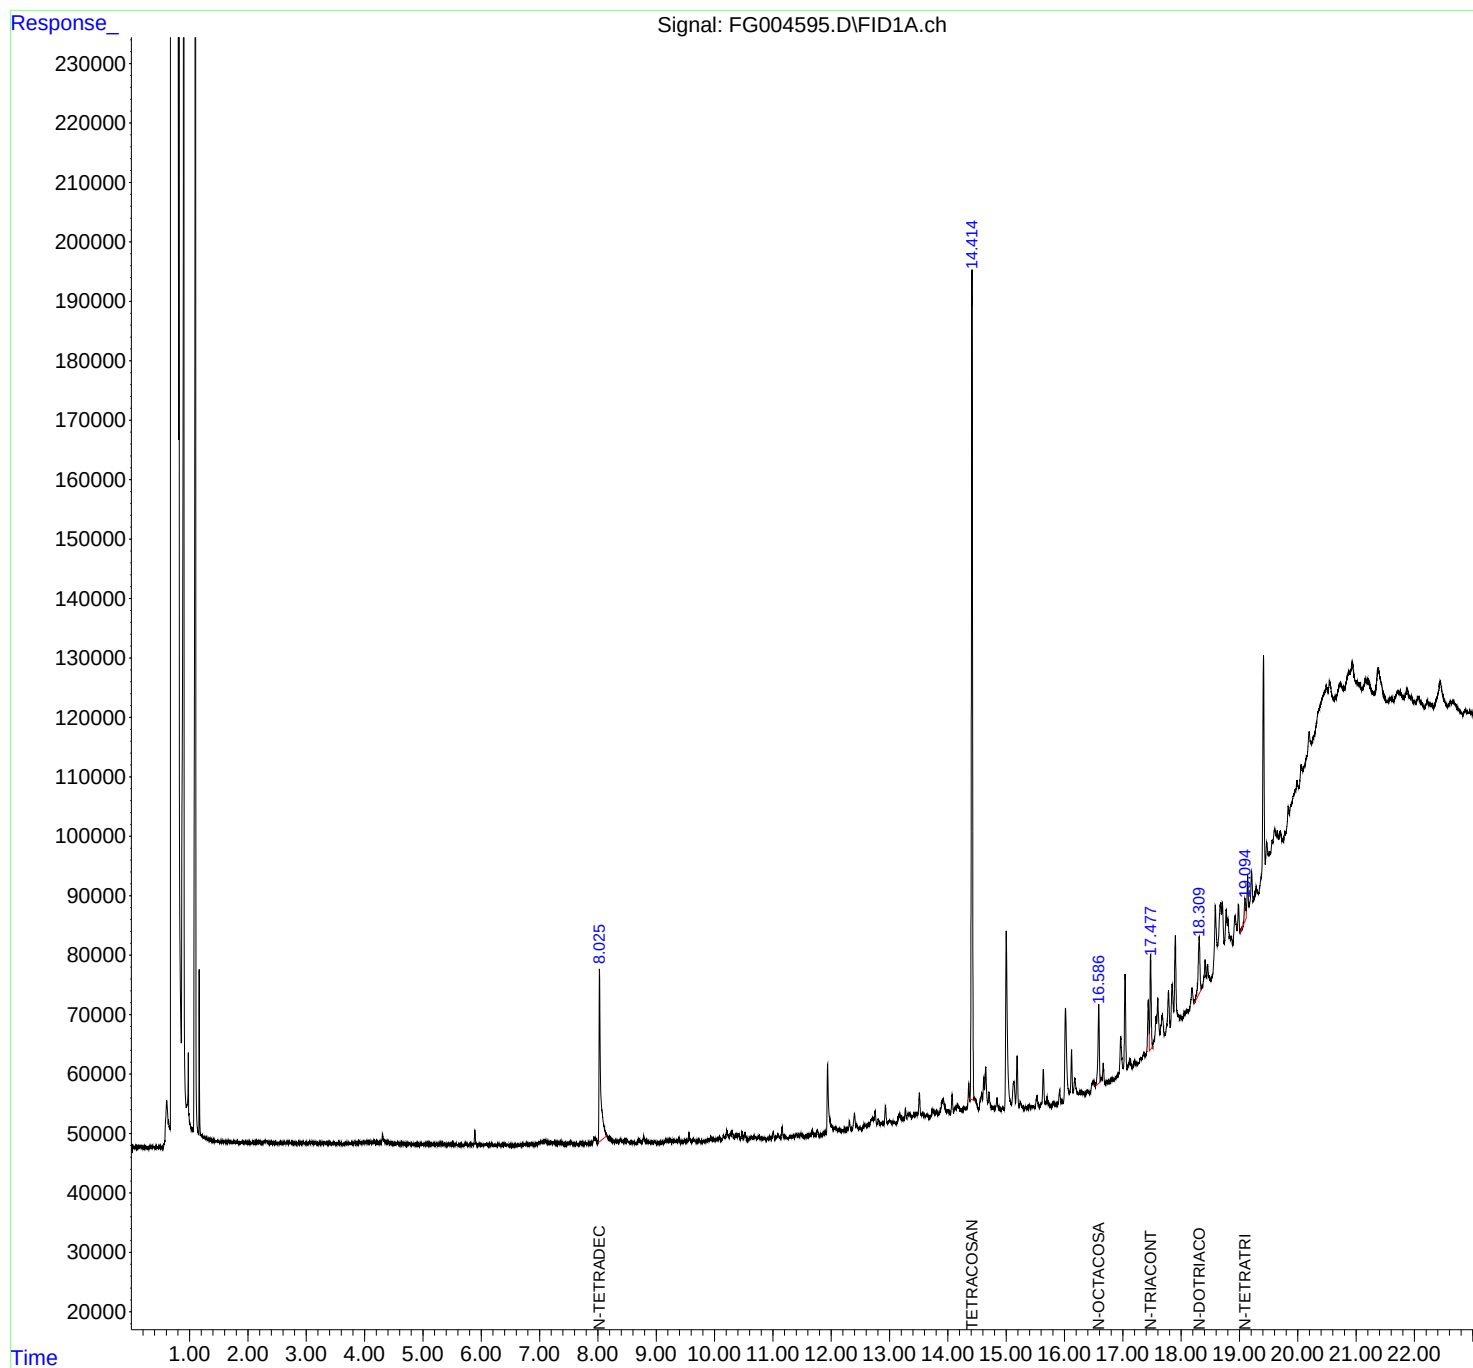


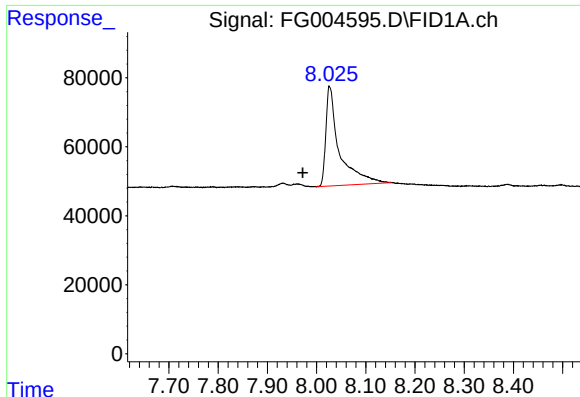

#4 N-TETRADECANE


R.T.: 8.027 min
Delta R.T.: 0.055 min
Response: 550846
Conc: 5.08 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-02-(0-2)-DUP

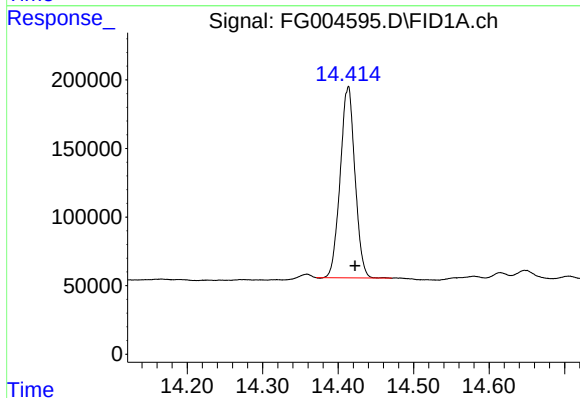


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.413 min
Delta R.T.: -0.009 min
Response: 1895105
Conc: 18.37 ug/ml

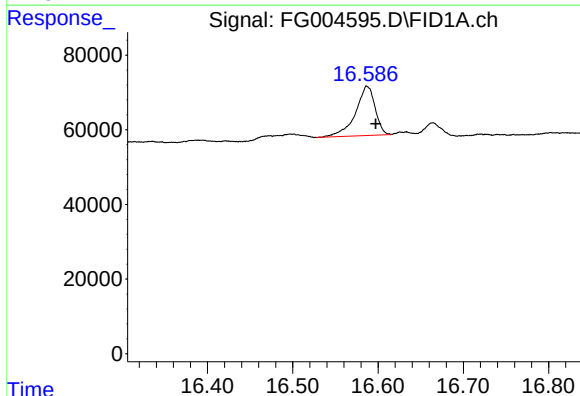


#12 N-OCTACOSANE

R.T.: 16.587 min
Delta R.T.: -0.010 min
Response: 211140
Conc: 1.83 ug/ml

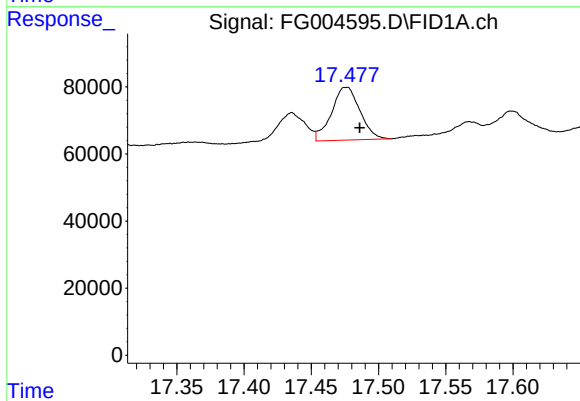

#13 N-TRIACONTANE


R.T.: 17.476 min
Delta R.T.: -0.010 min
Response: 231897
Conc: 1.95 ug/ml

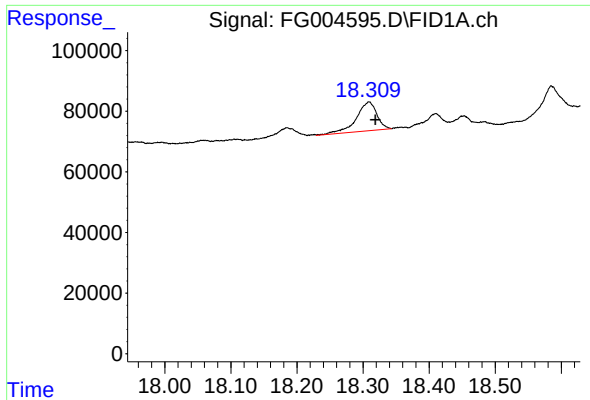

#14 N-DOTRIACONTANE

R.T.: 18.309 min
Delta R.T.: -0.009 min
Response: 207180
Conc: 1.77 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-02-(0-2)-DUP

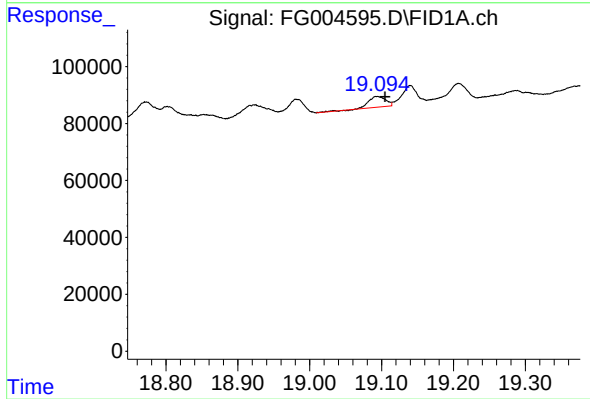

#15 N-TETRATRIACONTANE

R.T.: 19.093 min
Delta R.T.: -0.012 min
Response: 62659
Conc: 0.56 ug/ml