

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
 Data File : FG004597.D
 Signal(s) : FID1A.ch
 Acq On : 04 Apr 2019 18:17
 Operator : AJ\SJ
 Sample : K2240-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 SB-03-(0-6)

Integration File: autoint1.e
 Quant Time: Apr 05 01:42:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.416	2208470	21.411 ug/ml
Target Compounds			
4) N-TETRADECANE	8.026f	353134	3.259 ug/ml
6) N-OCTADECANE	11.040	91317	0.805 ug/ml
7) N-EICOSANE	12.370	583172	5.101 ug/ml
10) N-TETRACOSANE	14.612	512526	4.437 ug/ml
11) N-HEXACOSANE	15.638	184169	1.607 ug/ml
12) N-OCTACOSANE	16.591	724423	6.262 ug/ml
13) N-TRIACONTANE	17.474	958855	8.083 ug/ml
14) N-DOTRIACONTANE	18.309	1181994	10.080 ug/ml
15) N-TETRATRIACONTANE	19.105	556771	4.997 ug/ml
16) N-HEXATRIACONTANE	19.842	406450	3.646 ug/ml
17) N-OCTATRIACONTANE	20.555	261674	2.633 ug/ml
18) N-TETRACONTANE	21.387	200336	1.852 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
Data File : FG004597.D
Signal(s) : FID1A.ch
Acq On : 04 Apr 2019 18:17
Operator : AJ\SJ
Sample : K2240-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :
SB-03-(0-6)

Integration File: autoint1.e
Quant Time: Apr 05 01:42:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

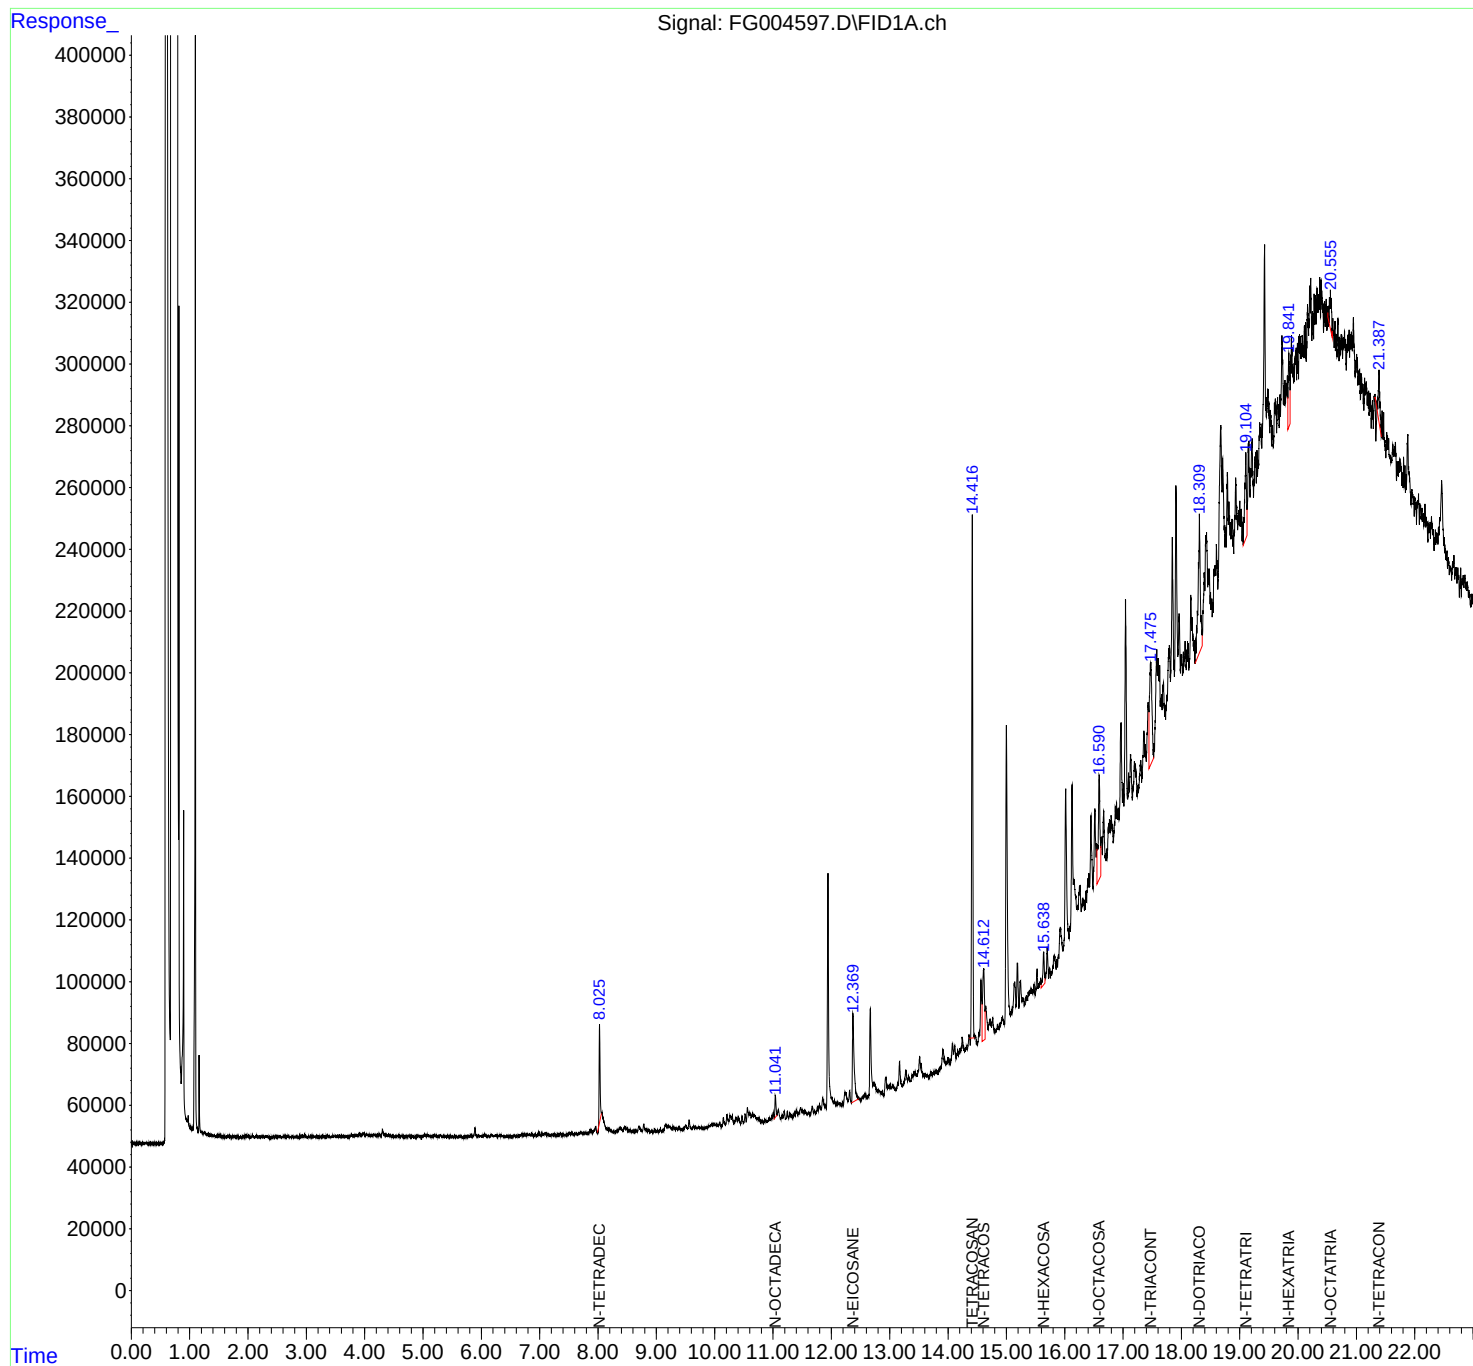


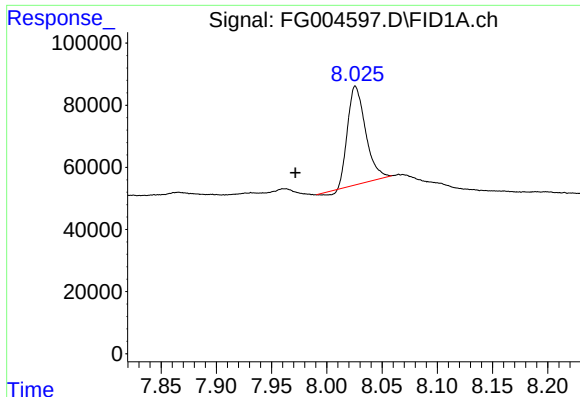

#4 N-TETRADECANE


R.T.: 8.026 min
Delta R.T.: 0.054 min
Response: 353134
Conc: 3.26 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-03-(0-6)

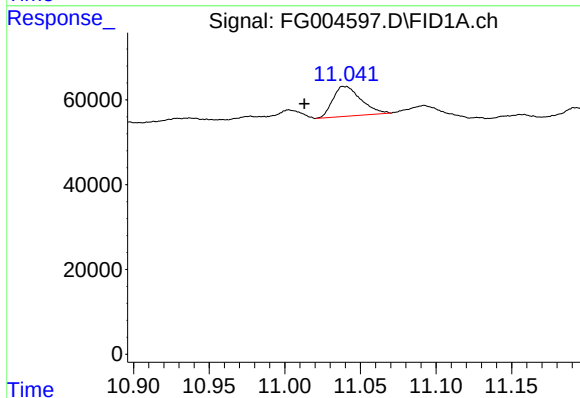


#6 N-OCTADECANE

R.T.: 11.040 min
Delta R.T.: 0.027 min
Response: 91317
Conc: 0.81 ug/ml

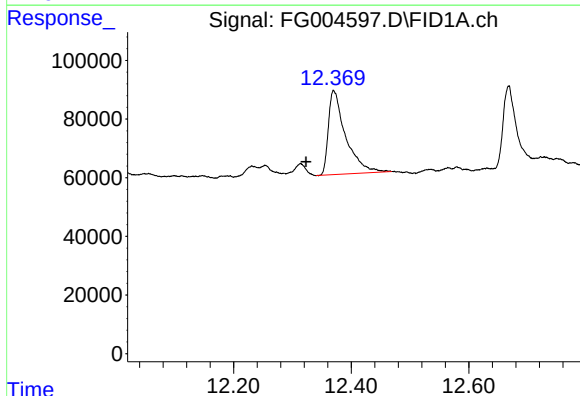


#7 N-EICOSANE

R.T.: 12.370 min
Delta R.T.: 0.047 min
Response: 583172
Conc: 5.10 ug/ml

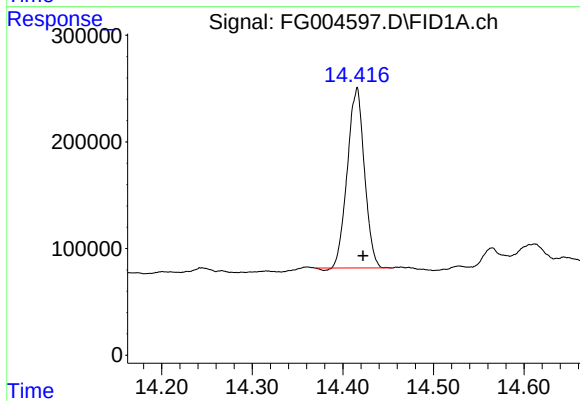

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.416 min
Delta R.T.: -0.007 min
Response: 2208470
Conc: 21.41 ug/ml

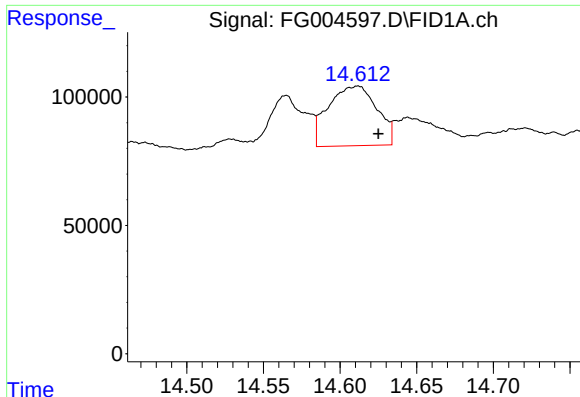

#10 N-TETRACOSANE


R.T.: 14.612 min
Delta R.T.: -0.013 min
Response: 512526
Conc: 4.44 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-03-(0-6)

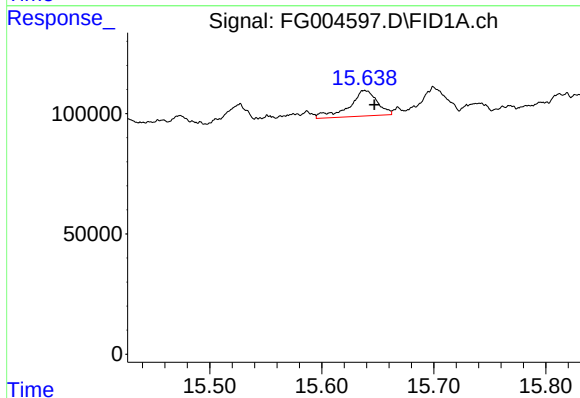


#11 N-HEXACOSANE

R.T.: 15.638 min
Delta R.T.: -0.009 min
Response: 184169
Conc: 1.61 ug/ml

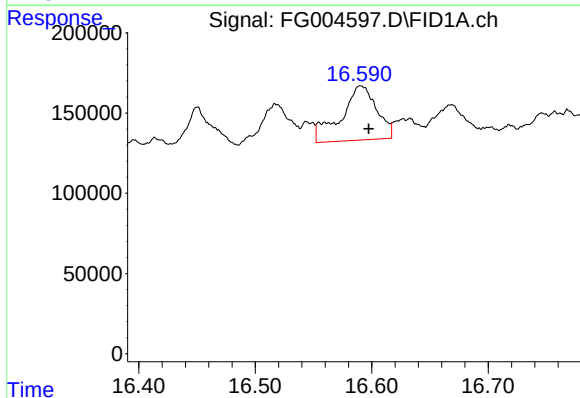


#12 N-OCTACOSANE

R.T.: 16.591 min
Delta R.T.: -0.006 min
Response: 724423
Conc: 6.26 ug/ml

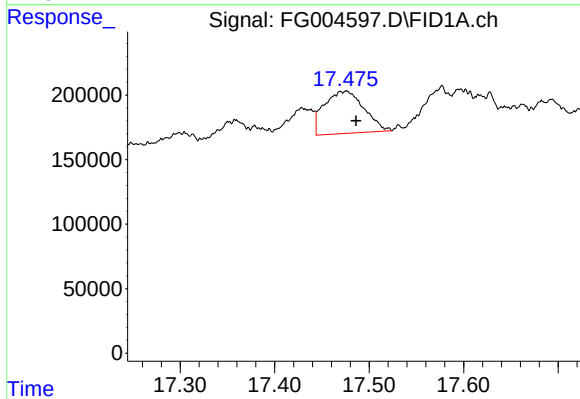

#13 N-TRIACONTANE


R.T.: 17.474 min
Delta R.T.: -0.012 min
Response: 958855
Conc: 8.08 ug/ml

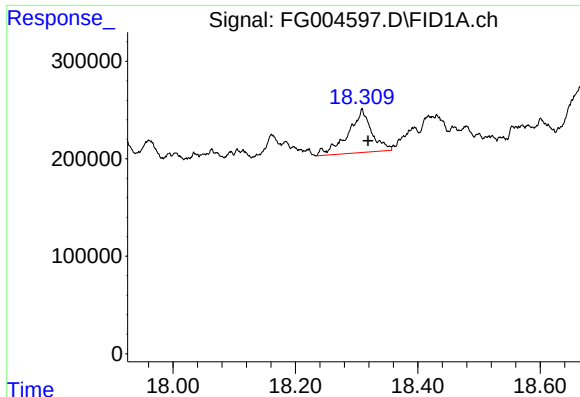

#14 N-DOTRIACONTANE


R.T.: 18.309 min
Delta R.T.: -0.009 min
Response: 1181994
Conc: 10.08 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-03-(0-6)

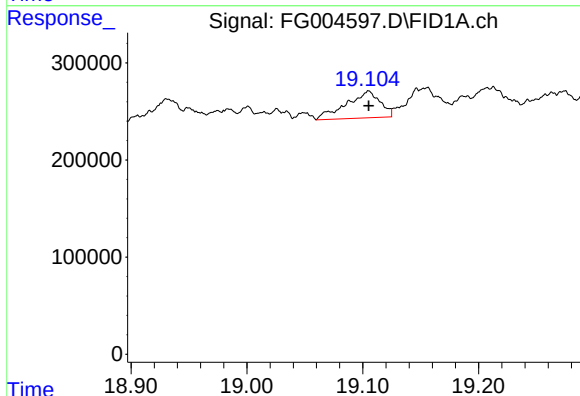


#15 N-TETRATRIACONTANE

R.T.: 19.105 min
Delta R.T.: 0.000 min
Response: 556771
Conc: 5.00 ug/ml

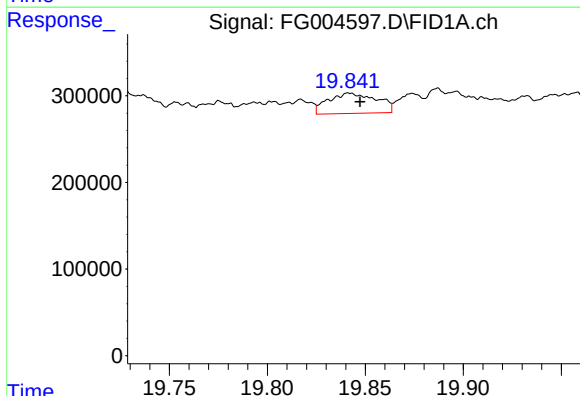


#16 N-HEXATRIACONTANE

R.T.: 19.842 min
Delta R.T.: -0.005 min
Response: 406450
Conc: 3.65 ug/ml

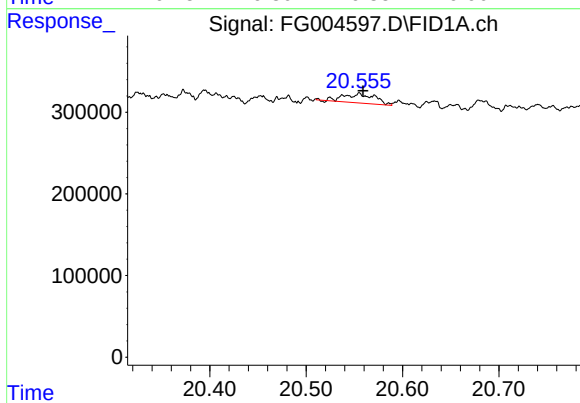

#17 N-OCTATRIACONTANE

R.T.: 20.555 min
Delta R.T.: -0.004 min
Response: 261674
Conc: 2.63 ug/ml

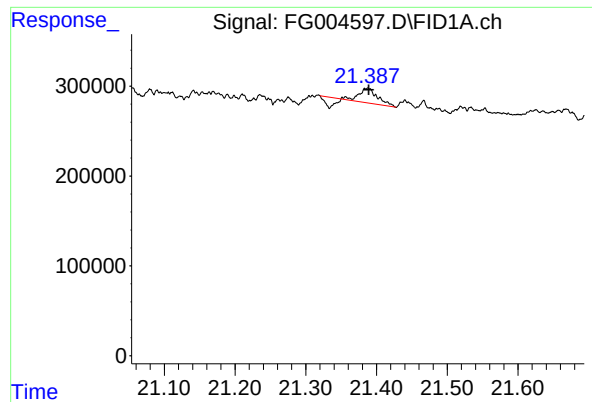

#18 N-TETRACONTANE

R.T.: 21.387 min
Delta R.T.: -0.002 min
Response: 200336
Conc: 1.85 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-03-(0-6)