

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
 Data File : FG004599.D
 Signal(s) : FID1A.ch
 Acq On : 04 Apr 2019 19:19
 Operator : AJ\SJ
 Sample : K2240-08 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 SB-03-(0-6)

Integration File: autoint1.e
 Quant Time: Apr 05 01:43:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.413	219569	2.129 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.590	99762	0.862 ug/ml
13) N-TRIACONTANE	17.479	158957	1.340 ug/ml
14) N-DOTRIACONTANE	18.310	144851	1.235 ug/ml
15) N-TETRATRIACONTANE	19.100	127449	1.144 ug/ml
16) N-HEXATRIACONTANE	19.859	235728	2.115 ug/ml
17) N-OCTATRIACONTANE	20.493f	104118	1.048 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
Data File : FG004599.D
Signal(s) : FID1A.ch
Acq On : 04 Apr 2019 19:19
Operator : AJ\SJ
Sample : K2240-08 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-03-(0-6)

Integration File: autoint1.e
Quant Time: Apr 05 01:43:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

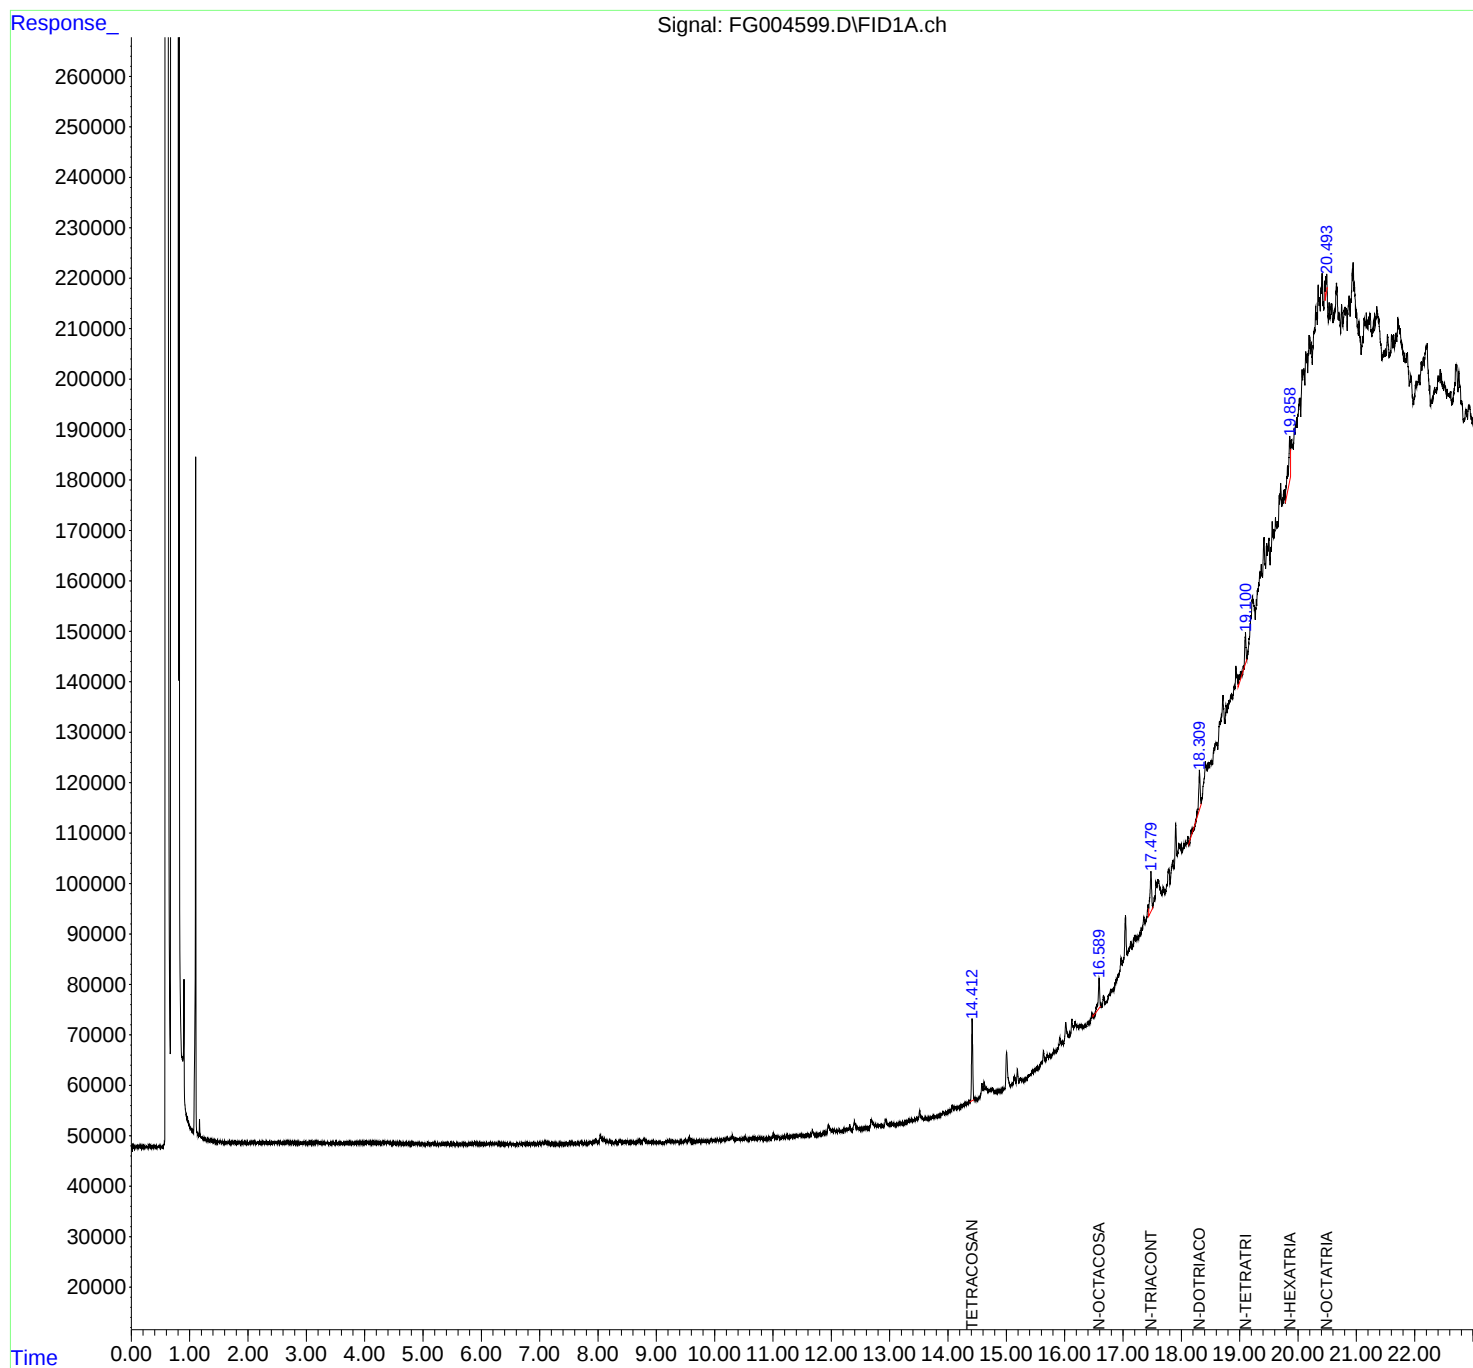


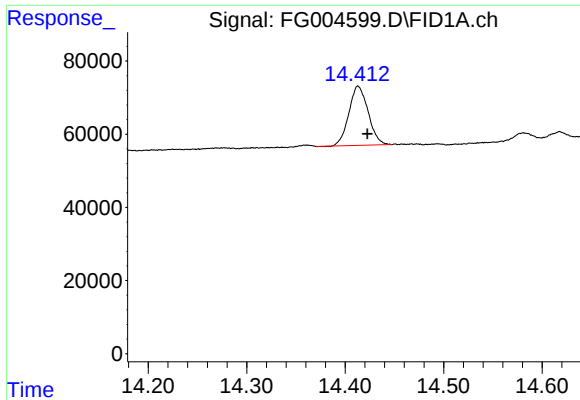

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.413 min
Delta R.T.: -0.009 min
Response: 219569
Conc: 2.13 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-03-(0-6)

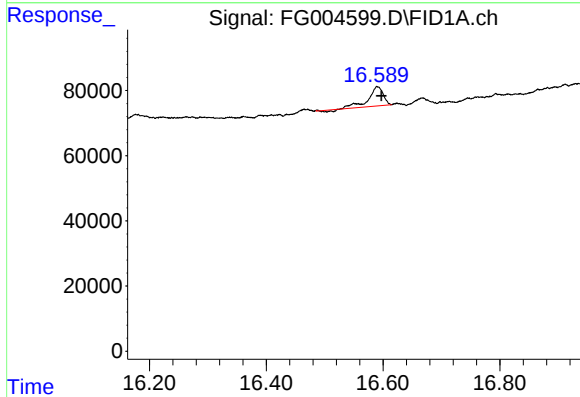


#12 N-OCTACOSANE

R.T.: 16.590 min
Delta R.T.: -0.007 min
Response: 99762
Conc: 0.86 ug/ml

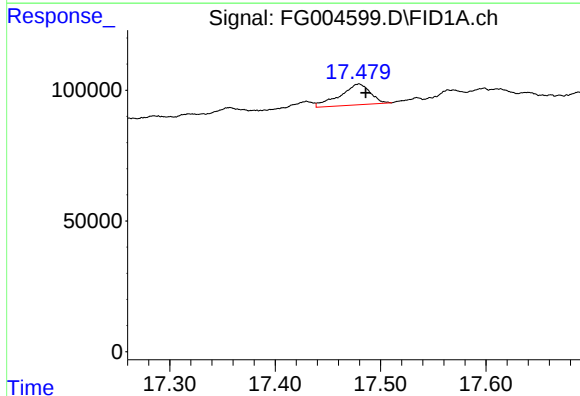


#13 N-TRIACONTANE

R.T.: 17.479 min
Delta R.T.: -0.007 min
Response: 158957
Conc: 1.34 ug/ml

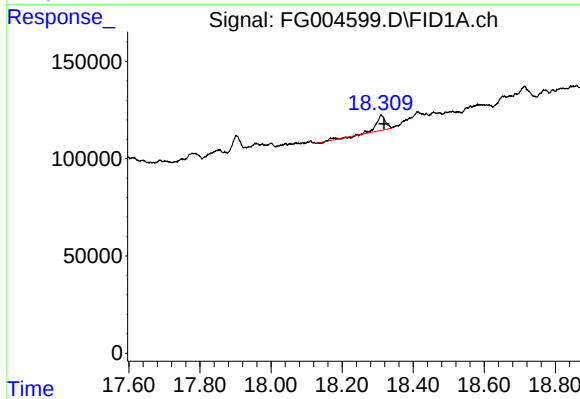

#14 N-DOTRIACONTANE


R.T.: 18.310 min
Delta R.T.: -0.009 min
Response: 144851
Conc: 1.24 ug/ml

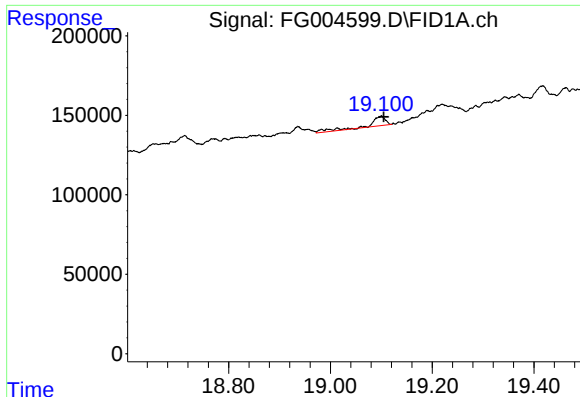

#15 N-TETRATRIACONTANE


R.T.: 19.100 min
Delta R.T.: -0.005 min
Response: 127449
Conc: 1.14 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-03-(0-6)

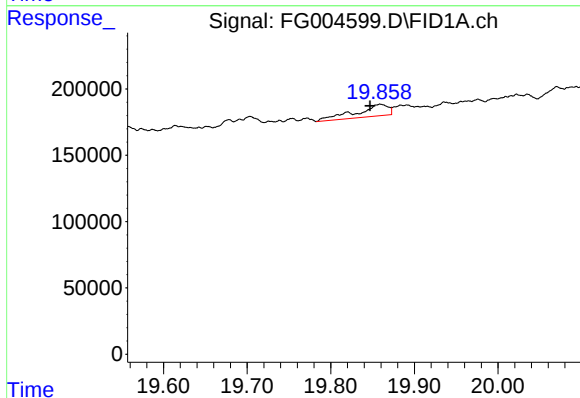

#16 N-HEXATRIACONTANE

R.T.: 19.859 min
Delta R.T.: 0.012 min
Response: 235728
Conc: 2.11 ug/ml

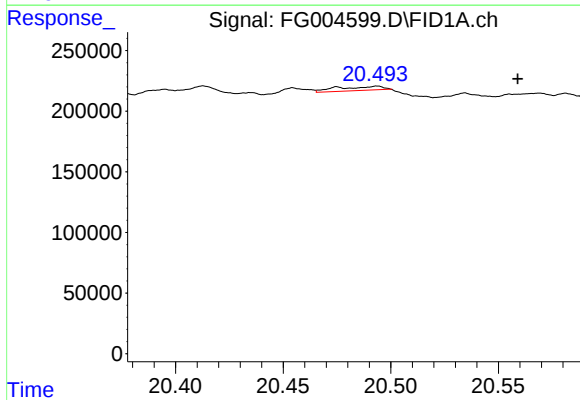

#17 N-OCTATRIACONTANE

R.T.: 20.493 min
Delta R.T.: -0.066 min
Response: 104118
Conc: 1.05 ug/ml