

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
Data File : FG004602.D
Signal(s) : FID1A.ch
Acq On : 04 Apr 2019 20:51
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Apr 05 01:44:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.414	1949047	18.896 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.477	399385	3.367 ug/ml
14) N-DOTRIACONTANE	18.311	206463	1.761 ug/ml
15) N-TETRATRIACONTANE	19.095	340445	3.056 ug/ml
16) N-HEXATRIACONTANE	19.851	109449	0.982 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
Data File : FG004602.D
Signal(s) : FID1A.ch
Acq On : 04 Apr 2019 20:51
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Apr 05 01:44:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

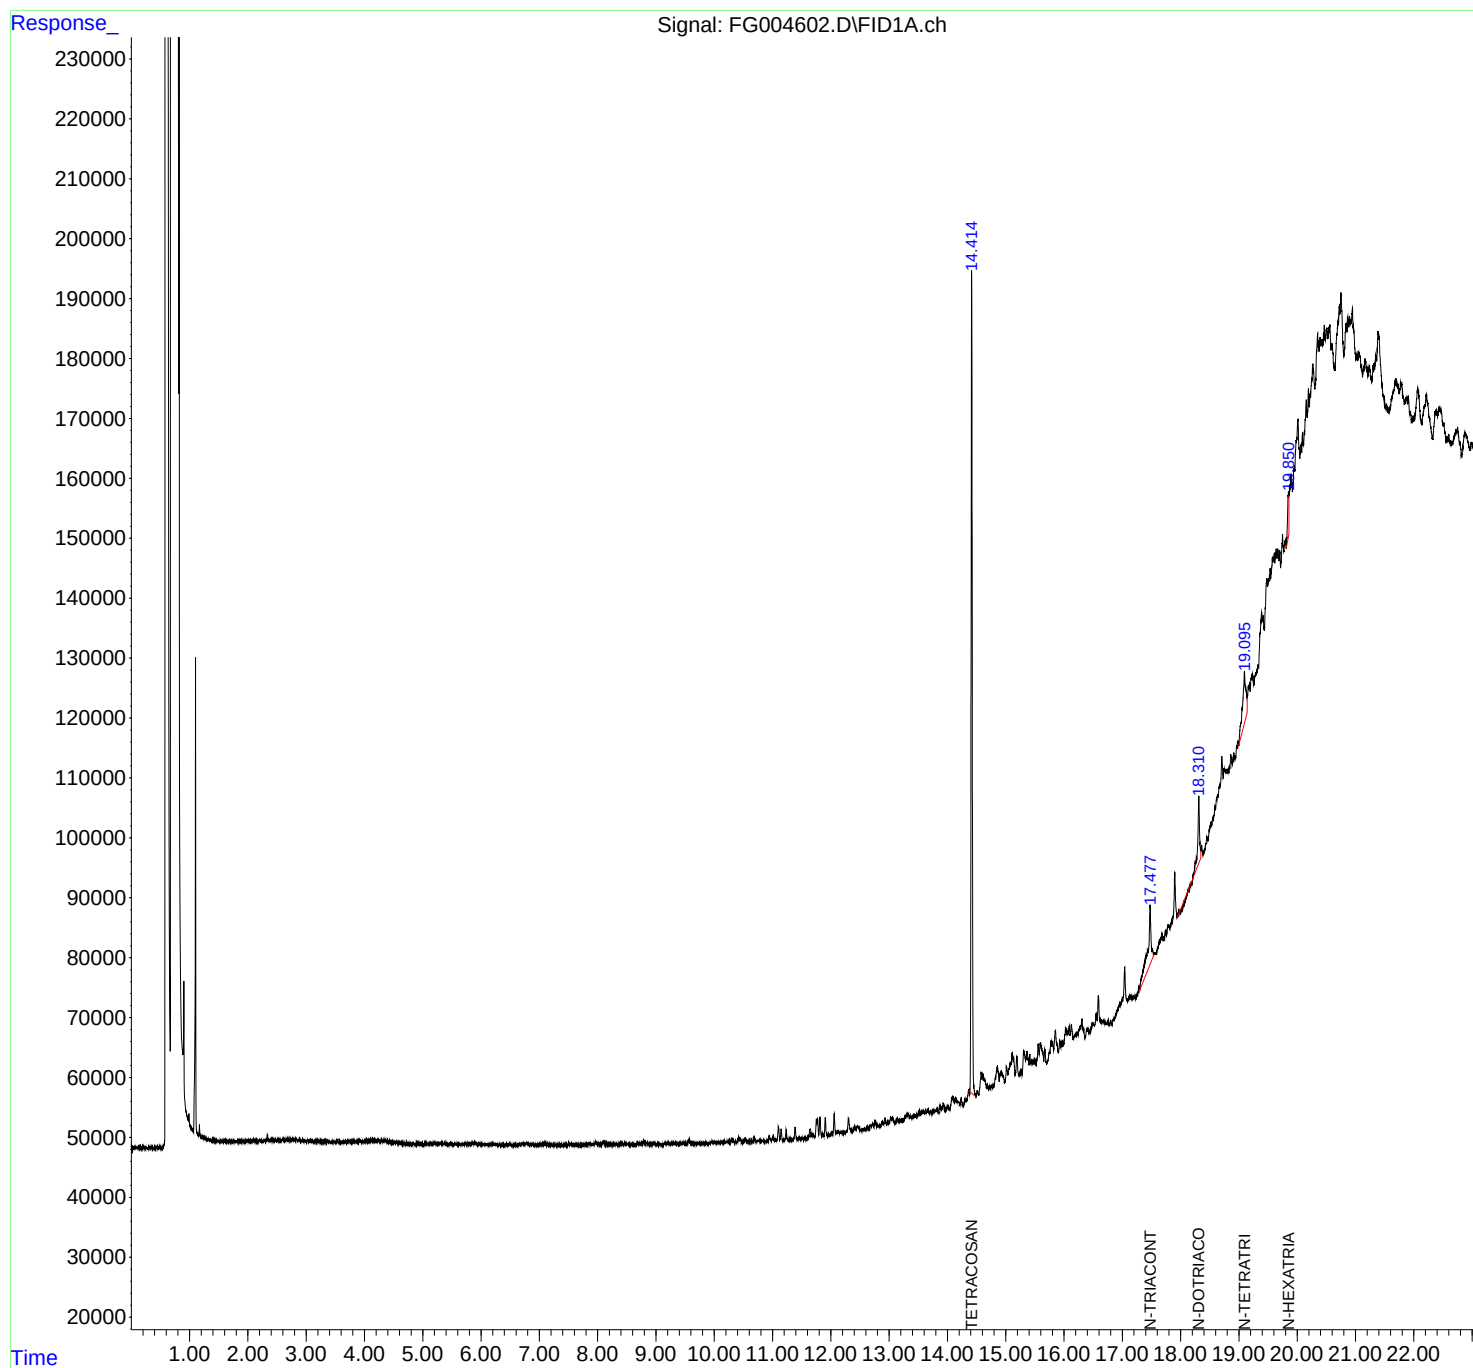


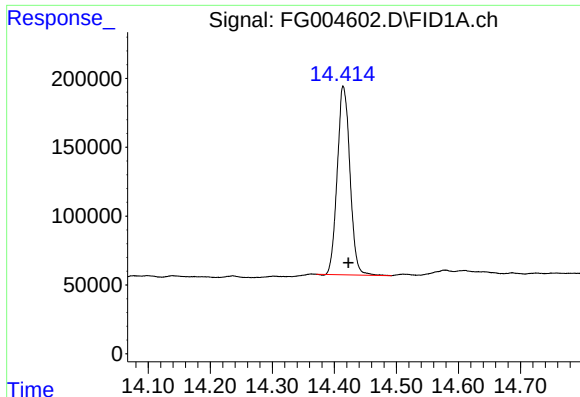

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.414 min
Delta R.T.: -0.008 min
Response: 1949047
Conc: 18.90 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

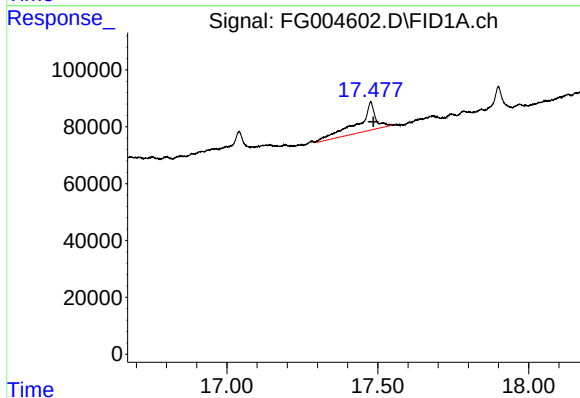


#13 N-TRIACONTANE

R.T.: 17.477 min
Delta R.T.: -0.009 min
Response: 399385
Conc: 3.37 ug/ml

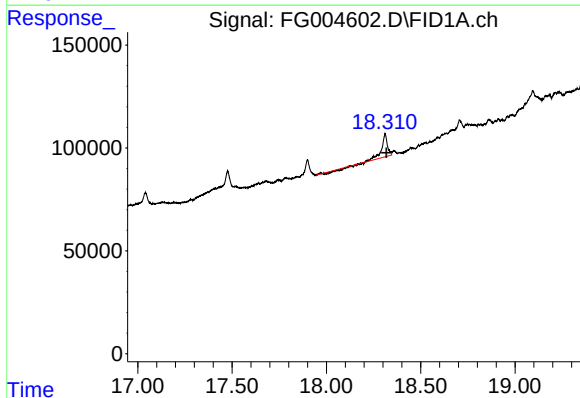


#14 N-DOTRIACONTANE

R.T.: 18.311 min
Delta R.T.: -0.007 min
Response: 206463
Conc: 1.76 ug/ml

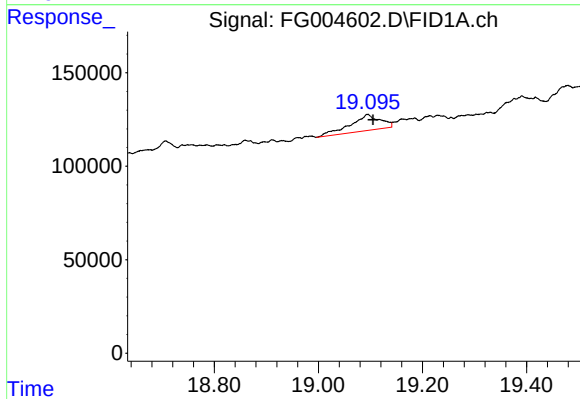

#15 N-TETRATRIACONTANE

R.T.: 19.095 min
Delta R.T.: -0.010 min
Response: 340445
Conc: 3.06 ug/ml

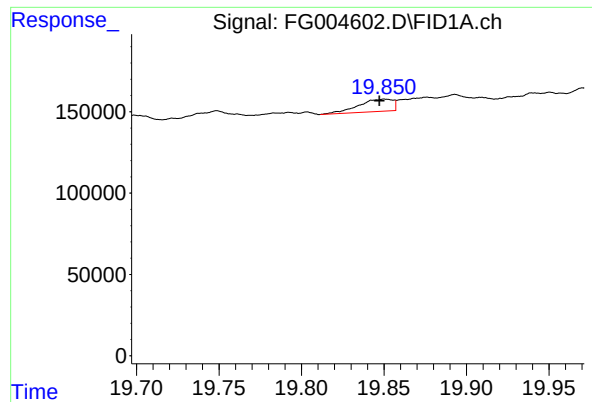

#16 N-HEXATRIACONTANE

R.T.: 19.851 min
Delta R.T.: 0.004 min
Response: 109449
Conc: 0.98 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK