

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
 Data File : FG004581.D
 Signal(s) : FID1A.ch
 Acq On : 04 Apr 2019 09:46
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Apr 04 11:15:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.416	4928000	47.776 ug/ml
Target Compounds			
2) N-DECANE	4.148	6393032	60.566 ug/ml
3) N-DODECANE	6.171	6423449	60.968 ug/ml
4) N-TETRADECANE	7.965	6389366	58.971 ug/ml
5) N-HEXADECANE	9.565	6266219	56.008 ug/ml
6) N-OCTADECANE	11.007	6102561	53.803 ug/ml
7) N-EICOSANE	12.316	5899111	51.603 ug/ml
8) N-DOCOSANE	13.516	5734116	50.162 ug/ml
10) N-TETRACOSANE	14.620	5672525	49.106 ug/ml
11) N-HEXACOSANE	15.642	5599005	48.842 ug/ml
12) N-OCTACOSANE	16.592	5670584	49.016 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
Data File : FG004581.D
Signal(s) : FID1A.ch
Acq On : 04 Apr 2019 09:46
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Apr 04 11:15:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

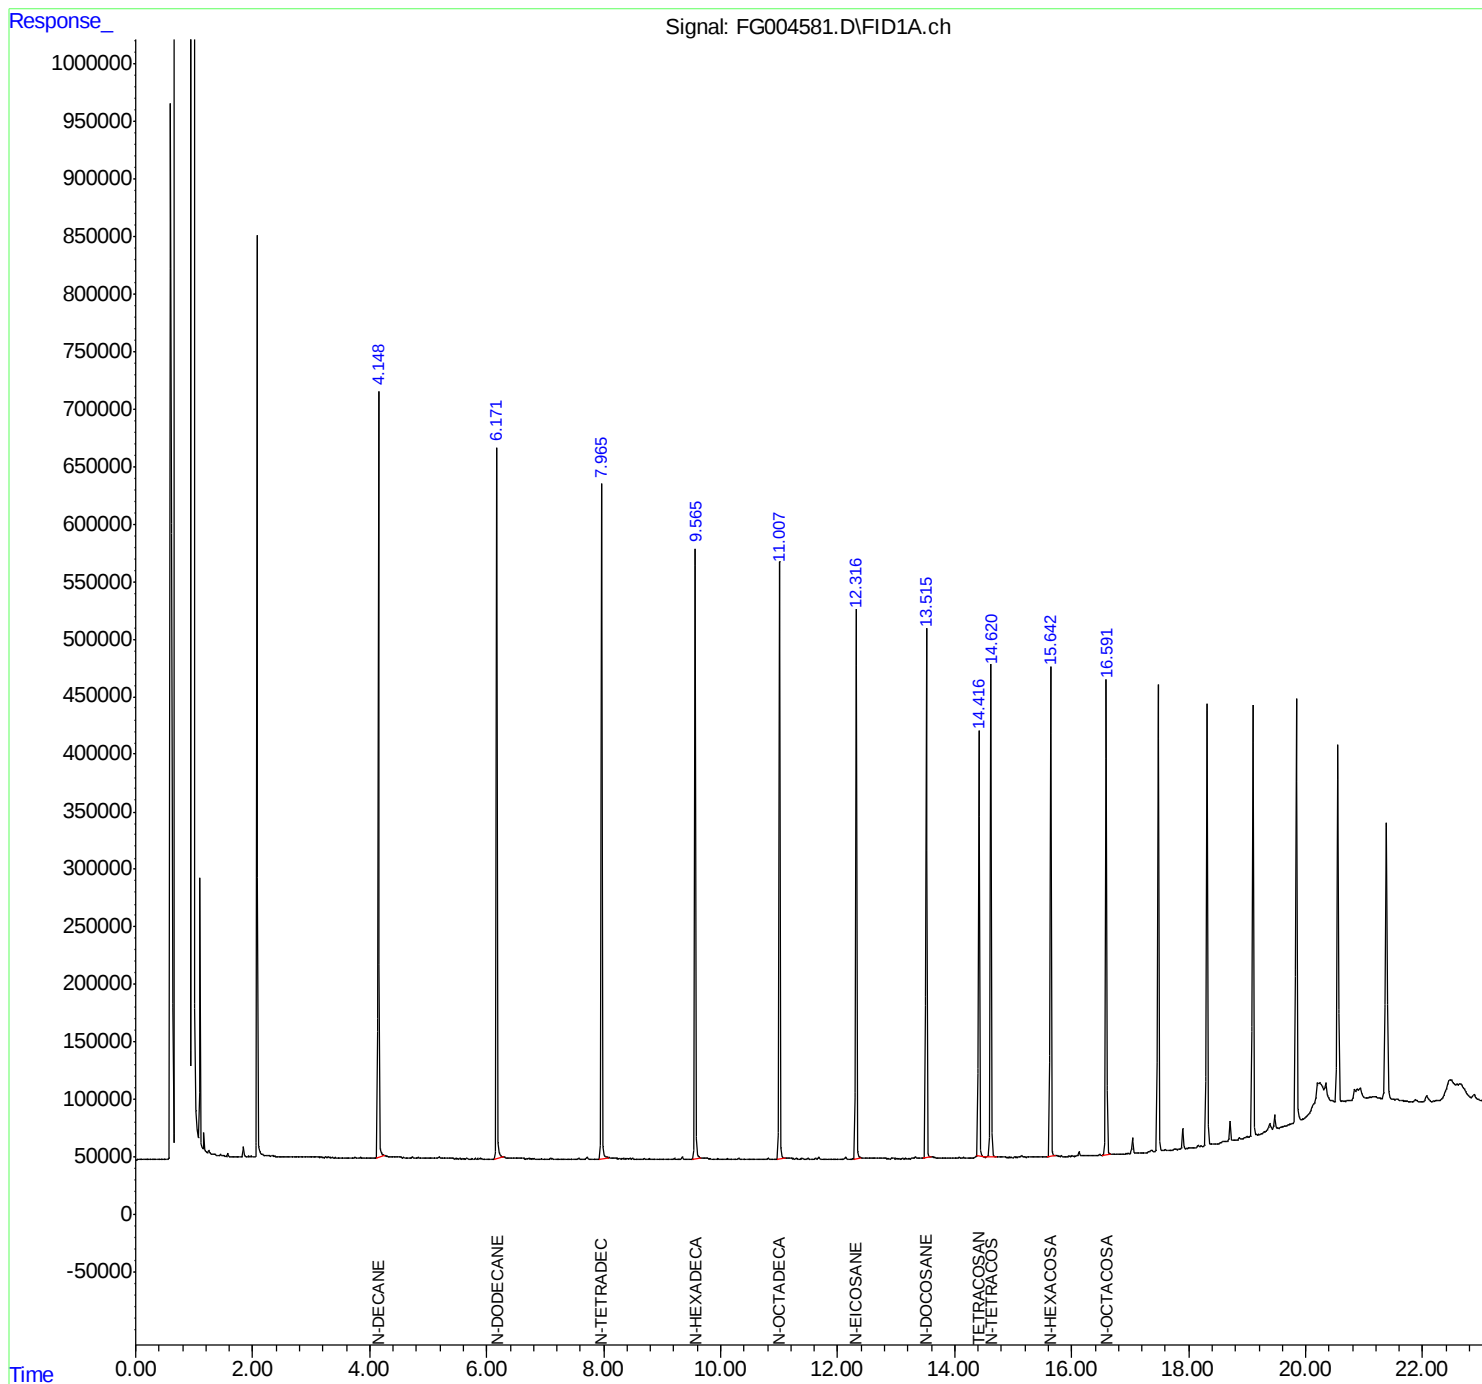


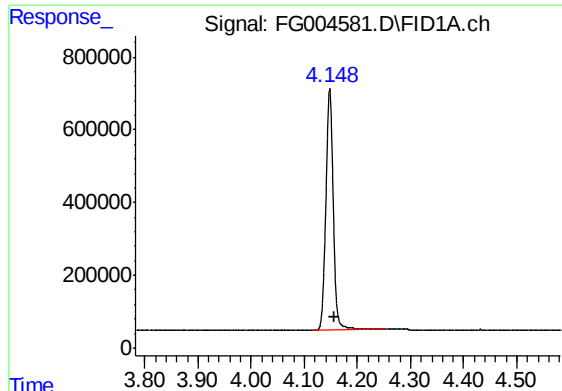

#2 N-DECANE


R.T.: 4.148 min
Delta R.T.: -0.009 min
Response: 6393032
Conc: 60.57 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

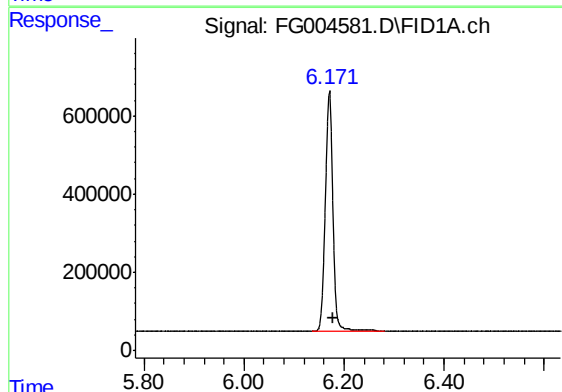


#3 N-DODECANE

R.T.: 6.171 min
Delta R.T.: -0.007 min
Response: 6423449
Conc: 60.97 ug/ml

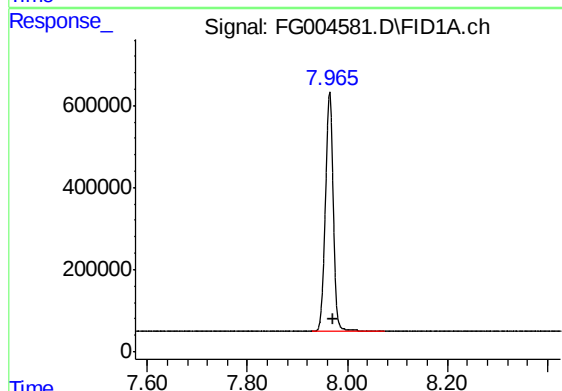


#4 N-TETRADECANE

R.T.: 7.965 min
Delta R.T.: -0.007 min
Response: 6389366
Conc: 58.97 ug/ml

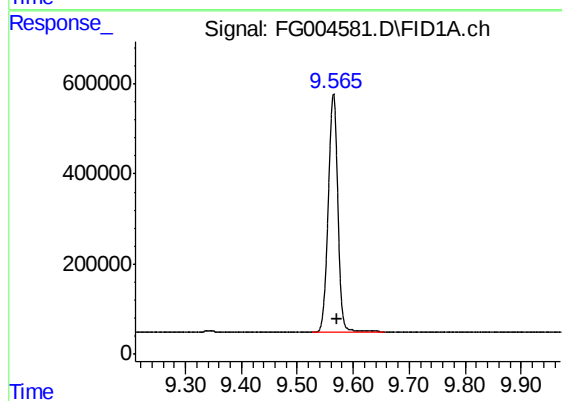

#5 N-HEXADECANE


R.T.: 9.565 min
Delta R.T.: -0.007 min
Response: 6266219
Conc: 56.01 ug/ml

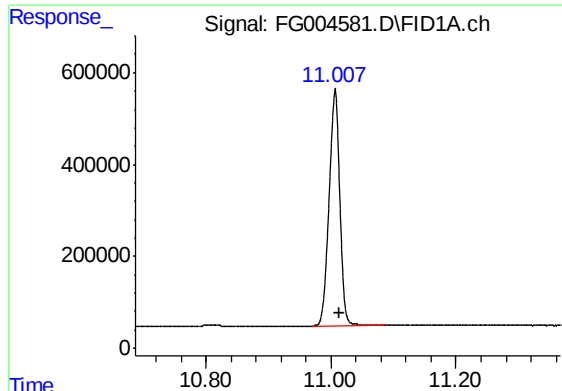

#6 N-OCTADECANE


R.T.: 11.007 min
Delta R.T.: -0.006 min
Response: 6102561
Conc: 53.80 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

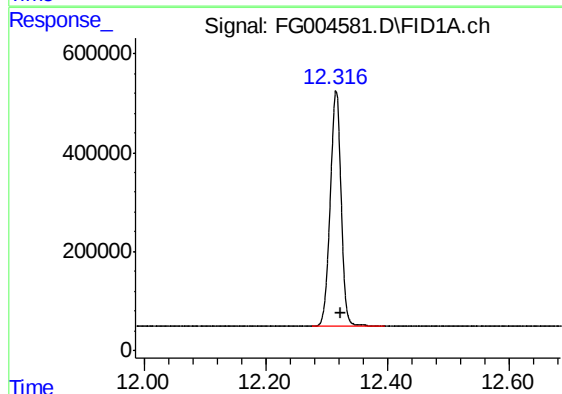


#7 N-EICOSANE

R.T.: 12.316 min
Delta R.T.: -0.007 min
Response: 5899111
Conc: 51.60 ug/ml

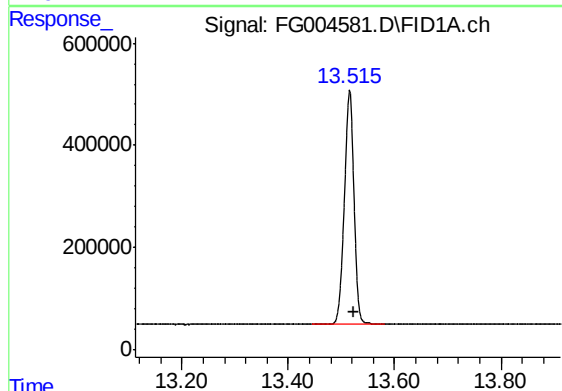


#8 N-DOCOSANE

R.T.: 13.516 min
Delta R.T.: -0.007 min
Response: 5734116
Conc: 50.16 ug/ml

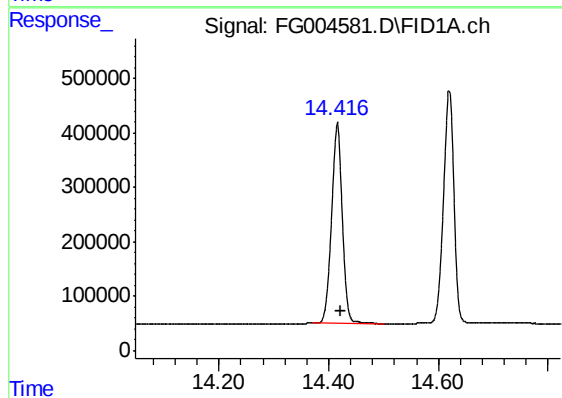

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.416 min
Delta R.T.: -0.007 min
Response: 4928000
Conc: 47.78 ug/ml

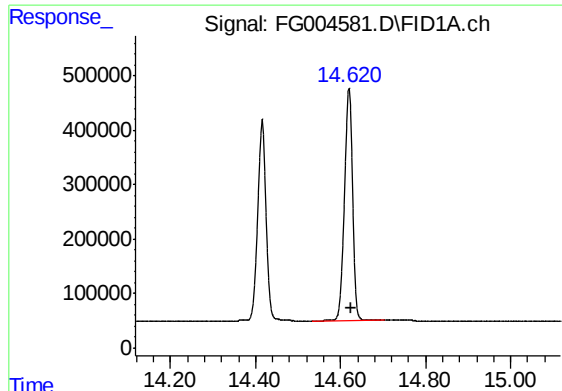

#10 N-TETRACOSANE


R.T.: 14.620 min
Delta R.T.: -0.005 min
Response: 5672525
Conc: 49.11 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

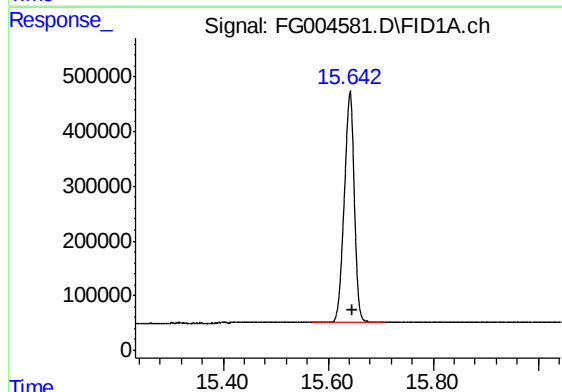

#11 N-HEXACOSANE

R.T.: 15.642 min
Delta R.T.: -0.005 min
Response: 5599005
Conc: 48.84 ug/ml

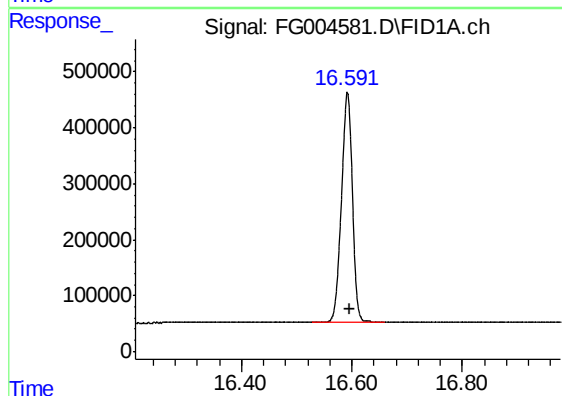

#12 N-OCTACOSANE

R.T.: 16.592 min
Delta R.T.: -0.005 min
Response: 5670584
Conc: 49.02 ug/ml