

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG040521\  
 Data File : FG007770.D  
 Signal(s) : FID1A.ch  
 Acq On : 05 Apr 2021 21:29  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Apr 06 03:07:42 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG040521.M  
 Quant Title :  
 QLast Update : Tue Apr 06 03:05:53 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units   |
|-------------------------------|---------|----------|--------------|
| -----                         |         |          |              |
| System Monitoring Compounds   |         |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.774  | 2809149  | 18.811 ug/ml |
| Target Compounds              |         |          |              |
| 14) N-DOTRIACONTANE           | 18.699  | 171933   | 1.126 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.251f | 487554   | 4.189 ug/ml  |
| -----                         |         |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG040521\  
Data File : FG007770.D  
Signal(s) : FID1A.ch  
Acq On : 05 Apr 2021 21:29  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Apr 06 03:07:42 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG040521.M  
Quant Title :  
QLast Update : Tue Apr 06 03:05:53 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

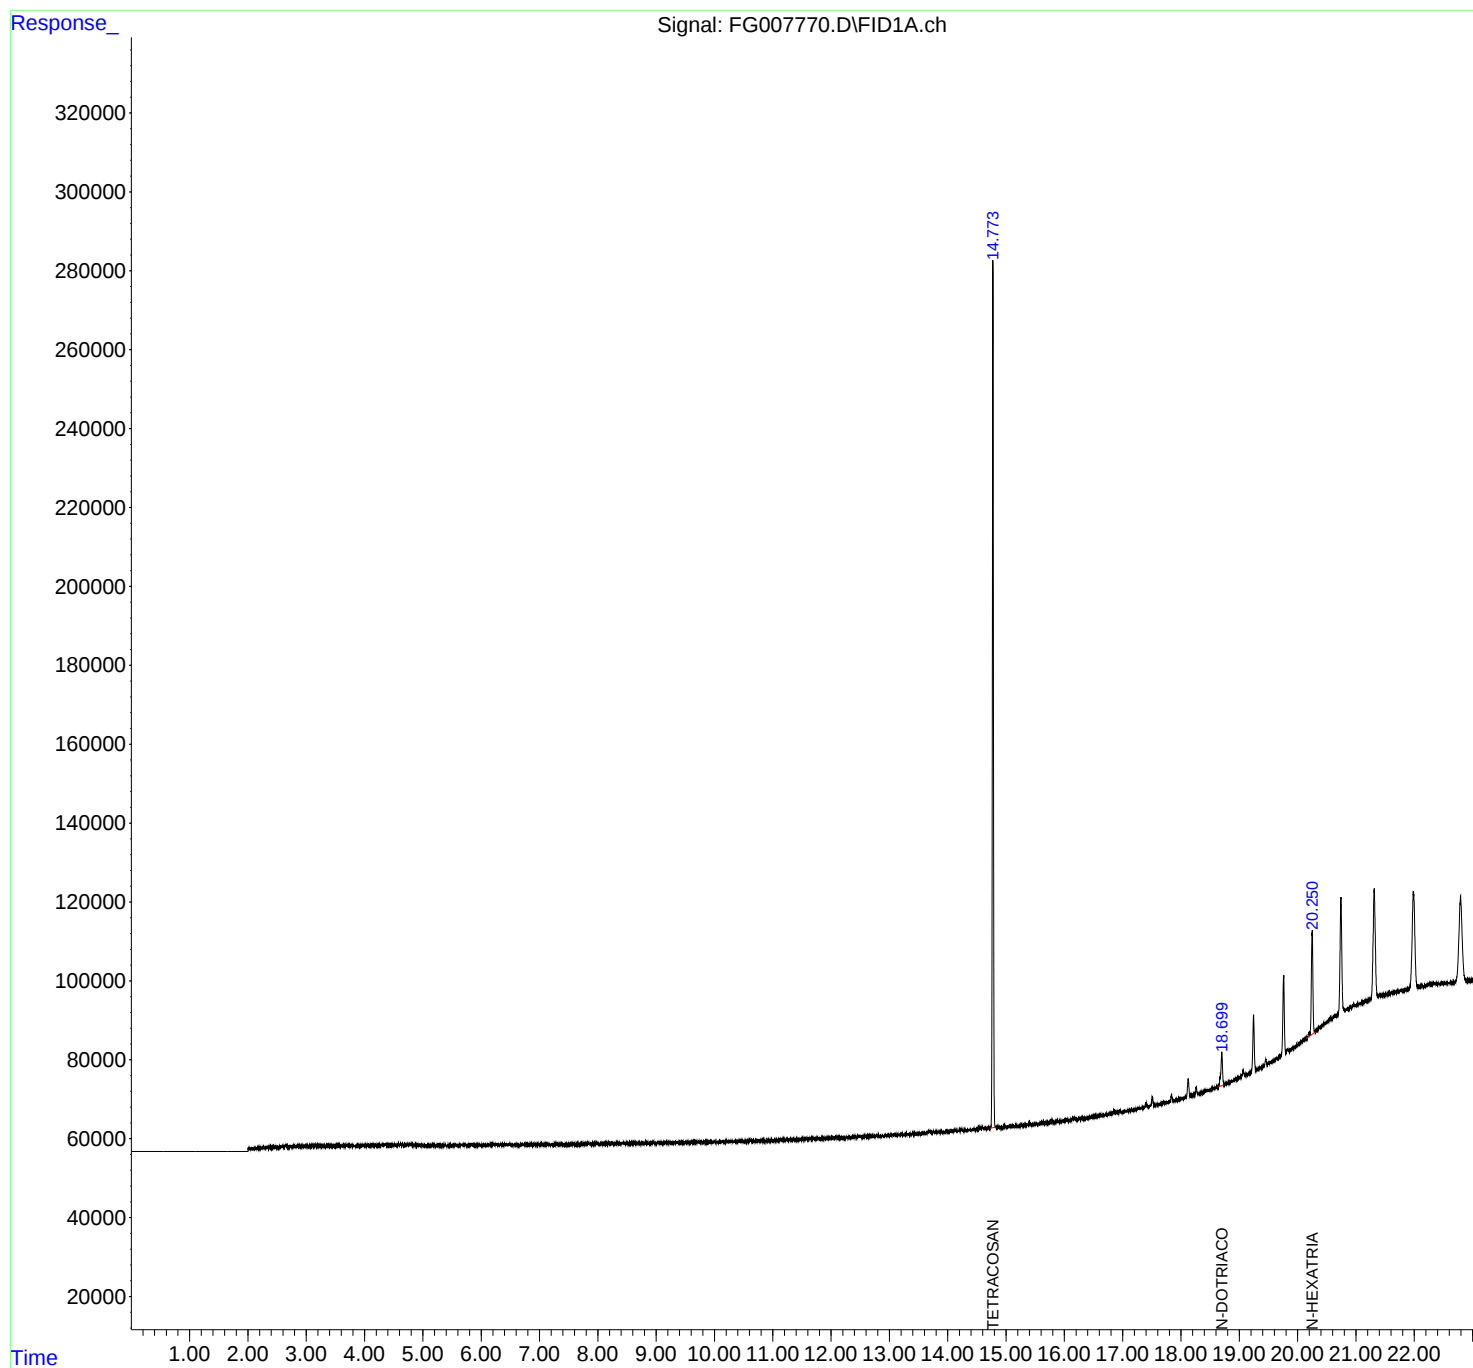


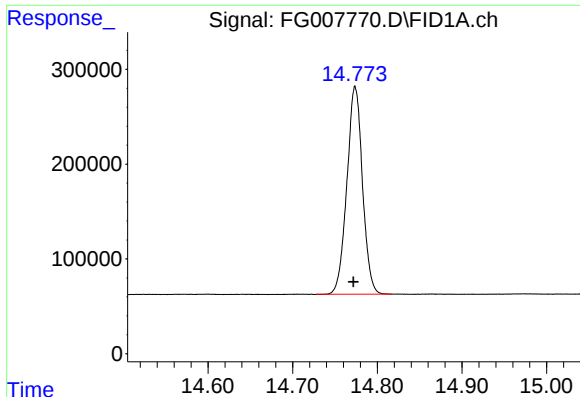

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.774 min  
Delta R.T.: 0.002 min  
Response: 2809149  
Conc: 18.81 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

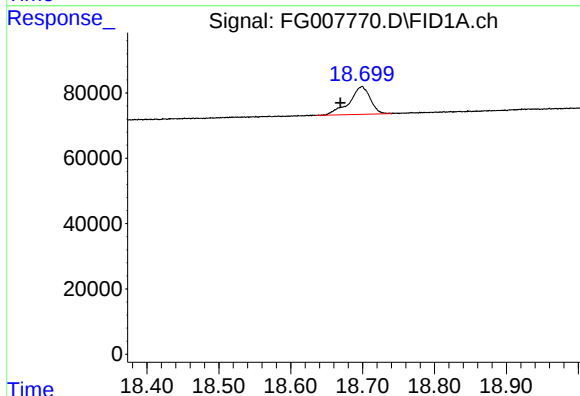

#14 N-DOTRIACONTANE

R.T.: 18.699 min  
Delta R.T.: 0.030 min  
Response: 171933  
Conc: 1.13 ug/ml

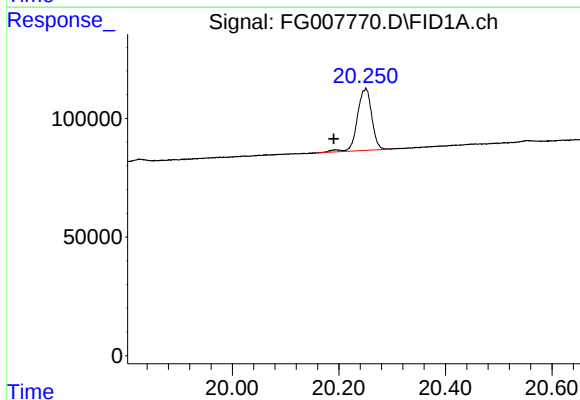

#16 N-HEXATRIACONTANE

R.T.: 20.251 min  
Delta R.T.: 0.060 min  
Response: 487554  
Conc: 4.19 ug/ml