

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040622\
Data File : FG009525.D
Signal(s) : FID1A.ch
Acq On : 06 Apr 2022 14:48
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 07 01:03:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 01 13:54:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.353	3377393	22.410 ug/ml
12) N-OCTACOSANE	16.812	2957917	22.664 ug/ml
13) N-TRIACONTANE	17.702	63567	0.515 ug/ml
14) N-DOTRIACONTANE	18.539	74837	0.645 ug/ml
15) N-TETRATRIACONTANE	19.326	61726	0.581 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040622\
Data File : FG009525.D
Signal(s) : FID1A.ch
Acq On : 06 Apr 2022 14:48
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 07 01:03:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 01 13:54:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

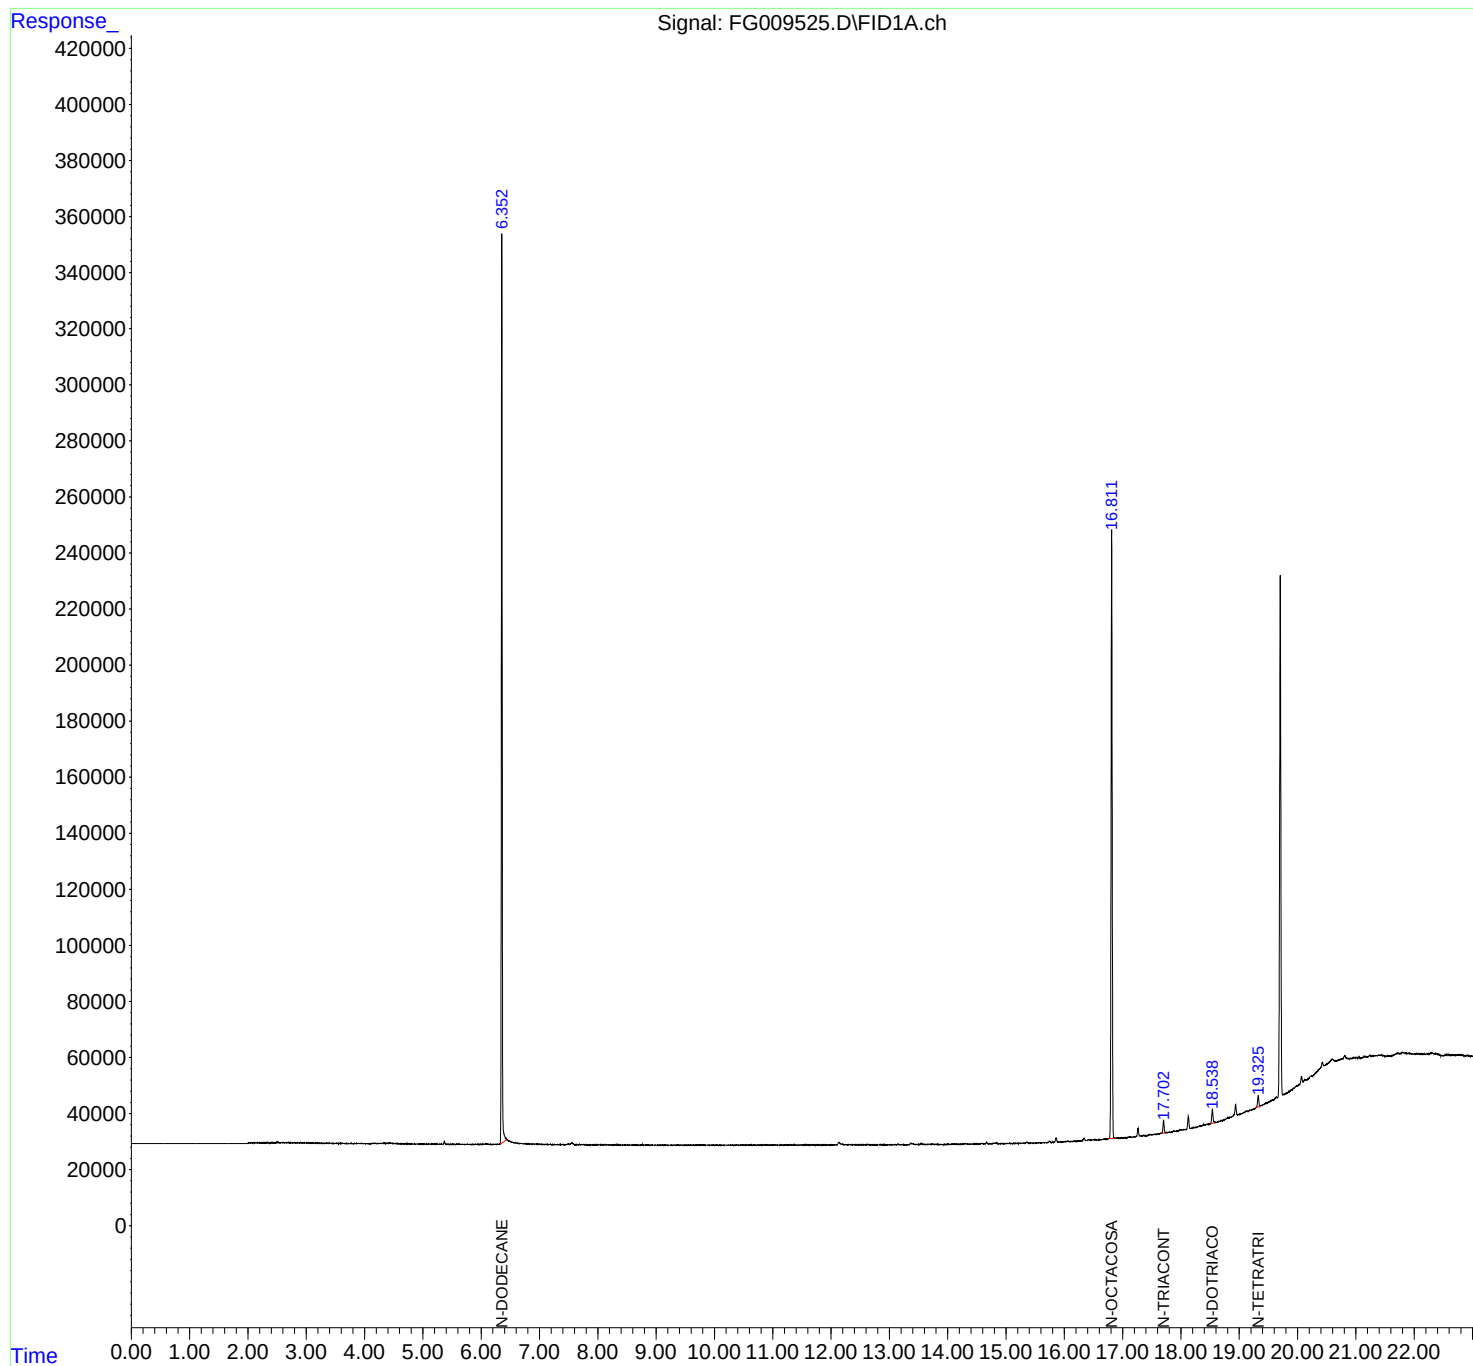


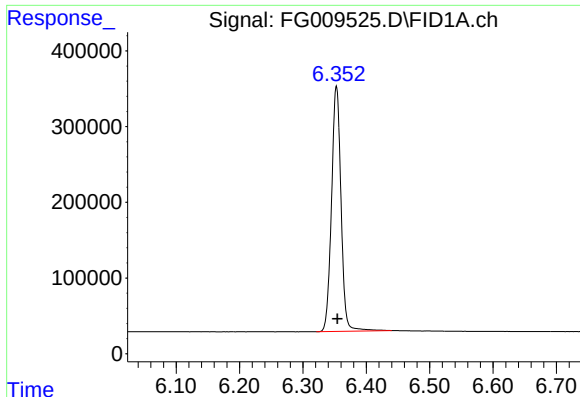

#3 N-DODECANE


R.T.: 6.353 min
Delta R.T.: -0.002 min
Response: 3377393
Conc: 22.41 ug/ml

Instrument :
FID_G
ClientSampleId :

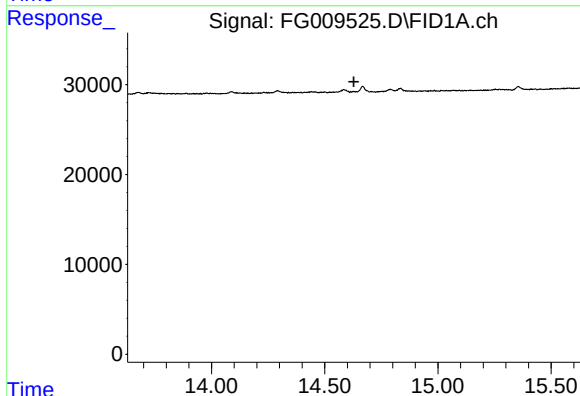


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.629 min
Response: 0
Conc: N.D.

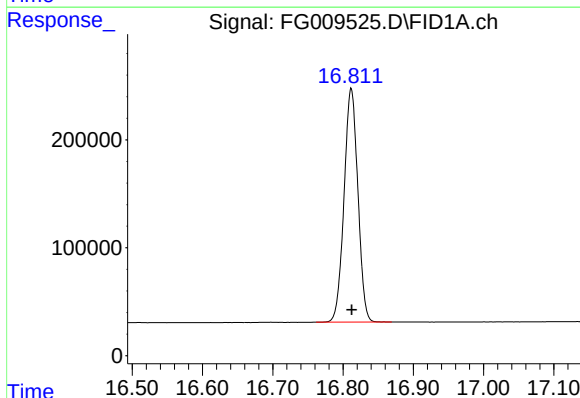


#12 N-OCTACOSANE

R.T.: 16.812 min
Delta R.T.: 0.000 min
Response: 2957917
Conc: 22.66 ug/ml

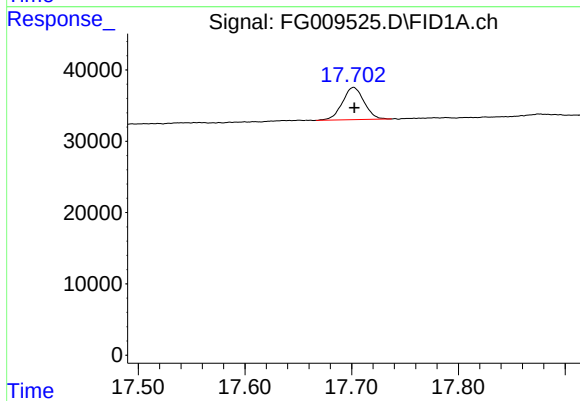

#13 N-TRIACONTANE


R.T.: 17.702 min
Delta R.T.: 0.000 min
Response: 63567
Conc: 0.51 ug/ml

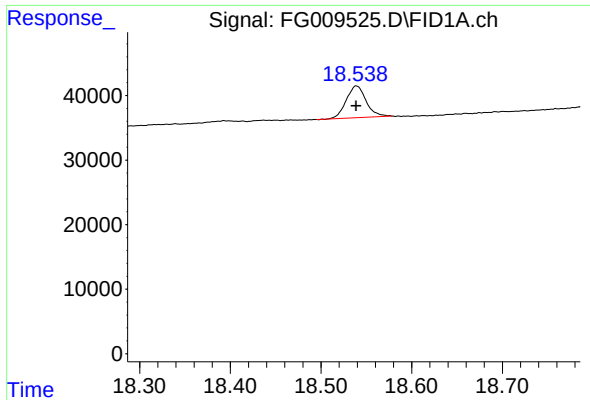

#14 N-DOTRIACONTANE

R.T.: 18.539 min
Delta R.T.: 0.000 min
Response: 74837
Conc: 0.64 ug/ml

Instrument :
FID_G
ClientSampleId :

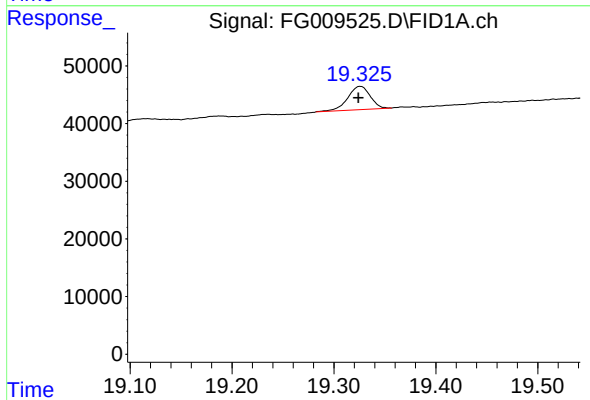

#15 N-TETRATRIACONTANE

R.T.: 19.326 min
Delta R.T.: 0.002 min
Response: 61726
Conc: 0.58 ug/ml