

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040623\
 Data File : FG011713.D
 Signal(s) : FID1A.ch
 Acq On : 06 Apr 2023 09:19
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 07 06:05:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
 Quant Title :
 QLast Update : Wed Mar 15 18:43:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.749	1998133	16.375 ug/ml
12) N-OCTACOSANE	17.245	1877544	18.107 ug/ml
13) N-TRIACONTANE	18.133	376072	3.795 ug/ml
14) N-DOTRIACONTANE	18.970	537759	5.798 ug/ml
15) N-TETRATRIACONTANE	19.757	482144	5.719 ug/ml
16) N-HEXATRIACONTANE	20.501	341513	4.436 ug/ml
17) N-OCTATRIACONTANE	21.254	267624	3.555 ug/ml
18) N-TETRACONTANE	22.200	205449	2.799 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040623\
Data File : FG011713.D
Signal(s) : FID1A.ch
Acq On : 06 Apr 2023 09:19
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 07 06:05:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

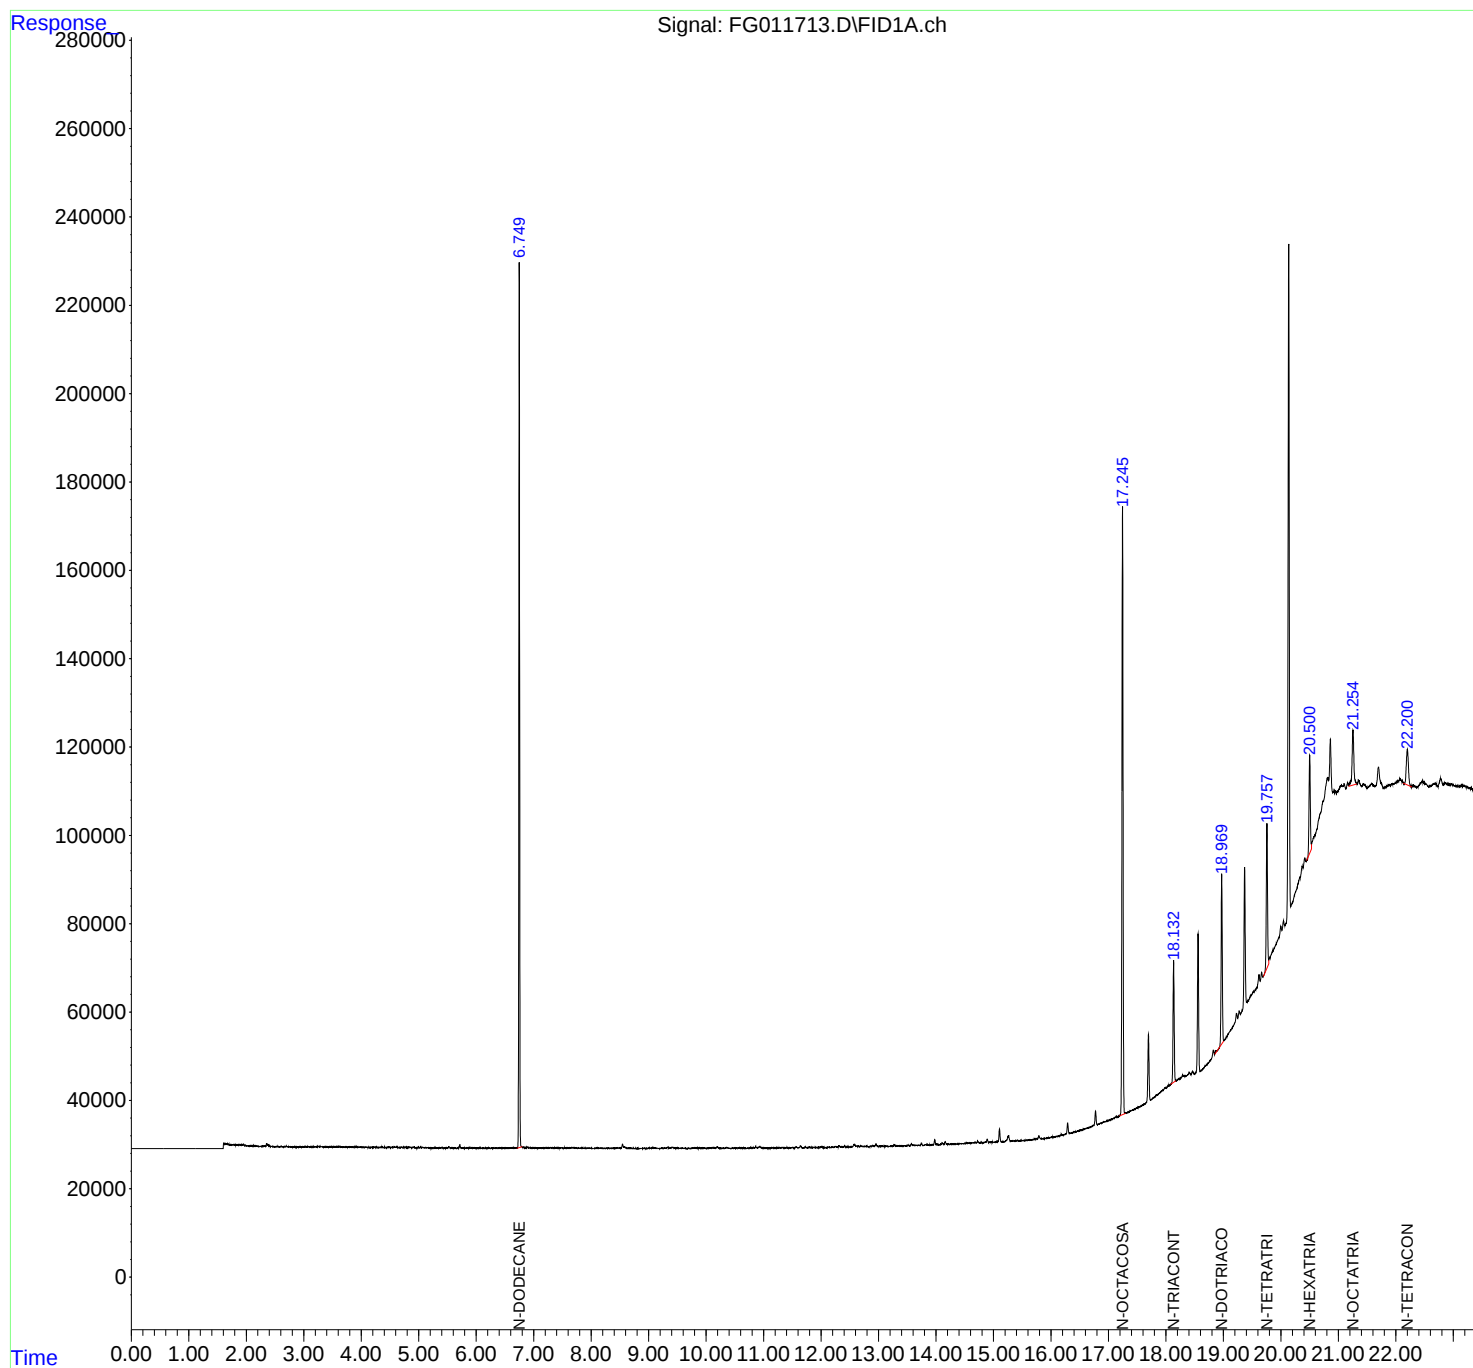


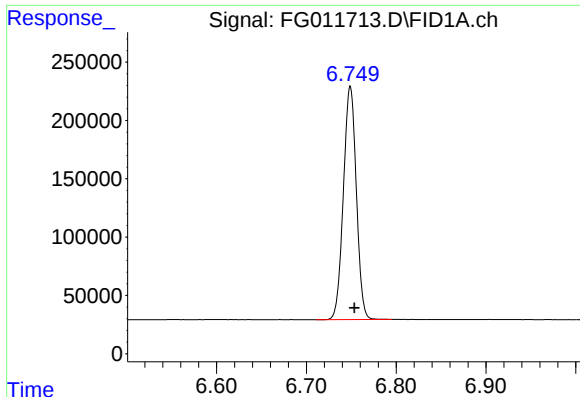

#3 N-DODECANE


R.T.: 6.749 min
Delta R.T.: -0.005 min
Response: 1998133
Conc: 16.37 ug/ml

Instrument :
FID_G
ClientSampleId :

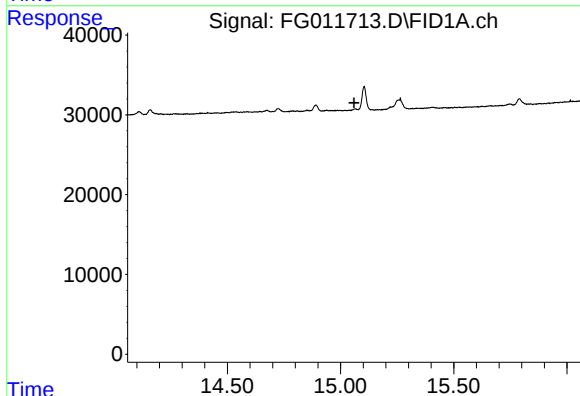


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.059 min
Response: 0
Conc: N.D.

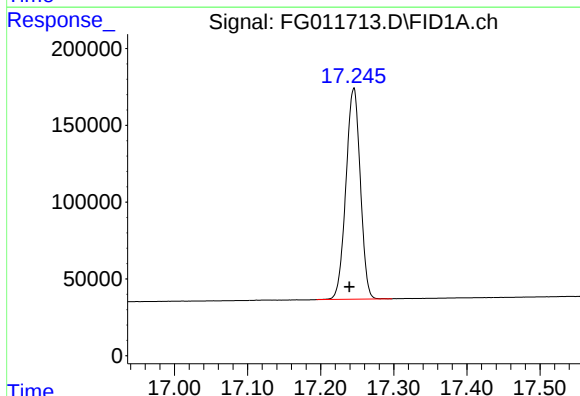


#12 N-OCTACOSANE

R.T.: 17.245 min
Delta R.T.: 0.006 min
Response: 1877544
Conc: 18.11 ug/ml

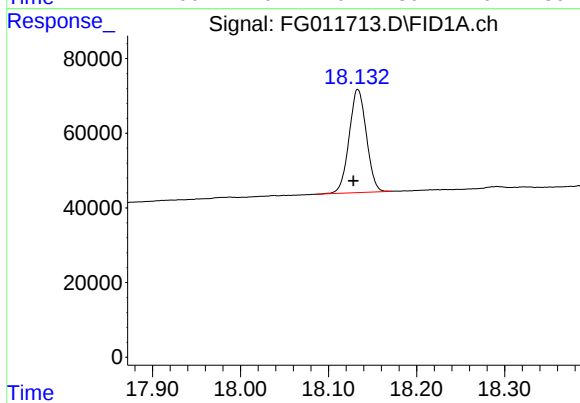

#13 N-TRIACONTANE


R.T.: 18.133 min
Delta R.T.: 0.005 min
Response: 376072
Conc: 3.79 ug/ml

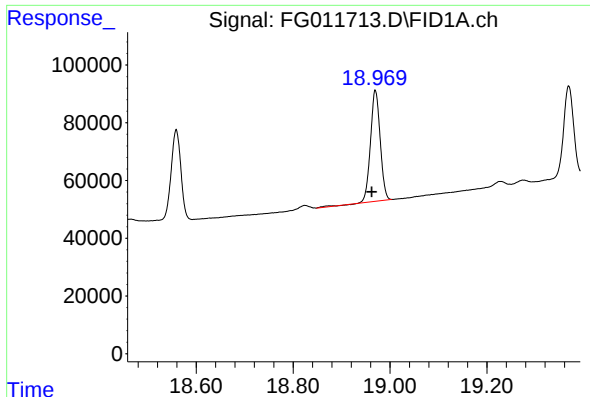

#14 N-DOTRIACONTANE


R.T.: 18.970 min
Delta R.T.: 0.007 min
Response: 537759
Conc: 5.80 ug/ml

Instrument :
FID_G
ClientSampleId :

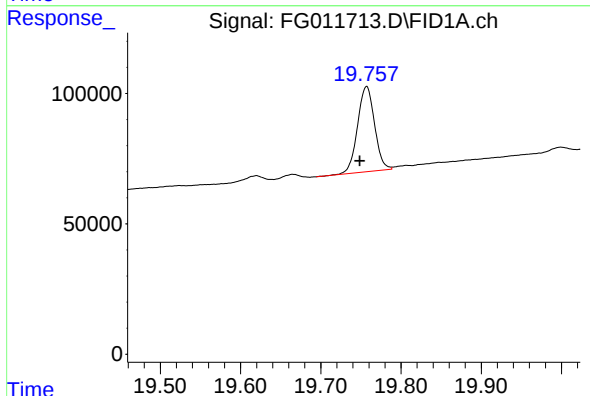


#15 N-TETRATRIACONTANE

R.T.: 19.757 min
Delta R.T.: 0.009 min
Response: 482144
Conc: 5.72 ug/ml

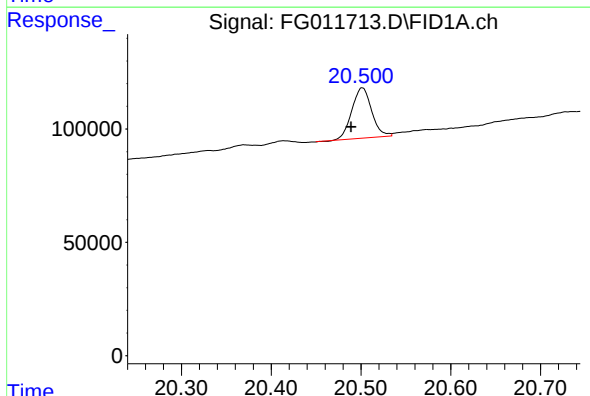


#16 N-HEXATRIACONTANE

R.T.: 20.501 min
Delta R.T.: 0.012 min
Response: 341513
Conc: 4.44 ug/ml

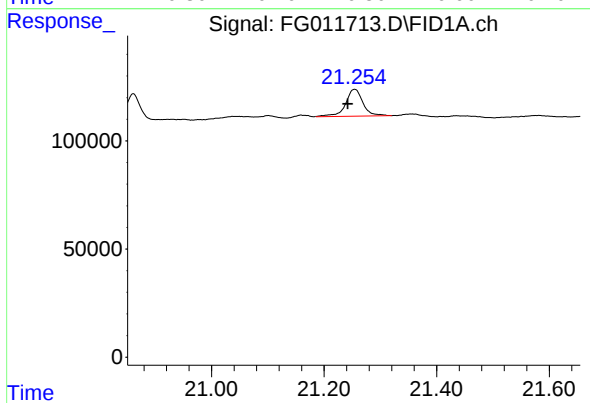

#17 N-OCTATRIACONTANE

R.T.: 21.254 min
Delta R.T.: 0.012 min
Response: 267624
Conc: 3.55 ug/ml

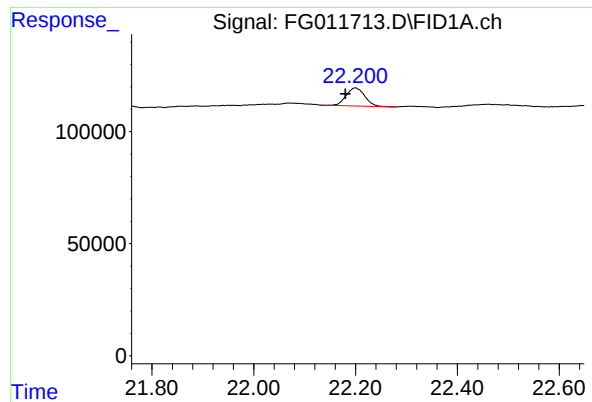

#18 N-TETRACONTANE

R.T.: 22.200 min
Delta R.T.: 0.019 min
Response: 205449
Conc: 2.80 ug/ml

Instrument :

FID_G

ClientSampleId :