

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040623\
Data File : FG011717.D
Signal(s) : FID1A.ch
Acq On : 06 Apr 2023 14:00
Operator : YP\AJ
Sample : PB151916BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB151916BL

Integration File: autoint1.e
Quant Time: Apr 07 06:05:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.060	1907844	18.955 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040623\
Data File : FG011717.D
Signal(s) : FID1A.ch
Acq On : 06 Apr 2023 14:00
Operator : YP\AJ
Sample : PB151916BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB151916BL

Integration File: autoint1.e
Quant Time: Apr 07 06:05:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

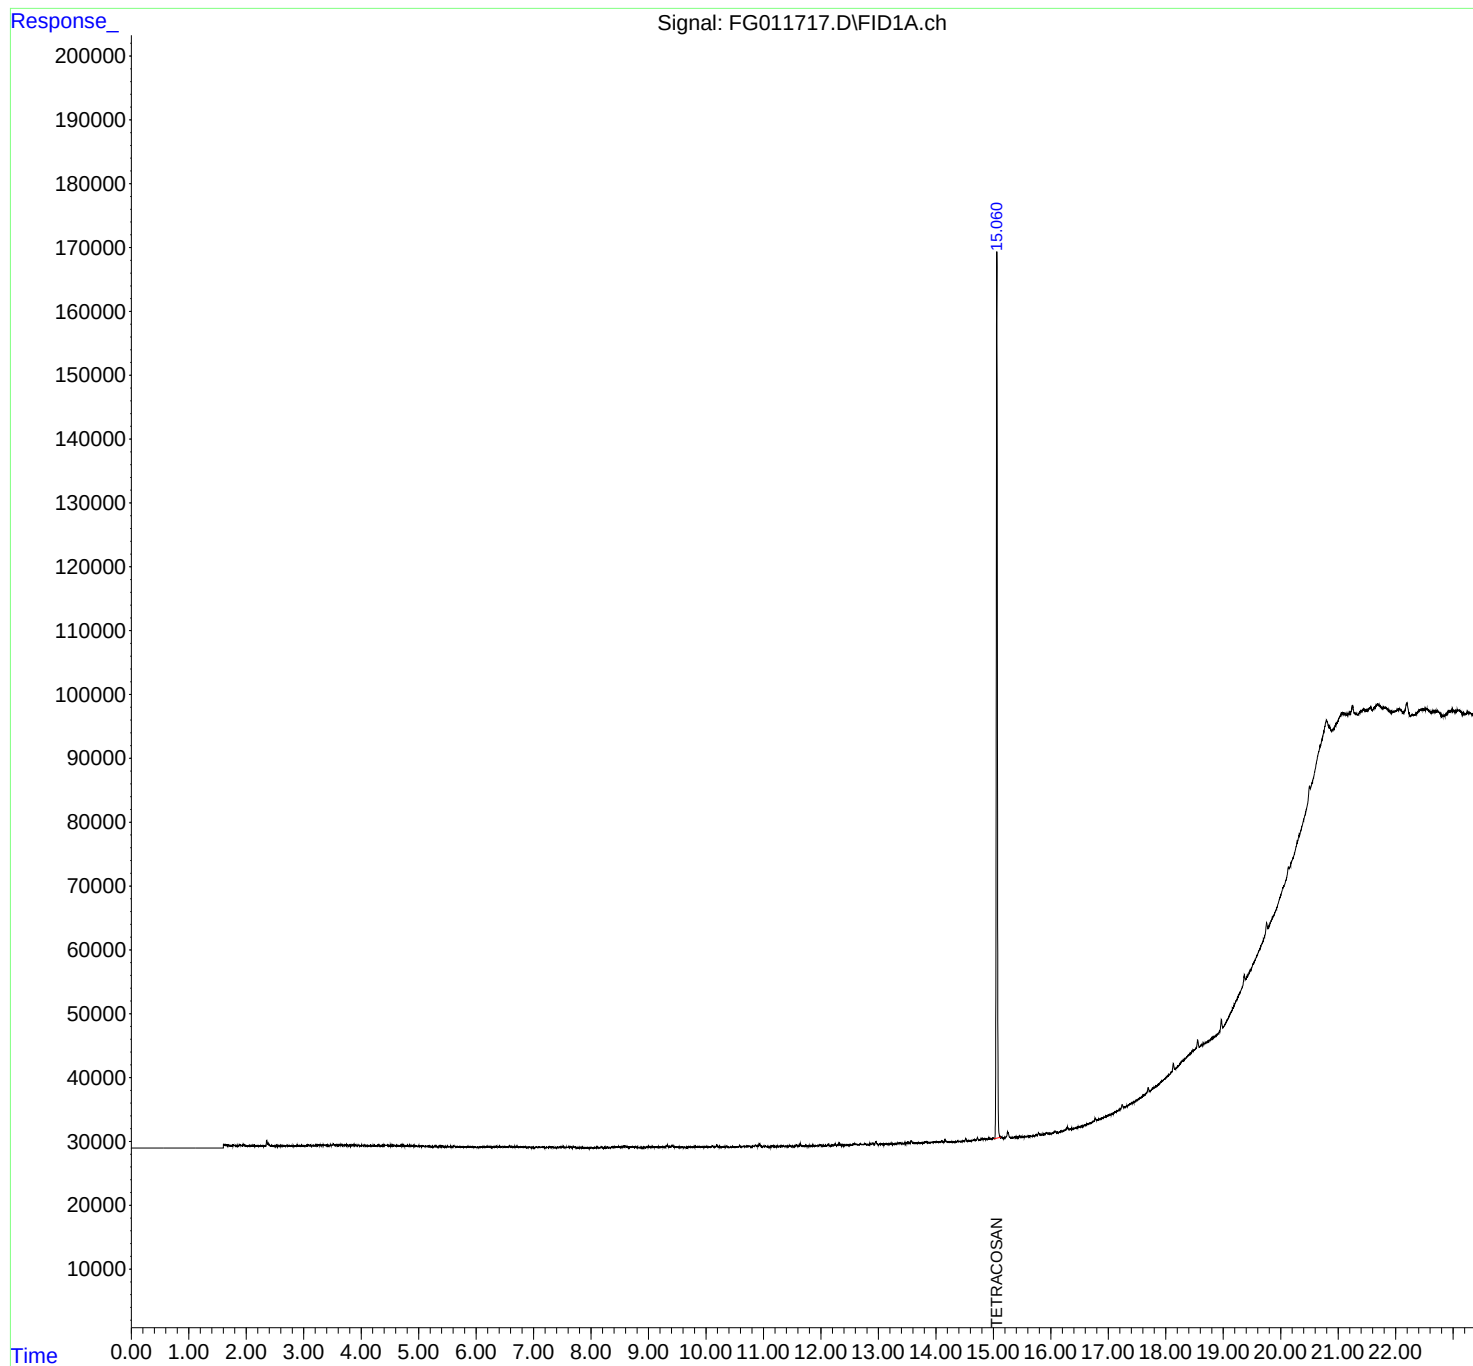

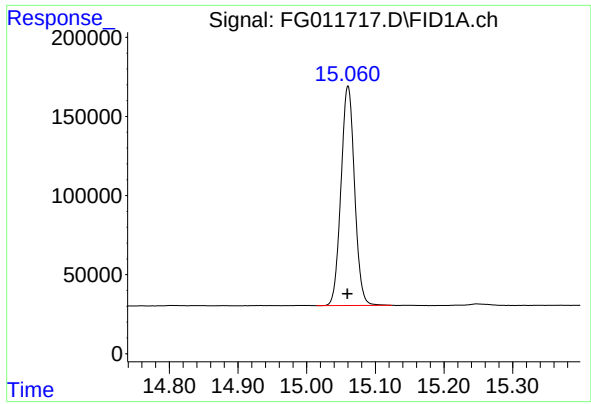

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.060 min
Delta R.T.: 0.001 min
Response: 1907844
Conc: 18.95 ug/ml

Instrument :
FID_G
ClientSampleId :
PB151916BL