

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040722\
 Data File : FG009535.D
 Signal(s) : FID1A.ch
 Acq On : 07 Apr 2022 11:08
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 08 02:28:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
 Quant Title :
 QLast Update : Fri Apr 01 13:54:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.354	3842962	25.499 ug/ml
12) N-OCTACOSANE	16.815	3119718	23.904 ug/ml
13) N-TRIACONTANE	17.705	73477	0.595 ug/ml
14) N-DOTRIACONTANE	18.540	87638	0.755 ug/ml
15) N-TETRATRIACONTANE	19.328	72610	0.683 ug/ml
16) N-HEXATRIACONTANE	20.073	47210	0.499 ug/ml
17) N-OCTATRIACONTANE	20.815	73343	0.852 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040722\
Data File : FG009535.D
Signal(s) : FID1A.ch
Acq On : 07 Apr 2022 11:08
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 02:28:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 01 13:54:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

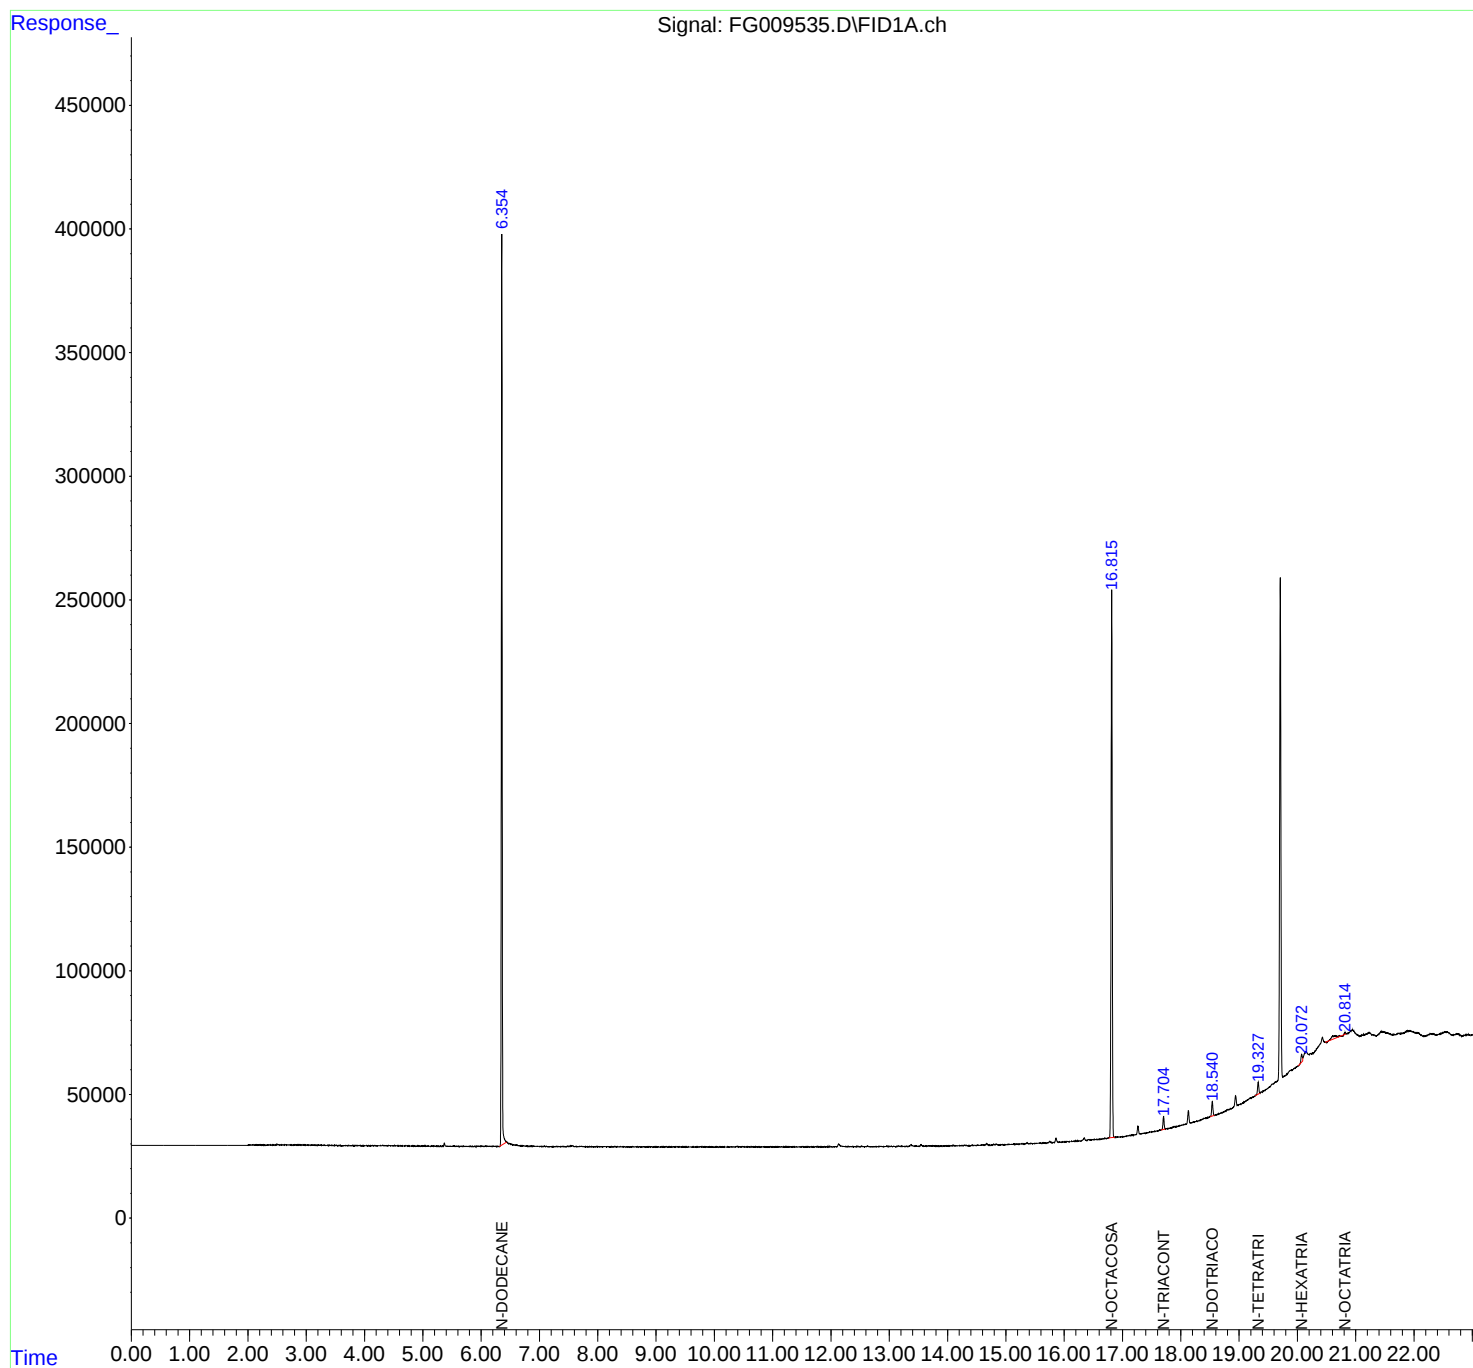


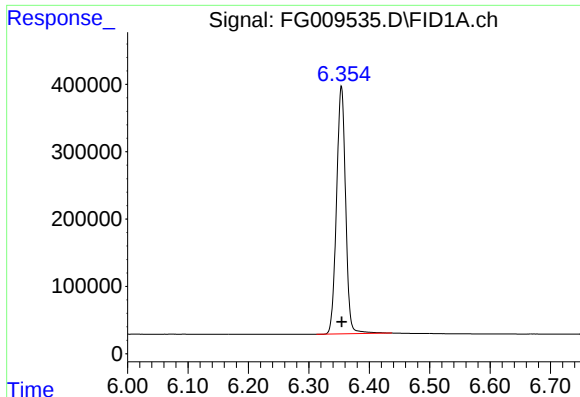

#3 N-DODECANE


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 3842962
Conc: 25.50 ug/ml

Instrument :
FID_G
ClientSampleId :

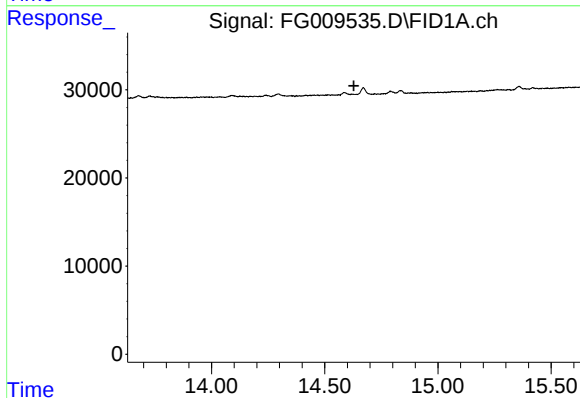


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.629 min
Response: 0
Conc: N.D.

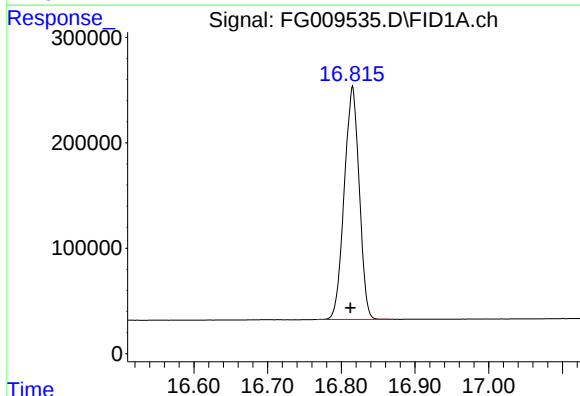


#12 N-OCTACOSANE

R.T.: 16.815 min
Delta R.T.: 0.003 min
Response: 3119718
Conc: 23.90 ug/ml

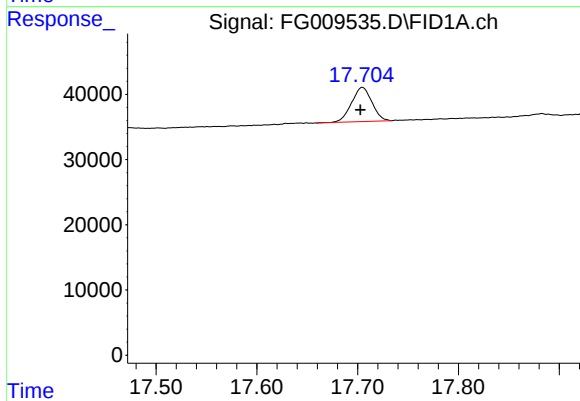

#13 N-TRIACONTANE


R.T.: 17.705 min
Delta R.T.: 0.002 min
Response: 73477
Conc: 0.60 ug/ml

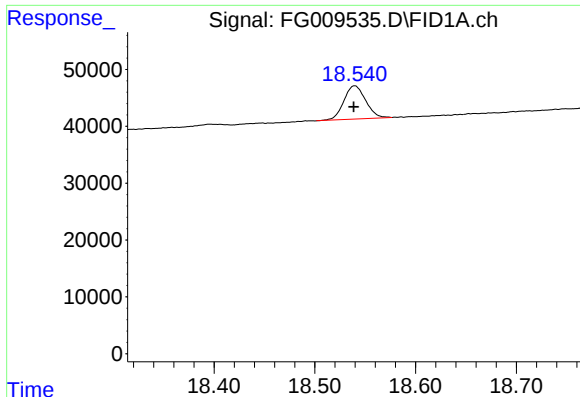

#14 N-DOTRIACONTANE


R.T.: 18.540 min
Delta R.T.: 0.001 min
Response: 87638
Conc: 0.75 ug/ml

Instrument :
FID_G
ClientSampleId :

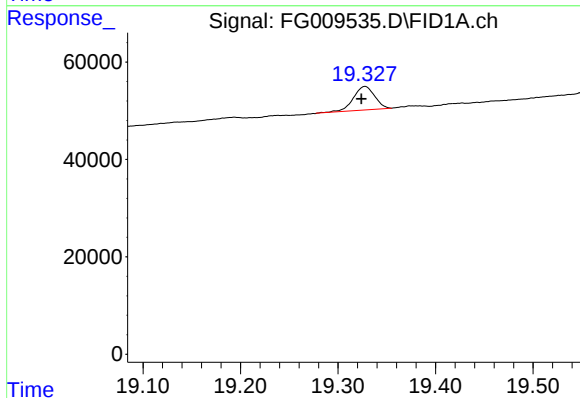


#15 N-TETRATRIACONTANE

R.T.: 19.328 min
Delta R.T.: 0.004 min
Response: 72610
Conc: 0.68 ug/ml

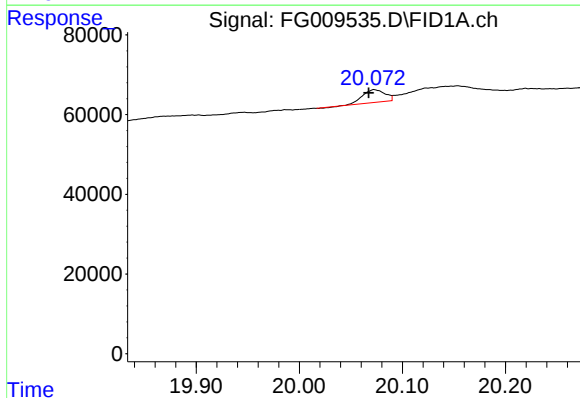

#16 N-HEXATRIACONTANE

R.T.: 20.073 min
Delta R.T.: 0.005 min
Response: 47210
Conc: 0.50 ug/ml

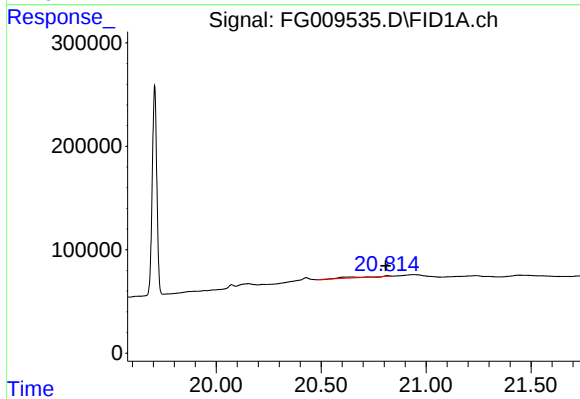

#17 N-OCTATRIACONTANE

R.T.: 20.815 min
Delta R.T.: 0.006 min
Response: 73343
Conc: 0.85 ug/ml