

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040723\
 Data File : FG011742.D
 Signal(s) : FID1A.ch
 Acq On : 07 Apr 2023 18:02
 Operator : YP\AJ
 Sample : 02213-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/10/2023
 Supervised By :Ankita Jodhani 04/10/2023

Integration File: autoint1.e
 Quant Time: Apr 10 03:35:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
 Quant Title :
 QLast Update : Wed Mar 15 18:43:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.050	1975569	19.627 ug/ml
Target Compounds			
2) N-DECANE	4.571	139457	1.154 ug/ml
3) N-DODECANE	6.742	138103	1.132 ug/ml
4) N-TETRADECANE	8.573	114436	0.940 ug/mlm
5) N-HEXADECANE	10.186	135969	1.103 ug/ml
6) N-OCTADECANE	11.633	145647	1.192 ug/ml
7) N-EICOSANE	12.946	143059	1.191 ug/ml
8) N-DOCOSANE	14.147	135966	1.185 ug/ml
10) N-TETRACOSANE	15.254	147985	1.310 ug/ml
11) N-HEXACOSANE	16.278	134061	1.241 ug/ml
12) N-OCTACOSANE	17.230	132828	1.281 ug/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040723\
Data File : FG011742.D
Signal(s) : FID1A.ch
Acq On : 07 Apr 2023 18:02
Operator : YP\AJ
Sample : 02213-09
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
MDL-WATER-03-QT2-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

Integration File: autoint1.e
Quant Time: Apr 10 03:35:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

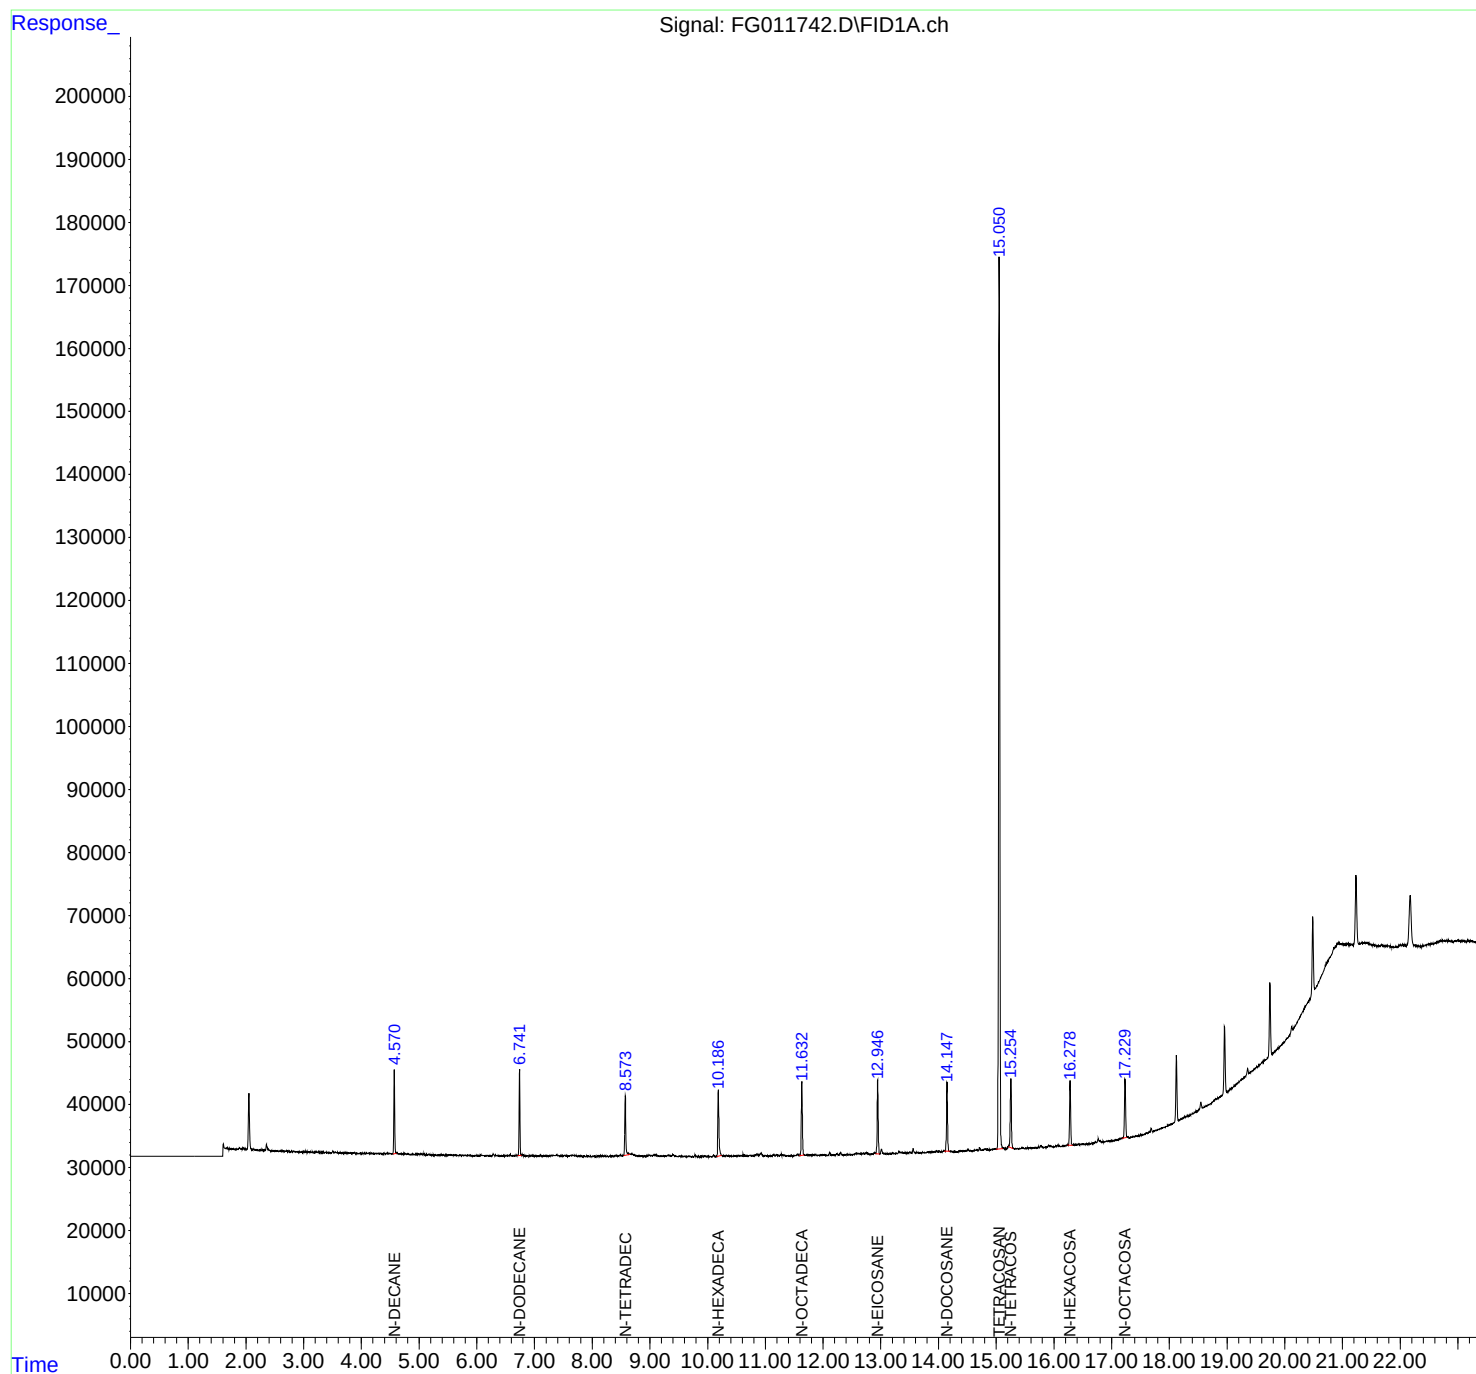

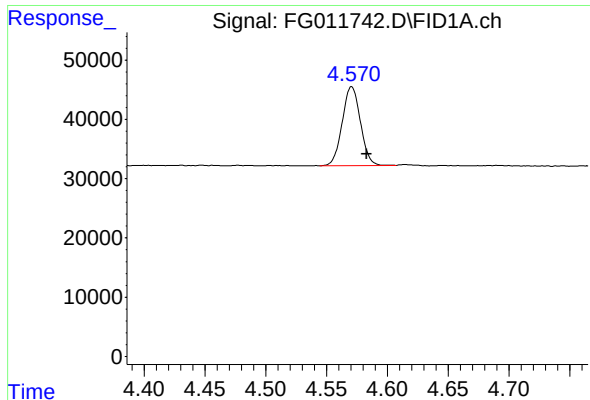


#2 N-DECANE

R.T.: 4.571 min
Delta R.T.: -0.012 min
Response: 139457
Conc: 1.15 ug/ml

Instrument :
FID_G
ClientSampleId :
MDL-WATER-03-QT2-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

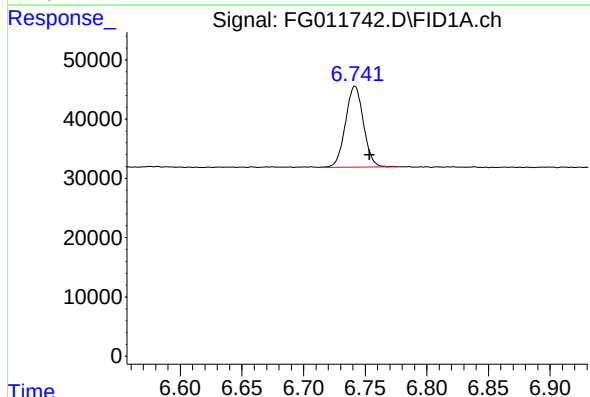


#3 N-DODECANE

R.T.: 6.742 min
Delta R.T.: -0.012 min
Response: 138103
Conc: 1.13 ug/ml

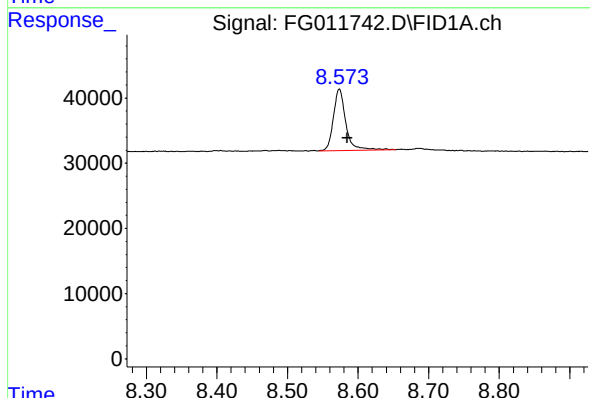


#4 N-TETRADECANE

R.T.: 8.573 min
Delta R.T.: -0.011 min
Response: 114436
Conc: 0.94 ug/ml m

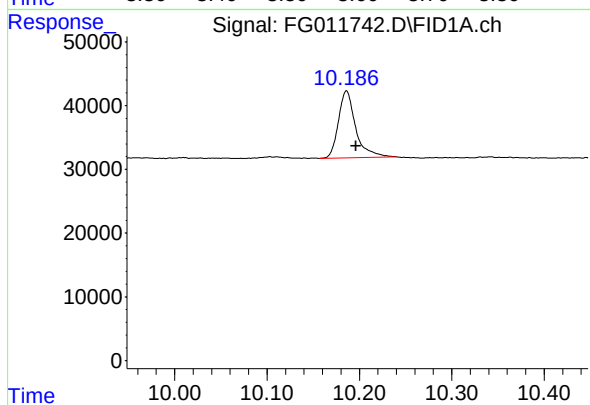

#5 N-HEXADECANE

R.T.: 10.186 min
Delta R.T.: -0.010 min
Response: 135969
Conc: 1.10 ug/ml

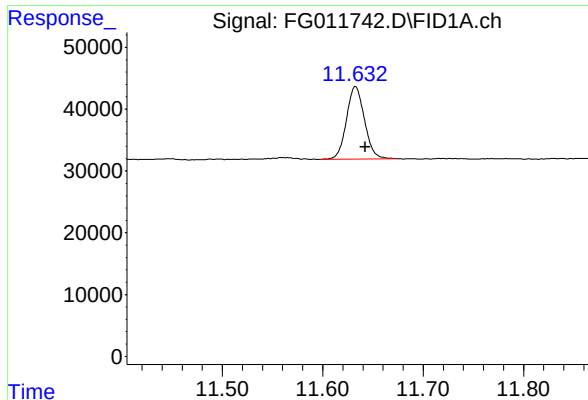


#6 N-OCTADECANE

R.T.: 11.633 min
Delta R.T.: -0.010 min
Response: 145647
Conc: 1.19 ug/ml

Instrument :
FID_G
ClientSampleId :
MDL-WATER-03-QT2-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

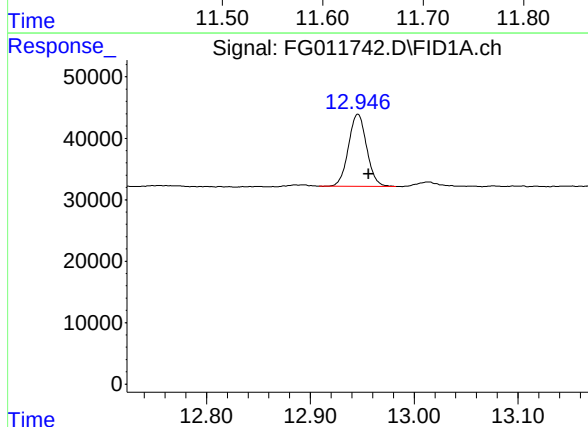


#7 N-EICOSANE

R.T.: 12.946 min
Delta R.T.: -0.010 min
Response: 143059
Conc: 1.19 ug/ml

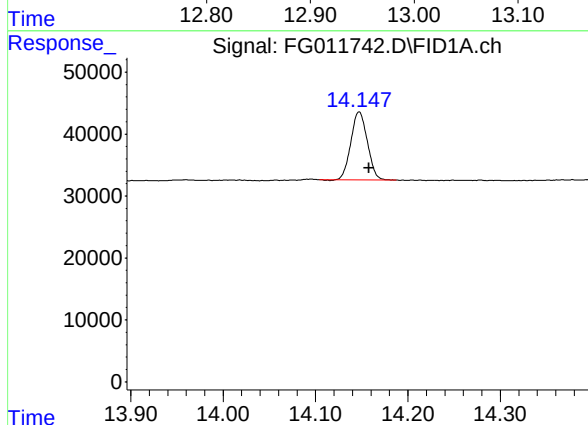


#8 N-DOCOSANE

R.T.: 14.147 min
Delta R.T.: -0.011 min
Response: 135966
Conc: 1.19 ug/ml

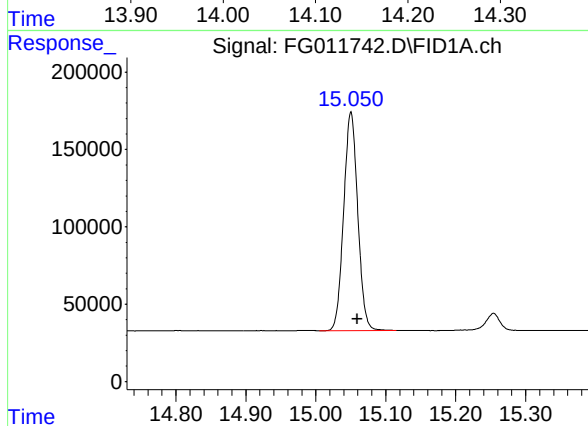

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.050 min
Delta R.T.: -0.009 min
Response: 1975569
Conc: 19.63 ug/ml

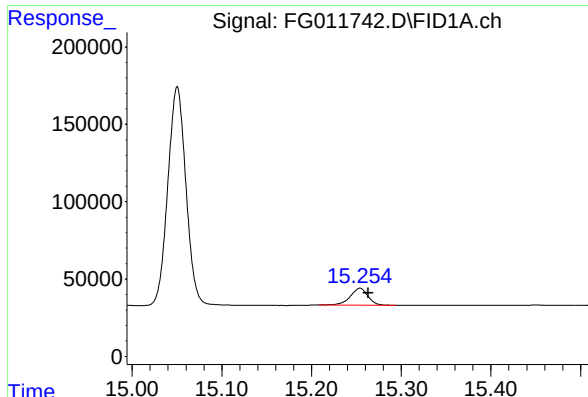


#10 N-TETRACOSANE

R.T.: 15.254 min
Delta R.T.: -0.009 min
Response: 147985
Conc: 1.31 ug/ml

Instrument : FID_G
ClientSampleId : MDL-WATER-03-QT2-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

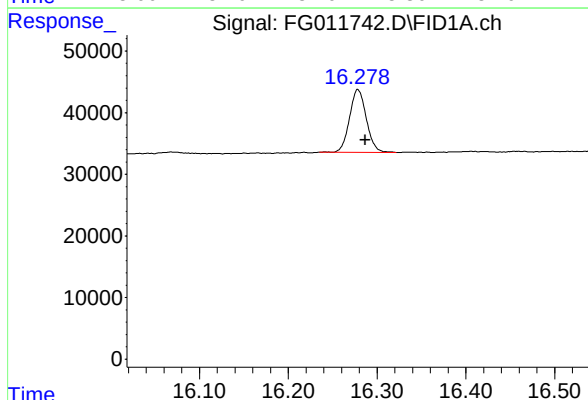

#11 N-HEXACOSANE

R.T.: 16.278 min
Delta R.T.: -0.008 min
Response: 134061
Conc: 1.24 ug/ml

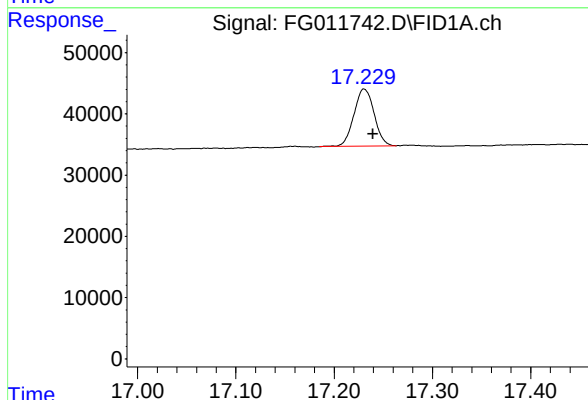

#12 N-OCTACOSANE

R.T.: 17.230 min
Delta R.T.: -0.009 min
Response: 132828
Conc: 1.28 ug/ml