

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040822\
Data File : FG009553.D
Signal(s) : FID1A.ch
Acq On : 08 Apr 2022 09:56
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 23:45:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.363	4277427	28.381 ug/ml
12)	N-OCTACOSANE	16.836	3690891	28.280 ug/ml
13)	N-TRIACONTANE	17.725	173887	1.408 ug/ml
14)	N-DOTRIACONTANE	18.564	232674	2.004 ug/ml
15)	N-TETRATRIACONTANE	19.352	430648	4.050 ug/ml
16)	N-HEXATRIACONTANE	20.097	790474	8.348 ug/ml
17)	N-OCTATRIACONTANE	20.840	803441	9.330 ug/ml
18)	N-TETRACONTANE	21.767	241565	2.799 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040822\
Data File : FG009553.D
Signal(s) : FID1A.ch
Acq On : 08 Apr 2022 09:56
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 23:45:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

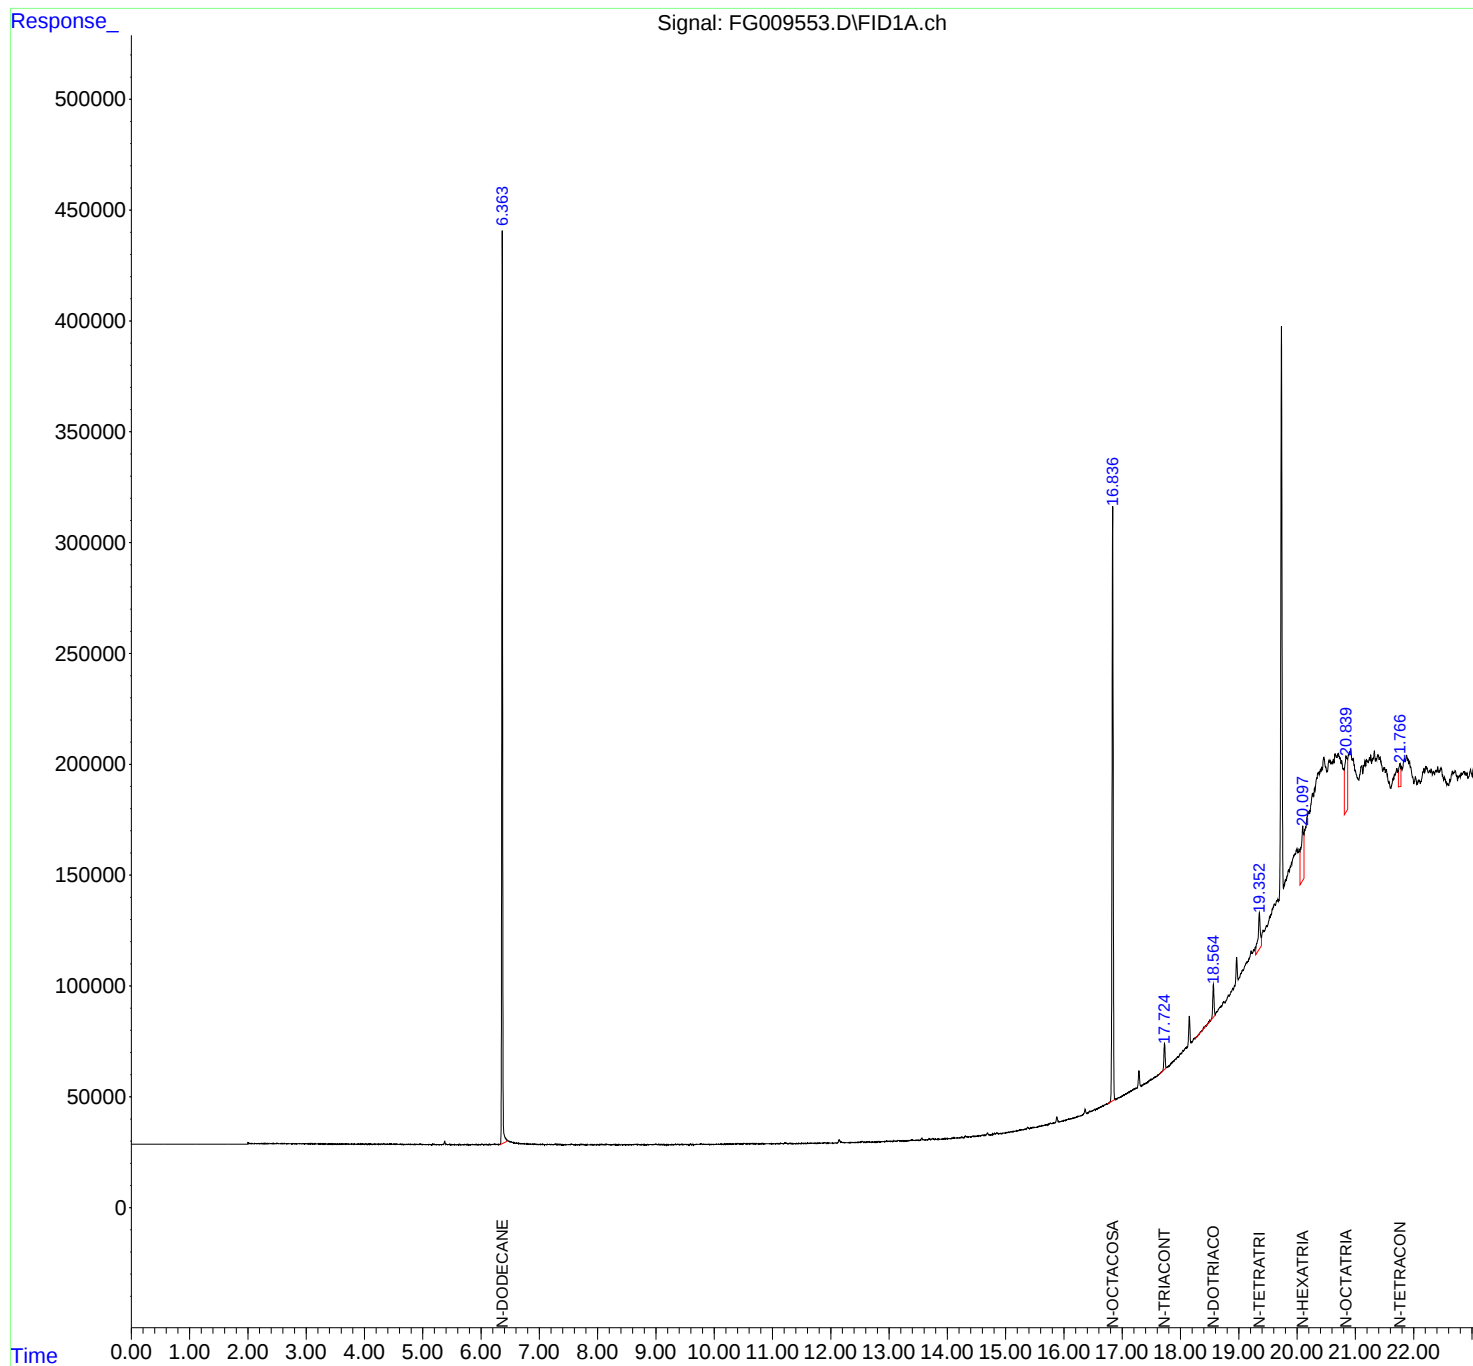


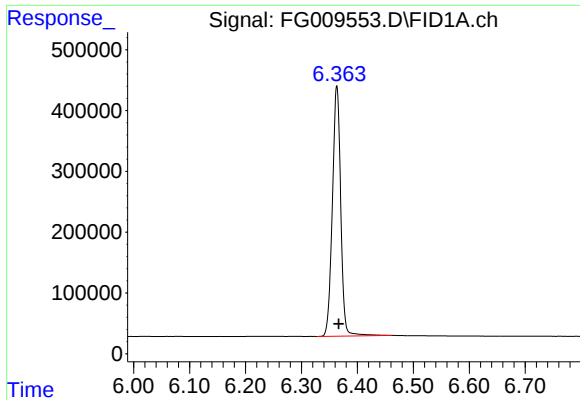

#3 N-DODECANE


R.T.: 6.363 min
Delta R.T.: -0.003 min
Response: 4277427
Conc: 28.38 ug/ml

Instrument :
FID_G
ClientSampleId :

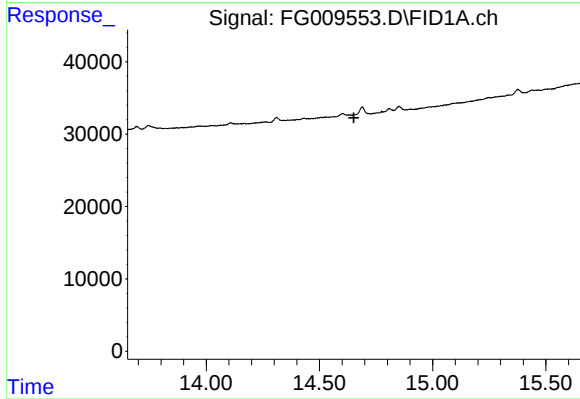


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.652 min
Response: 0
Conc: N.D.

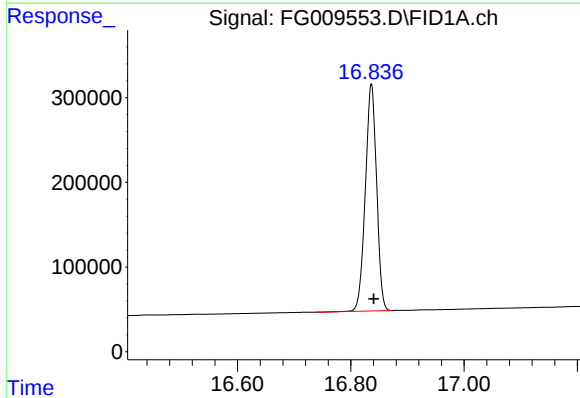


#12 N-OCTACOSANE

R.T.: 16.836 min
Delta R.T.: -0.004 min
Response: 3690891
Conc: 28.28 ug/ml

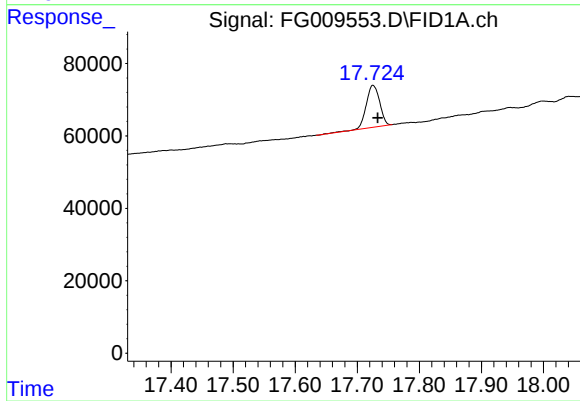

#13 N-TRIACONTANE


R.T.: 17.725 min
Delta R.T.: -0.008 min
Response: 173887
Conc: 1.41 ug/ml

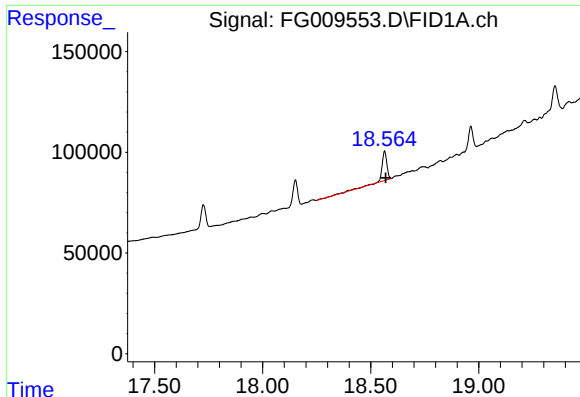

#14 N-DOTRIACONTANE


R.T.: 18.564 min
Delta R.T.: -0.006 min
Response: 232674
Conc: 2.00 ug/ml

Instrument :
FID_G
ClientSampleId :

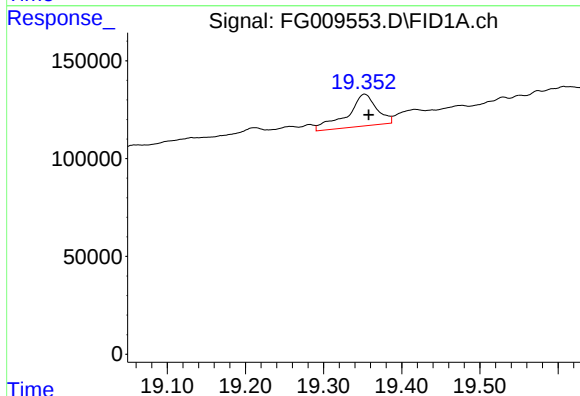


#15 N-TETRATRIACONTANE

R.T.: 19.352 min
Delta R.T.: -0.005 min
Response: 430648
Conc: 4.05 ug/ml

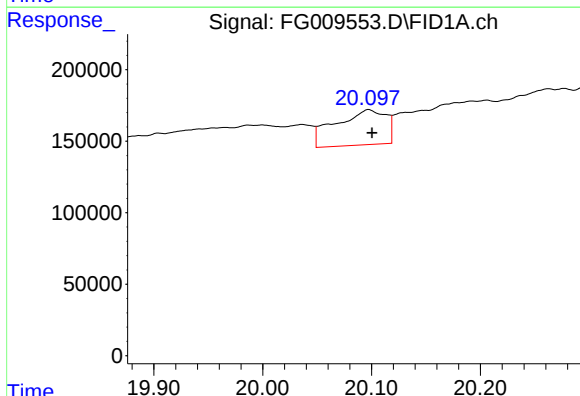


#16 N-HEXATRIACONTANE

R.T.: 20.097 min
Delta R.T.: -0.003 min
Response: 790474
Conc: 8.35 ug/ml

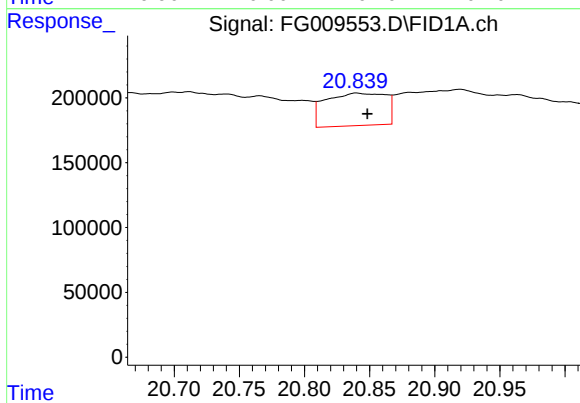

#17 N-OCTATRIACONTANE

R.T.: 20.840 min
Delta R.T.: -0.009 min
Response: 803441
Conc: 9.33 ug/ml

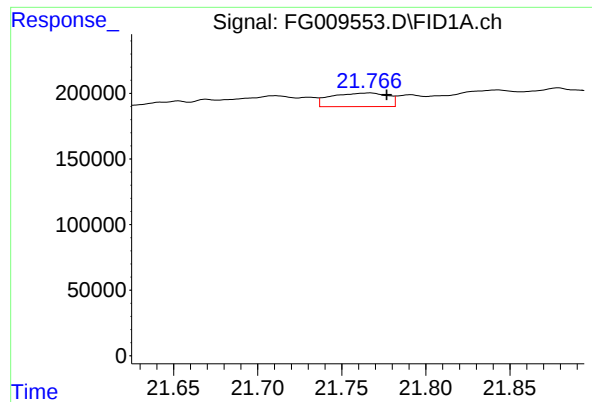

#18 N-TETRACONTANE

R.T.: 21.767 min
Delta R.T.: -0.010 min
Response: 241565
Conc: 2.80 ug/ml

Instrument :
FID_G
ClientSampleId :