

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040823\
Data File : FG011746.D
Signal(s) : FID1A.ch
Acq On : 07 Apr 2023 20:29
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 04:18:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.954	53627	0.578 ug/ml
15) N-TETRATRIACONTANE	19.741	59031	0.700 ug/ml
16) N-HEXATRIACONTANE	20.484	67196	0.873 ug/ml
17) N-OCTATRIACONTANE	21.234	95081	1.263 ug/ml
18) N-TETRACONTANE	22.172	151191	2.060 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040823\
Data File : FG011746.D
Signal(s) : FID1A.ch
Acq On : 07 Apr 2023 20:29
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 04:18:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

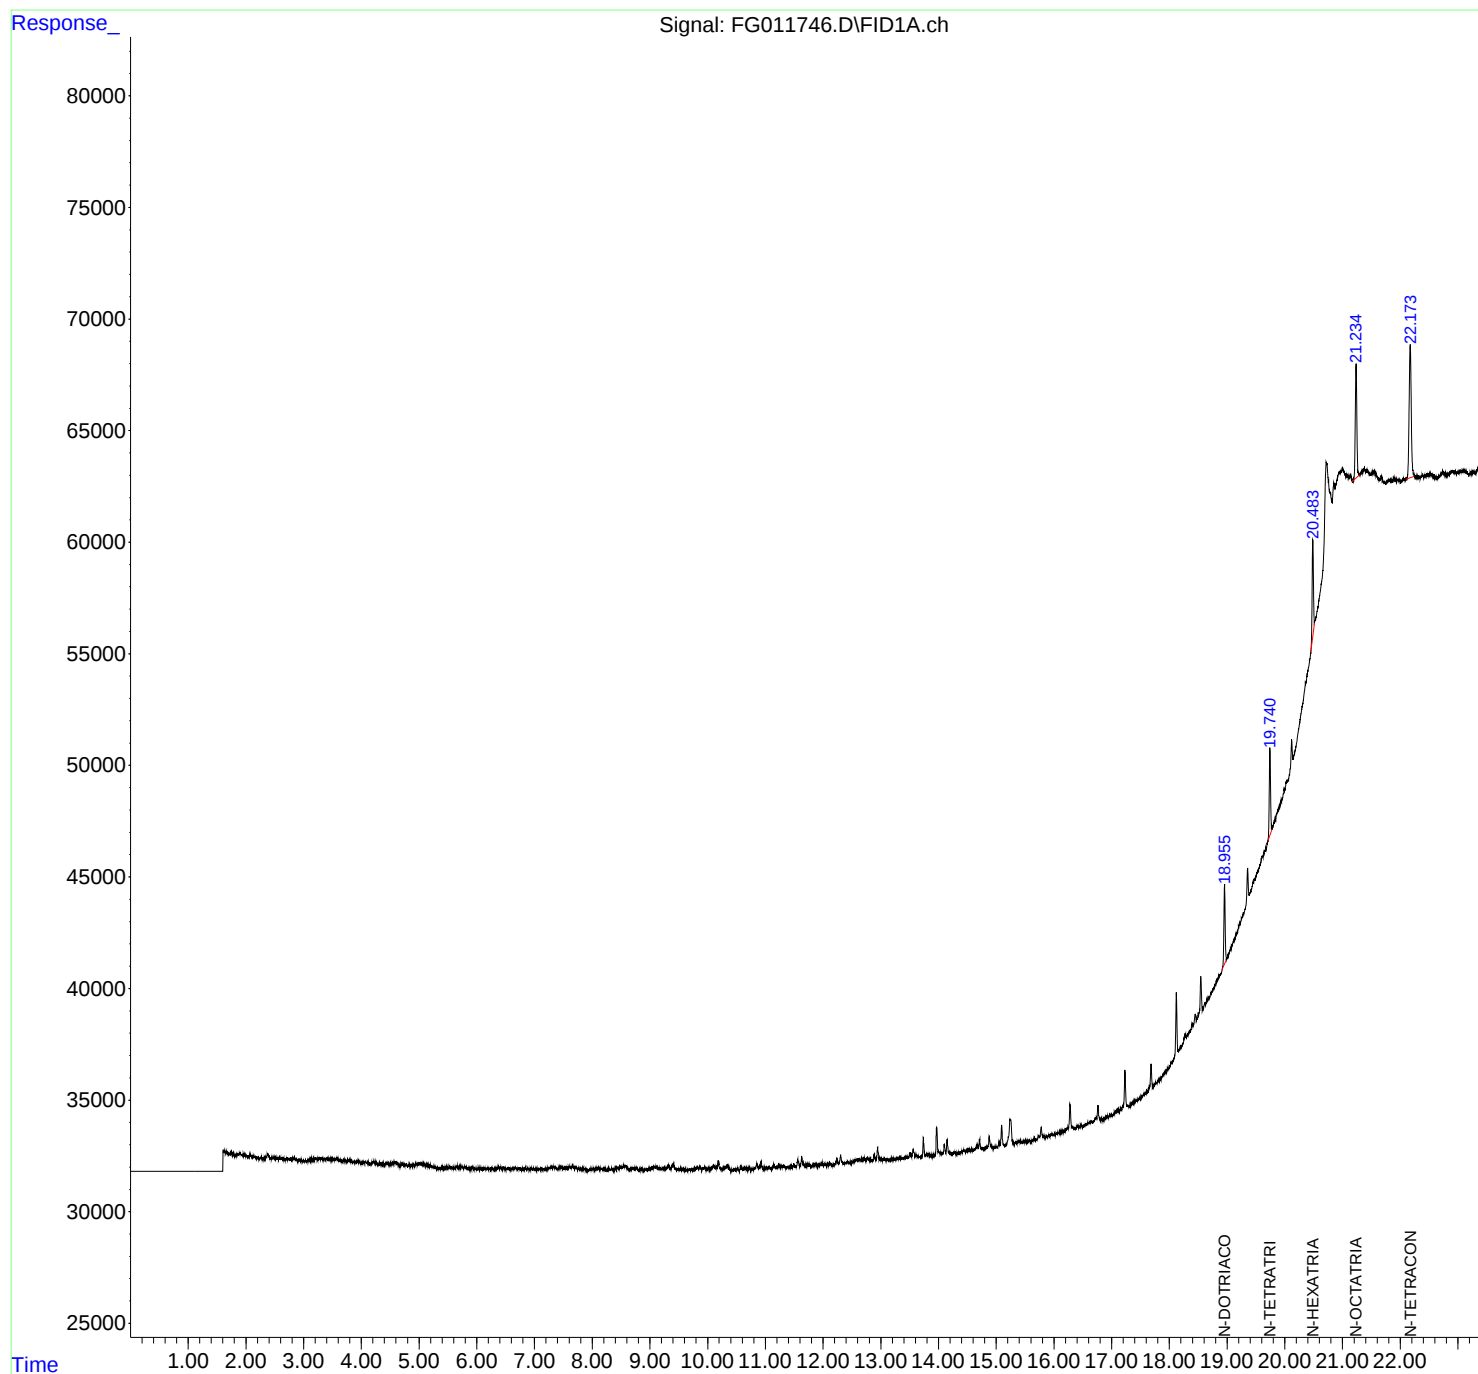


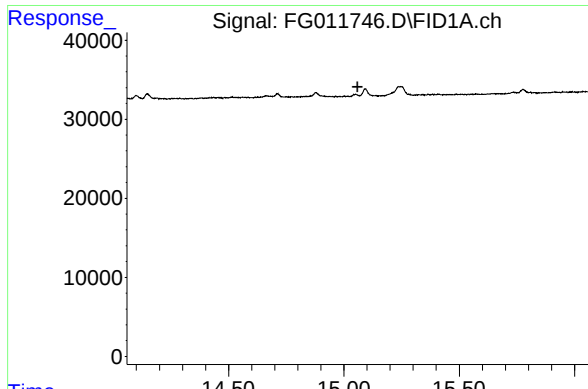

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.059 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

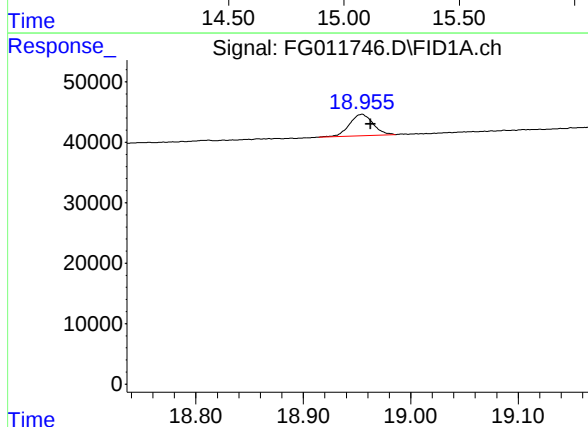


#14 N-DOTRIACONTANE

R.T.: 18.954 min
Delta R.T.: -0.008 min
Response: 53627
Conc: 0.58 ug/ml

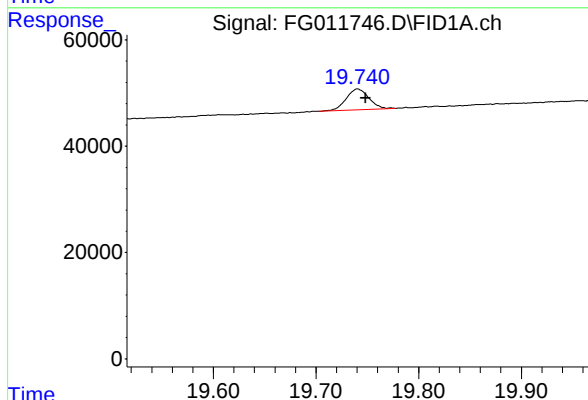


#15 N-TETRATRIACONTANE

R.T.: 19.741 min
Delta R.T.: -0.008 min
Response: 59031
Conc: 0.70 ug/ml

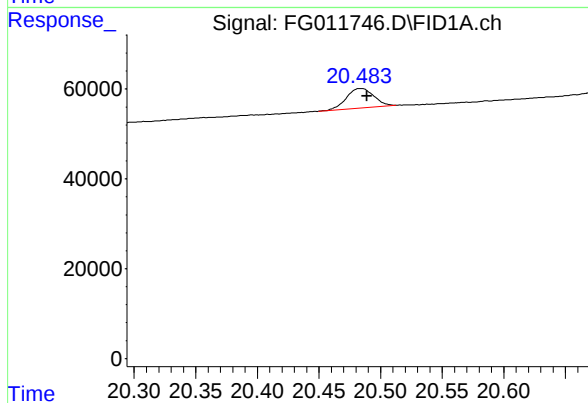

#16 N-HEXATRIACONTANE

R.T.: 20.484 min
Delta R.T.: -0.005 min
Response: 67196
Conc: 0.87 ug/ml

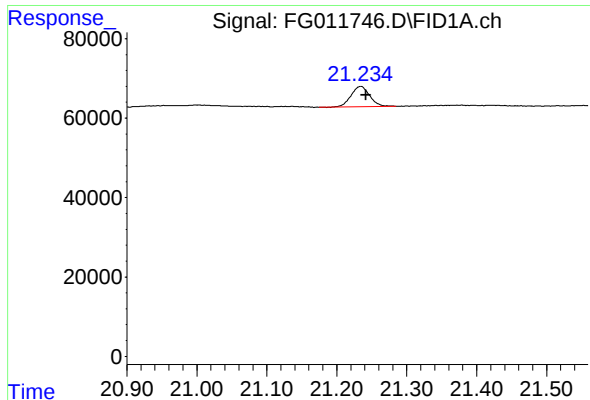


#17 N-OCTATRIACONTANE

R.T.: 21.234 min
Delta R.T.: -0.008 min
Response: 95081
Conc: 1.26 ug/ml

Instrument :

FID_G

ClientSampleId :

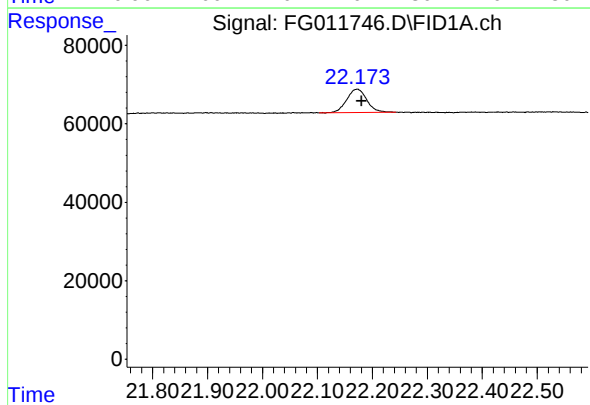

#18 N-TETRACONTANE

R.T.: 22.172 min
Delta R.T.: -0.008 min
Response: 151191
Conc: 2.06 ug/ml