

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040823\
 Data File : FG011749.D
 Signal(s) : FID1A.ch
 Acq On : 07 Apr 2023 21:57
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 10 04:18:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
 Quant Title :
 QLast Update : Wed Mar 15 18:43:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.741	2903758	23.796 ug/ml
12) N-OCTACOSANE	17.229	2436338	23.496 ug/ml
13) N-TRIACONTANE	18.117	54796	0.553 ug/ml
14) N-DOTRIACONTANE	18.953	76137	0.821 ug/ml
15) N-TETRATRIACONTANE	19.739	81675	0.969 ug/ml
16) N-HEXATRIACONTANE	20.482	79447	1.032 ug/ml
17) N-OCTATRIACONTANE	21.230	97014	1.289 ug/ml
18) N-TETRACONTANE	22.168	144775	1.973 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040823\
Data File : FG011749.D
Signal(s) : FID1A.ch
Acq On : 07 Apr 2023 21:57
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 04:18:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

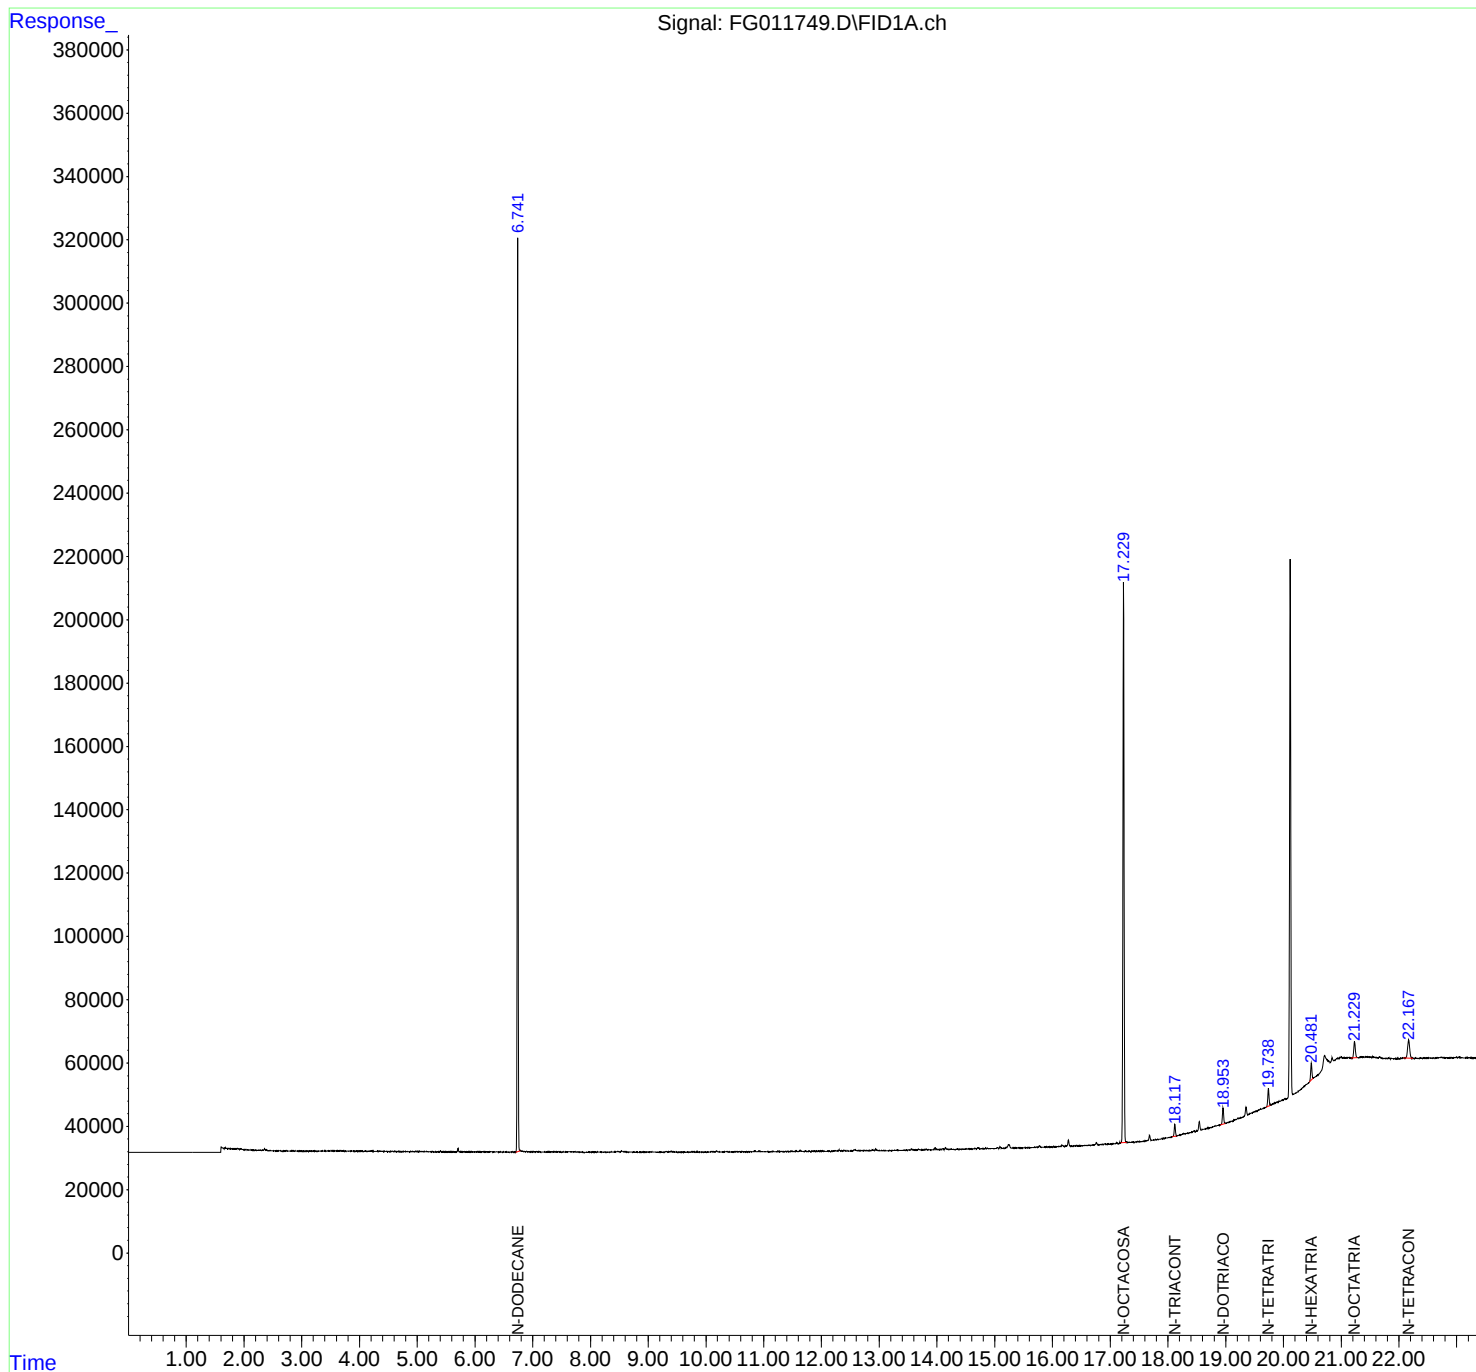


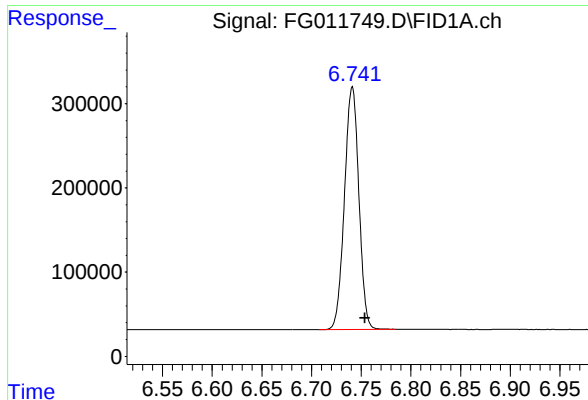

#3 N-DODECANE


R.T.: 6.741 min
Delta R.T.: -0.012 min
Response: 2903758
Conc: 23.80 ug/ml

Instrument :
FID_G
ClientSampleId :

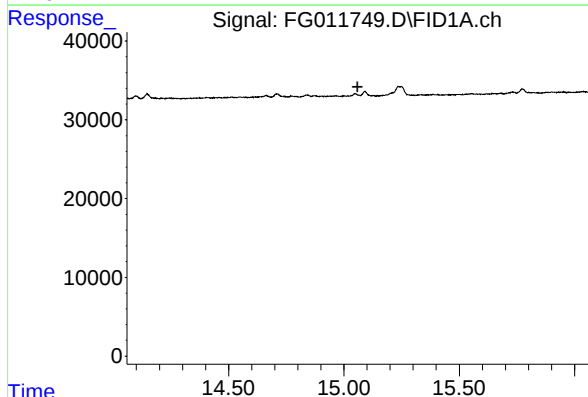


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.059 min
Response: 0
Conc: N.D.

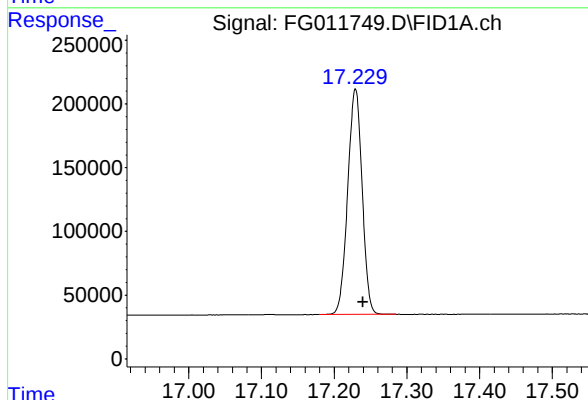


#12 N-OCTACOSANE

R.T.: 17.229 min
Delta R.T.: -0.010 min
Response: 2436338
Conc: 23.50 ug/ml

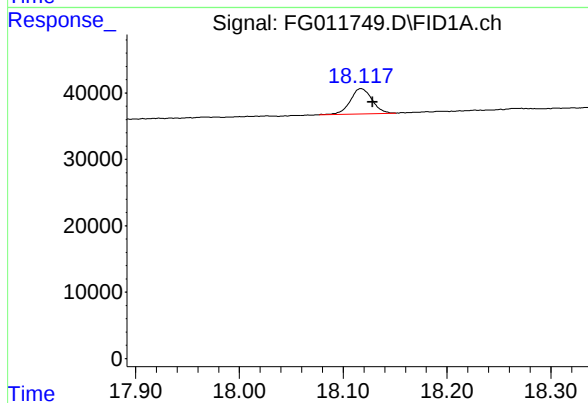

#13 N-TRIACONTANE


R.T.: 18.117 min
Delta R.T.: -0.011 min
Response: 54796
Conc: 0.55 ug/ml

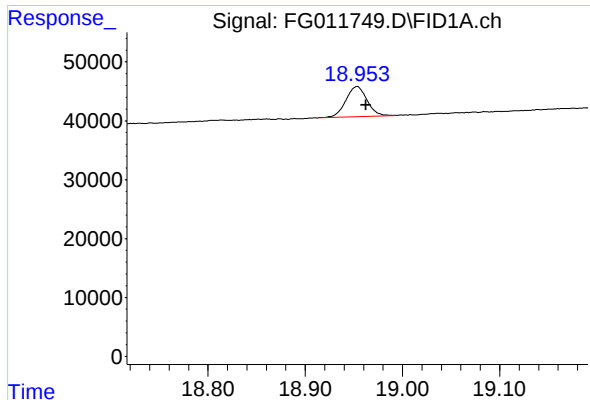

#14 N-DOTRIACONTANE


R.T.: 18.953 min
Delta R.T.: -0.009 min
Response: 76137
Conc: 0.82 ug/ml

Instrument :
FID_G
ClientSampleId :

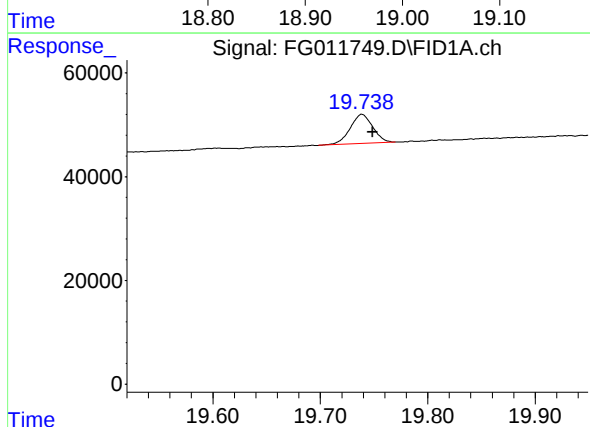


#15 N-TETRATRIACONTANE

R.T.: 19.739 min
Delta R.T.: -0.010 min
Response: 81675
Conc: 0.97 ug/ml

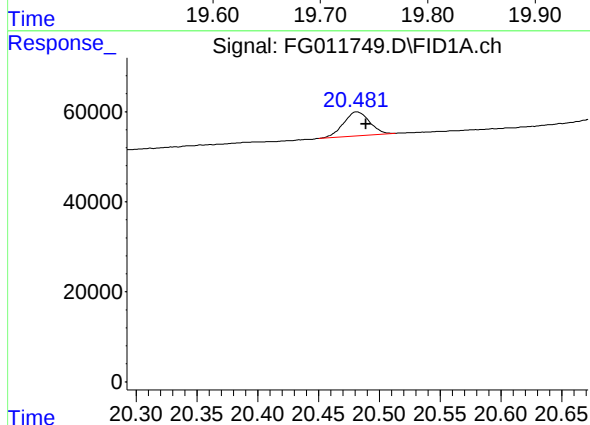


#16 N-HEXATRIACONTANE

R.T.: 20.482 min
Delta R.T.: -0.007 min
Response: 79447
Conc: 1.03 ug/ml

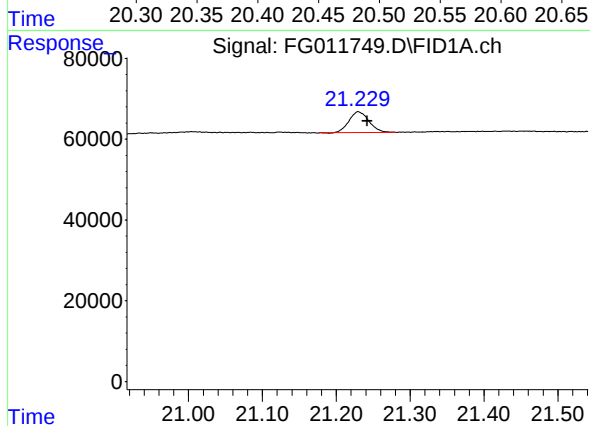

#17 N-OCTATRIACONTANE

R.T.: 21.230 min
Delta R.T.: -0.013 min
Response: 97014
Conc: 1.29 ug/ml

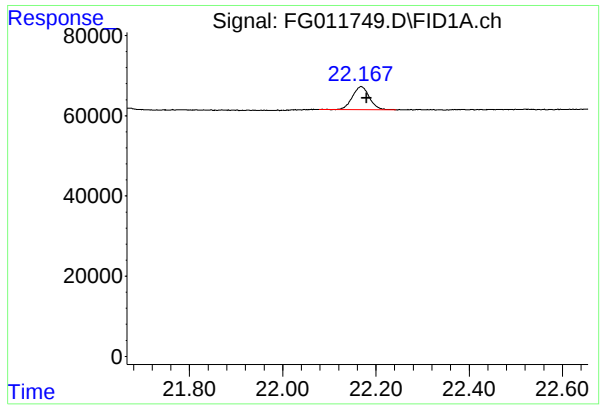

#18 N-TETRACONTANE

R.T.: 22.168 min
Delta R.T.: -0.012 min
Response: 144775
Conc: 1.97 ug/ml

Instrument :
FID_G
ClientSampleId :