

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040823\
Data File : FG011753.D
Signal(s) : FID1A.ch
Acq On : 07 Apr 2023 23:55
Operator : YP\AJ
Sample : PB151919BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 04:19:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.048	2124887	21.111 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.118	49771	0.502 ug/ml
14) N-DOTRIACONTANE	18.953	60420	0.651 ug/ml
15) N-TETRATRIACONTANE	19.740	51104	0.606 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040823\
Data File : FG011753.D
Signal(s) : FID1A.ch
Acq On : 07 Apr 2023 23:55
Operator : YP\AJ
Sample : PB151919BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 04:19:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

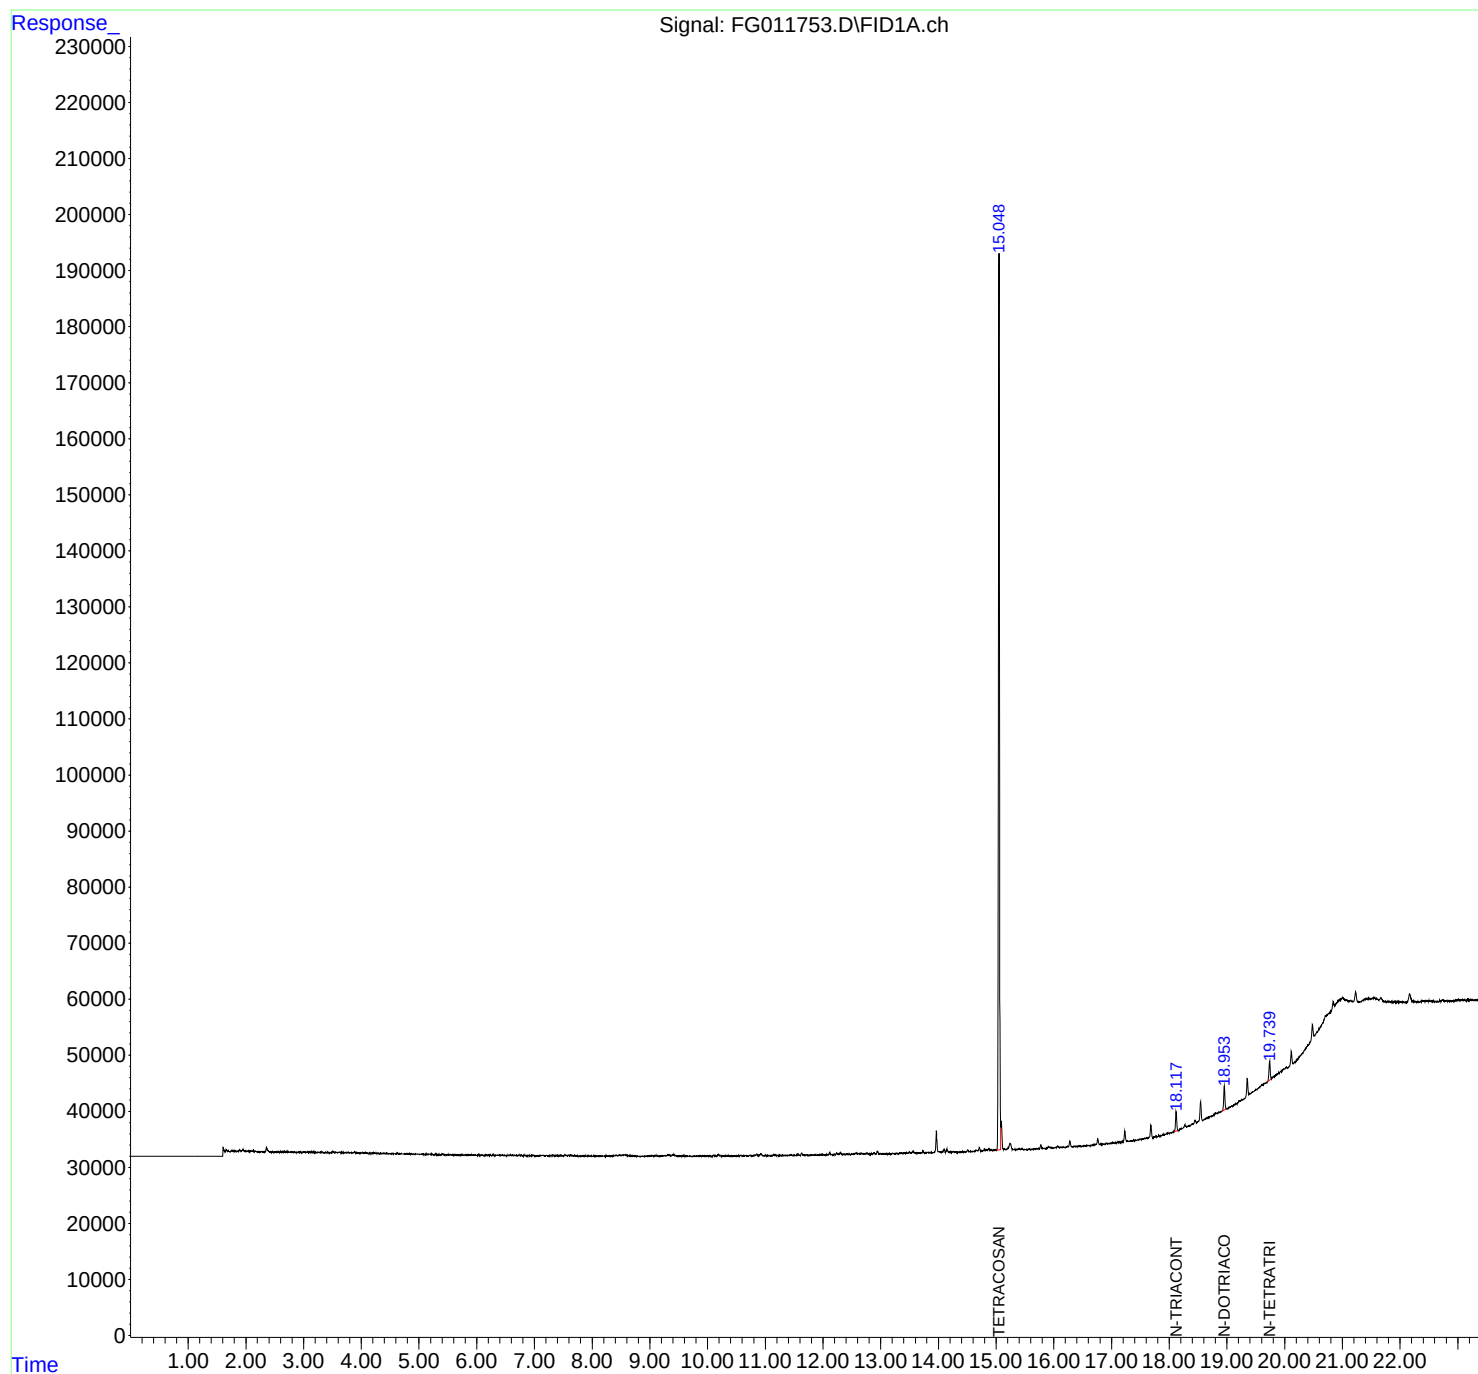


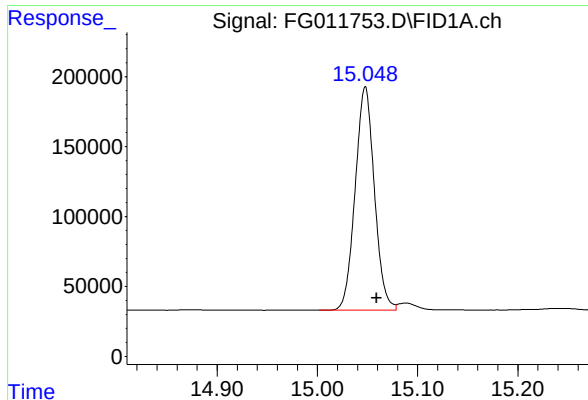

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.048 min
Delta R.T.: -0.011 min
Response: 2124887
Conc: 21.11 ug/ml

Instrument :
FID_G
ClientSampleId :

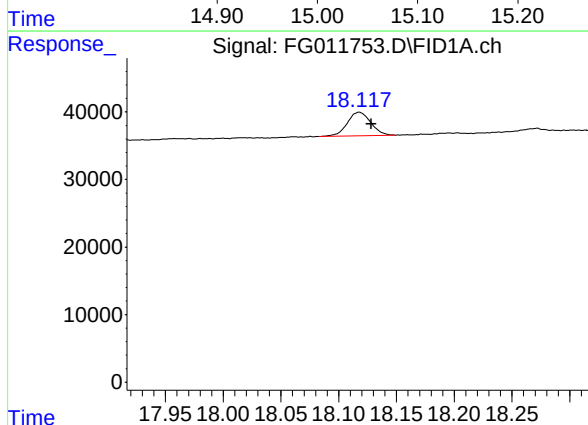


#13 N-TRIACONTANE

R.T.: 18.118 min
Delta R.T.: -0.010 min
Response: 49771
Conc: 0.50 ug/ml

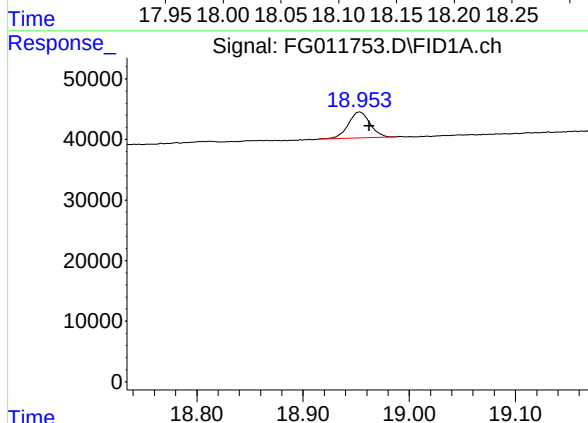

#14 N-DOTRIACONTANE

R.T.: 18.953 min
Delta R.T.: -0.009 min
Response: 60420
Conc: 0.65 ug/ml

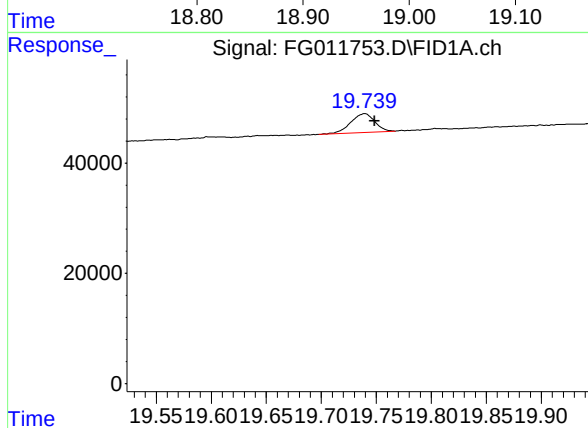

#15 N-TETRATRIACONTANE

R.T.: 19.740 min
Delta R.T.: -0.009 min
Response: 51104
Conc: 0.61 ug/ml