

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
Data File : FG004621.D
Signal(s) : FID1A.ch
Acq On : 09 Apr 2019 15:31
Operator : AJ\SJ
Sample : I.BLK
Misc : LOQ-WATER-01 (10 PPM)
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Apr 10 00:43:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.411	1848121	17.917 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.309	106557	0.909 ug/ml
18) N-TETRACONTANE	21.397	208778	1.930 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
Data File : FG004621.D
Signal(s) : FID1A.ch
Acq On : 09 Apr 2019 15:31
Operator : AJ\SJ
Sample : I.BLK
Misc : LOQ-WATER-01 (10 PPM)
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :
I.BLK

Integration File: autoint1.e
Quant Time: Apr 10 00:43:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

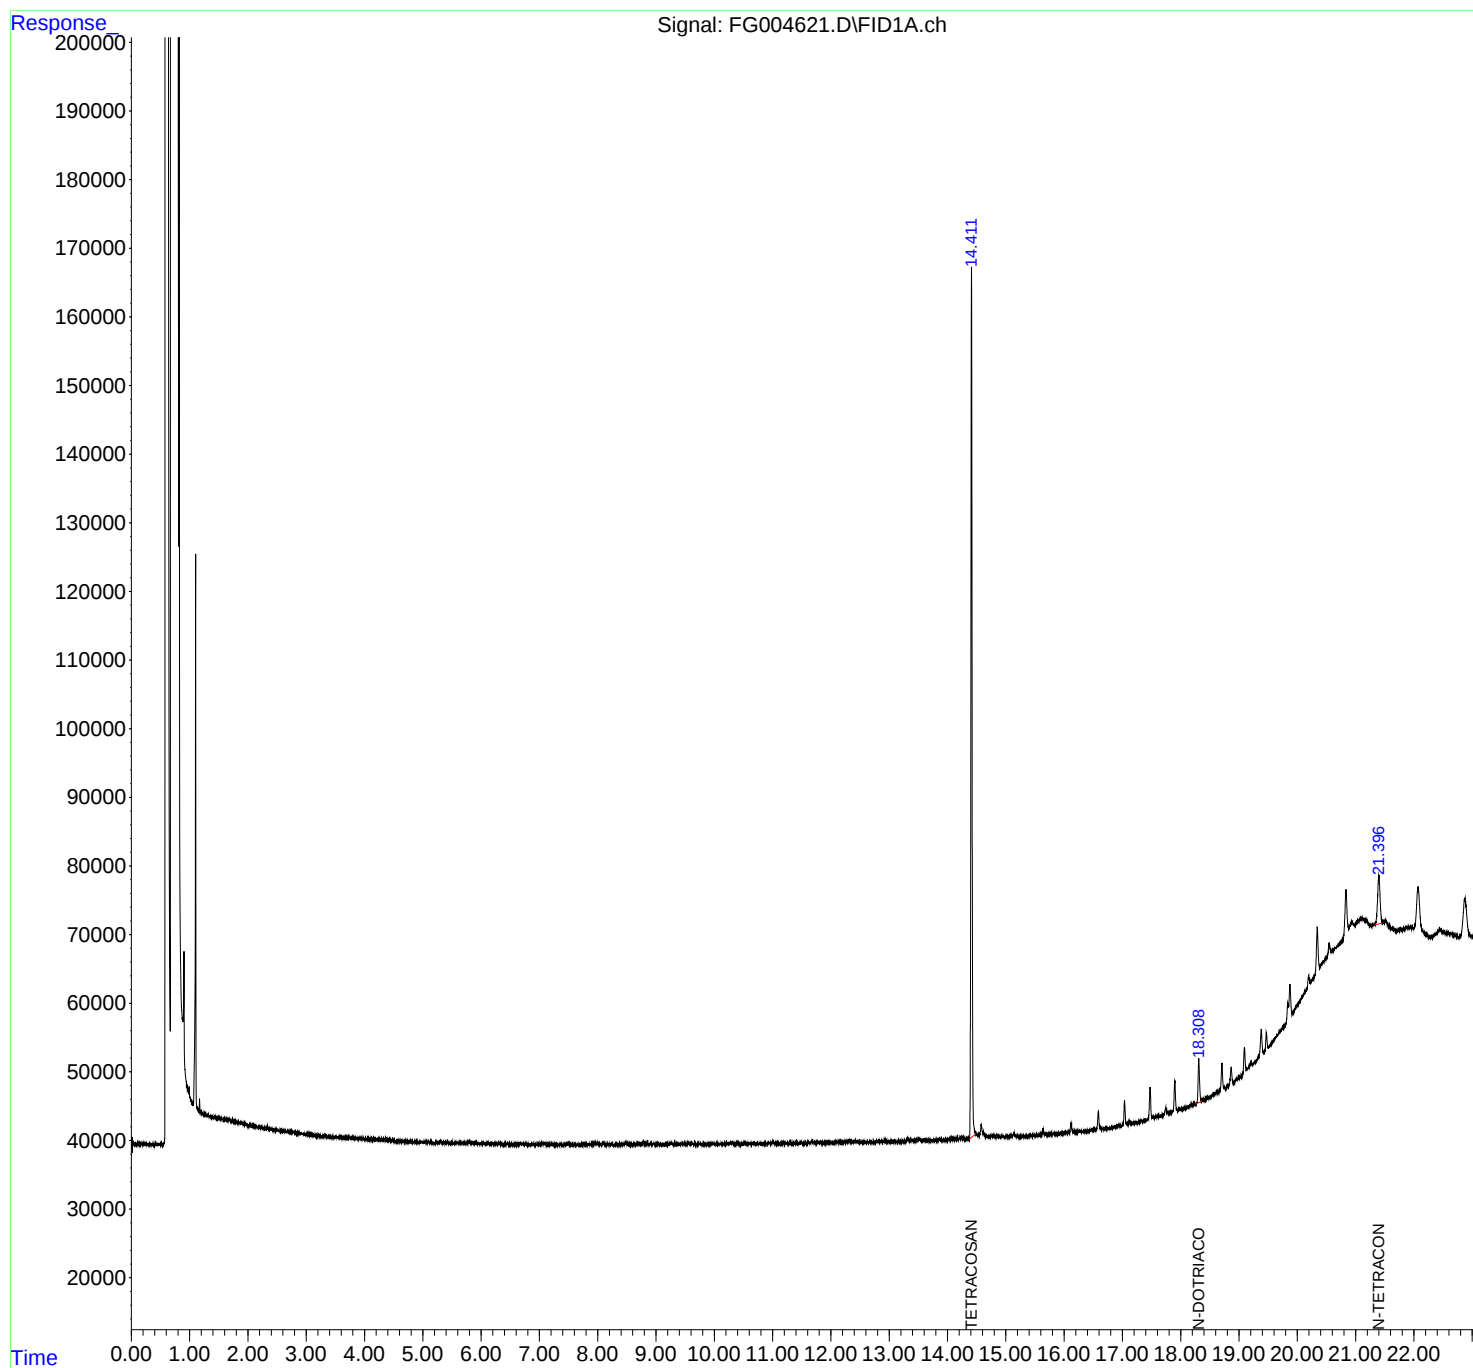


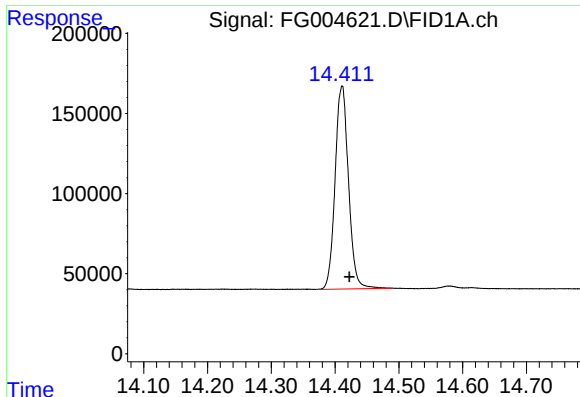

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.411 min
Delta R.T.: -0.011 min
Response: 1848121
Conc: 17.92 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

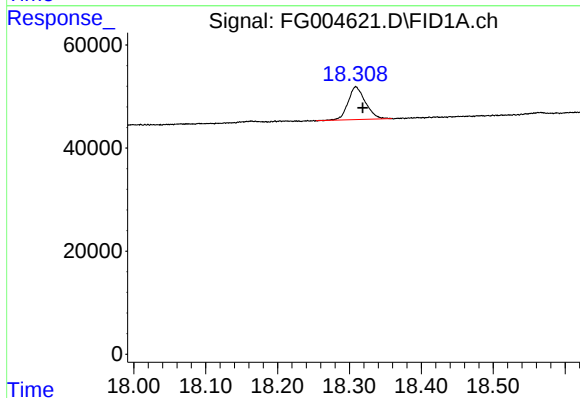

#14 N-DOTRIACONTANE

R.T.: 18.309 min
Delta R.T.: -0.010 min
Response: 106557
Conc: 0.91 ug/ml

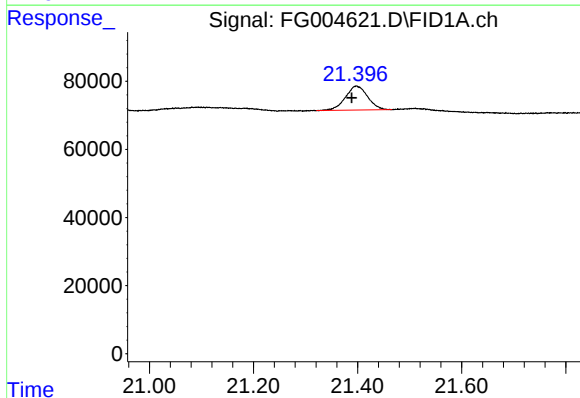

#18 N-TETRACONTANE

R.T.: 21.397 min
Delta R.T.: 0.008 min
Response: 208778
Conc: 1.93 ug/ml