

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
 Data File : FG004623.D
 Signal(s) : FID1A.ch
 Acq On : 09 Apr 2019 16:33
 Operator : AJ\SJ
 Sample : K2338-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 TP-2-DEEP

Integration File: autoint1.e
 Quant Time: Apr 10 00:43:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.409	1443249	13.992 ug/ml
Target Compounds			
4) N-TETRADECANE	8.026f	214682	1.981 ug/ml
7) N-EICOSANE	12.381f	184755	1.616 ug/ml
10) N-TETRACOSANE	14.614	288516	2.498 ug/ml
12) N-OCTACOSANE	16.584	287133	2.482 ug/ml
13) N-TRIACONTANE	17.473	450700	3.799 ug/ml
14) N-DOTRIACONTANE	18.307	380923	3.249 ug/ml
16) N-HEXATRIACONTANE	19.875	229304	2.057 ug/ml
18) N-TETRACONTANE	21.399	449094	4.152 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
Data File : FG004623.D
Signal(s) : FID1A.ch
Acq On : 09 Apr 2019 16:33
Operator : AJ\SJ
Sample : K2338-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-2-DEEP

Integration File: autoint1.e
Quant Time: Apr 10 00:43:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

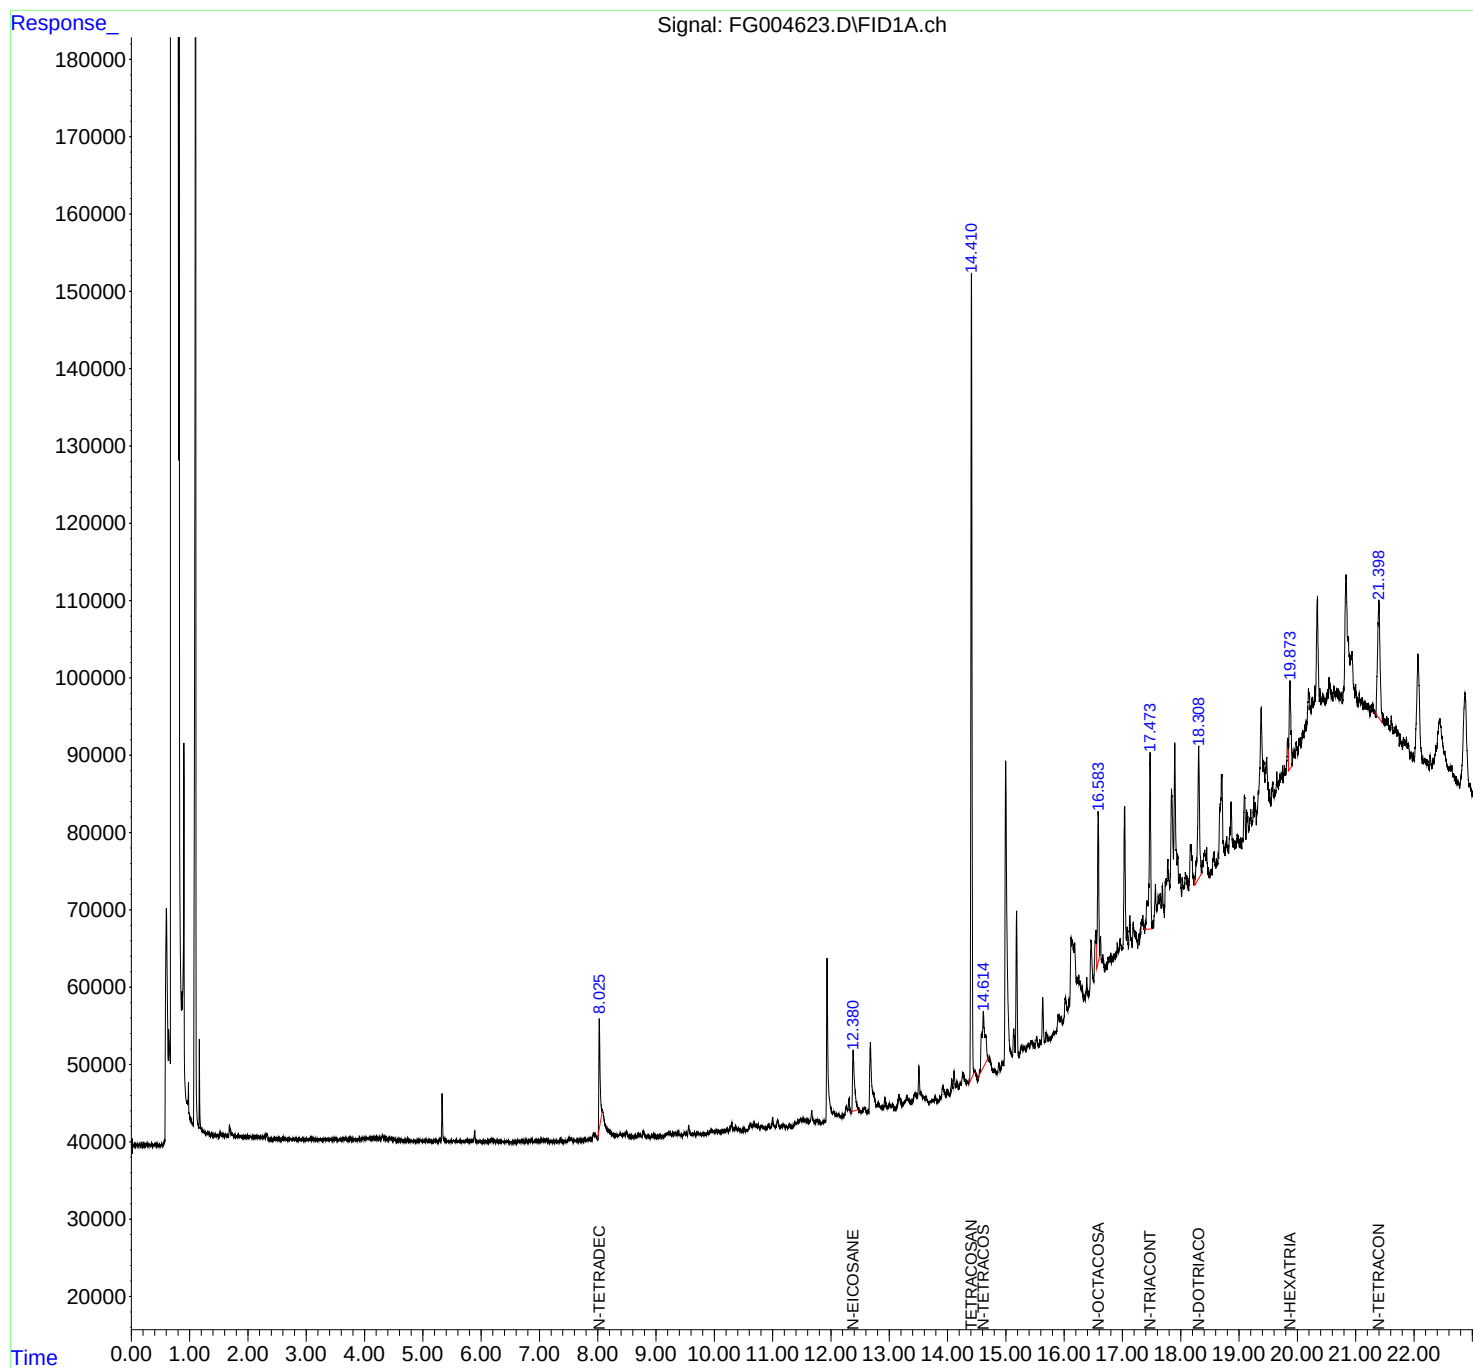


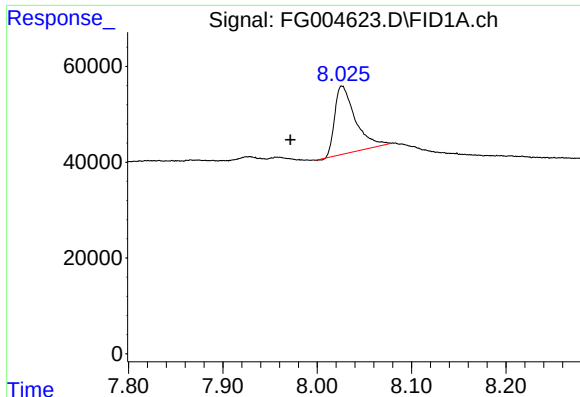

#4 N-TETRADECANE


R.T.: 8.026 min
Delta R.T.: 0.055 min
Response: 214682
Conc: 1.98 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-2-DEEP

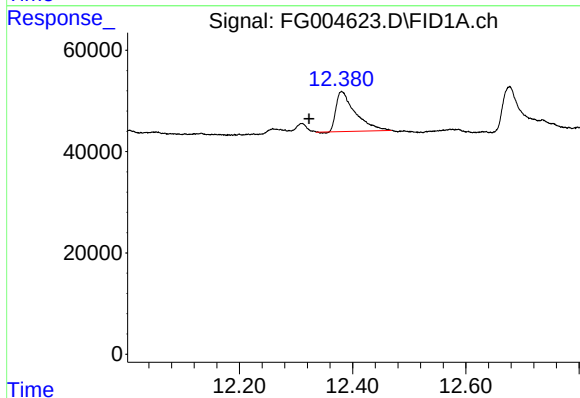


#7 N-EICOSANE

R.T.: 12.381 min
Delta R.T.: 0.058 min
Response: 184755
Conc: 1.62 ug/ml

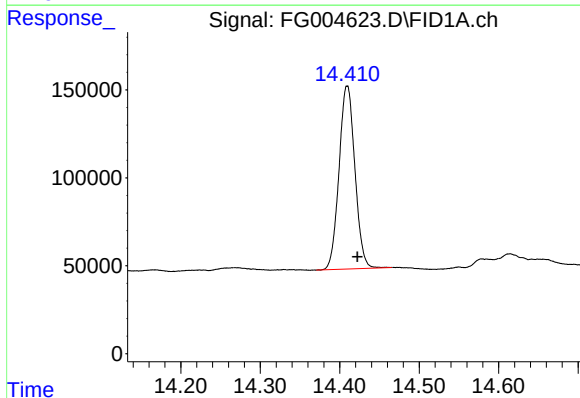


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.409 min
Delta R.T.: -0.013 min
Response: 1443249
Conc: 13.99 ug/ml

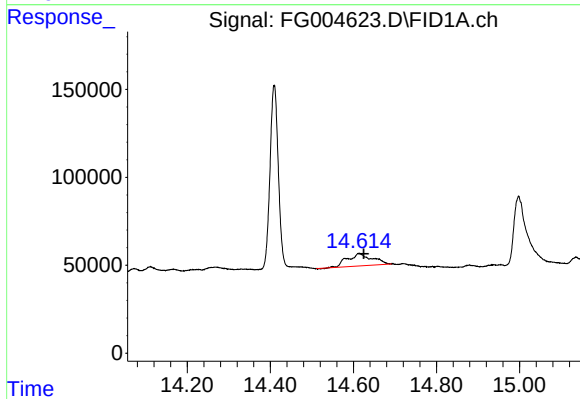

#10 N-TETRACOSANE


R.T.: 14.614 min
Delta R.T.: -0.011 min
Response: 288516
Conc: 2.50 ug/ml

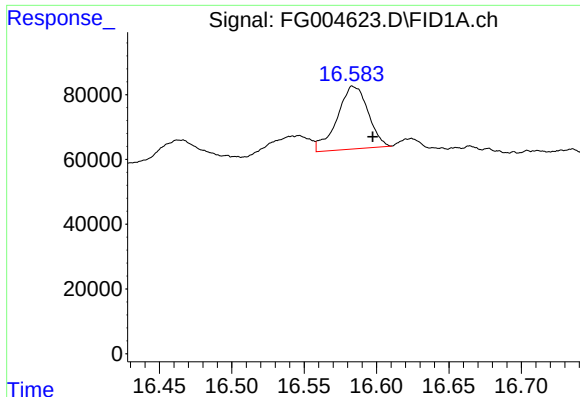

#12 N-OCTACOSANE


R.T.: 16.584 min
Delta R.T.: -0.013 min
Response: 287133
Conc: 2.48 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-2-DEEP

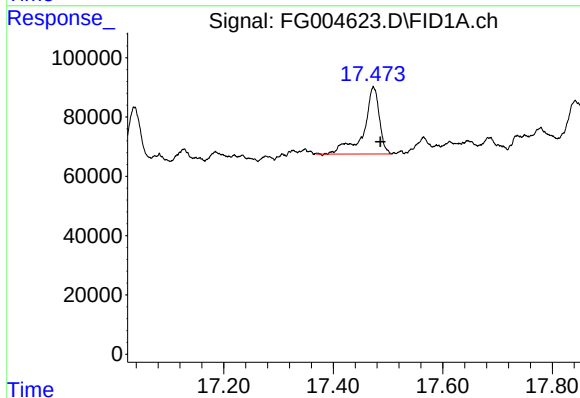


#13 N-TRIACONTANE

R.T.: 17.473 min
Delta R.T.: -0.013 min
Response: 450700
Conc: 3.80 ug/ml

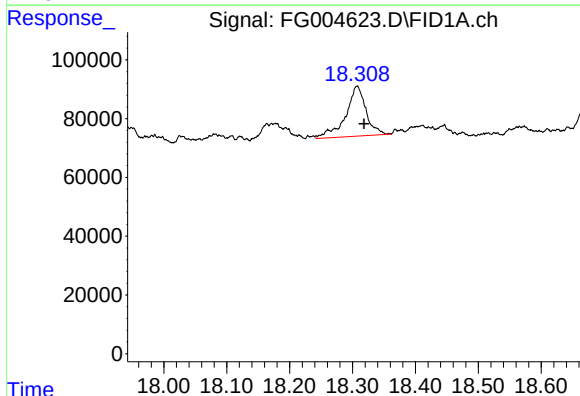


#14 N-DOTRIACONTANE

R.T.: 18.307 min
Delta R.T.: -0.011 min
Response: 380923
Conc: 3.25 ug/ml

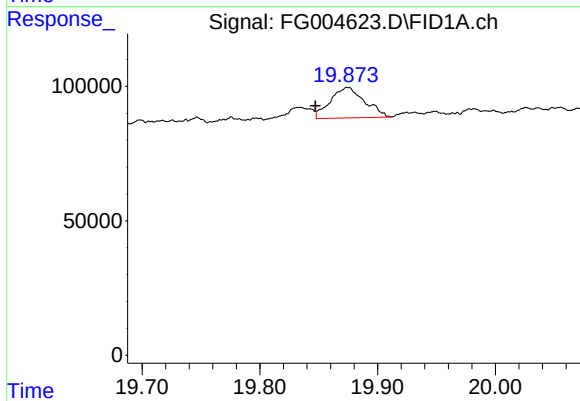

#16 N-HEXATRIACONTANE

R.T.: 19.875 min
Delta R.T.: 0.028 min
Response: 229304
Conc: 2.06 ug/ml

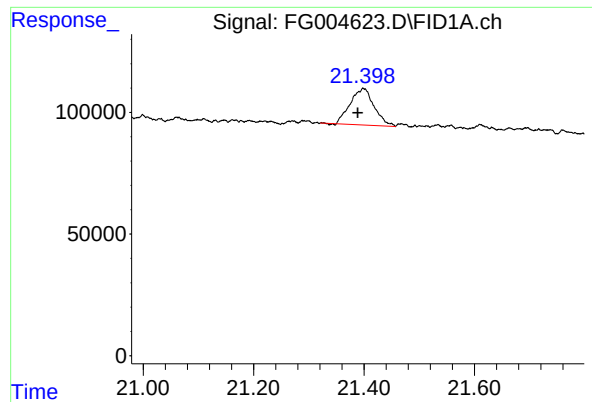

#18 N-TETRACONTANE

R.T.: 21.399 min
Delta R.T.: 0.010 min
Response: 449094
Conc: 4.15 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-2-DEEP