

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
 Data File : FG004625.D
 Signal(s) : FID1A.ch
 Acq On : 09 Apr 2019 17:35
 Operator : AJ\SJ
 Sample : K2338-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 TP-3-SHALLOW

Integration File: autoint1.e
 Quant Time: Apr 10 00:44:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.410	1643732	15.936 ug/ml
Target Compounds			
4) N-TETRADECANE	8.026f	377142	3.481 ug/ml
11) N-HEXACOSANE	15.633	150640	1.314 ug/ml
12) N-OCTACOSANE	16.584	485848	4.200 ug/ml
13) N-TRIACONTANE	17.472	551922	4.652 ug/ml
14) N-DOTRIACONTANE	18.306	357931	3.052 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
Data File : FG004625.D
Signal(s) : FID1A.ch
Acq On : 09 Apr 2019 17:35
Operator : AJ\SJ
Sample : K2338-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-3-SHALLOW

Integration File: autoint1.e
Quant Time: Apr 10 00:44:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

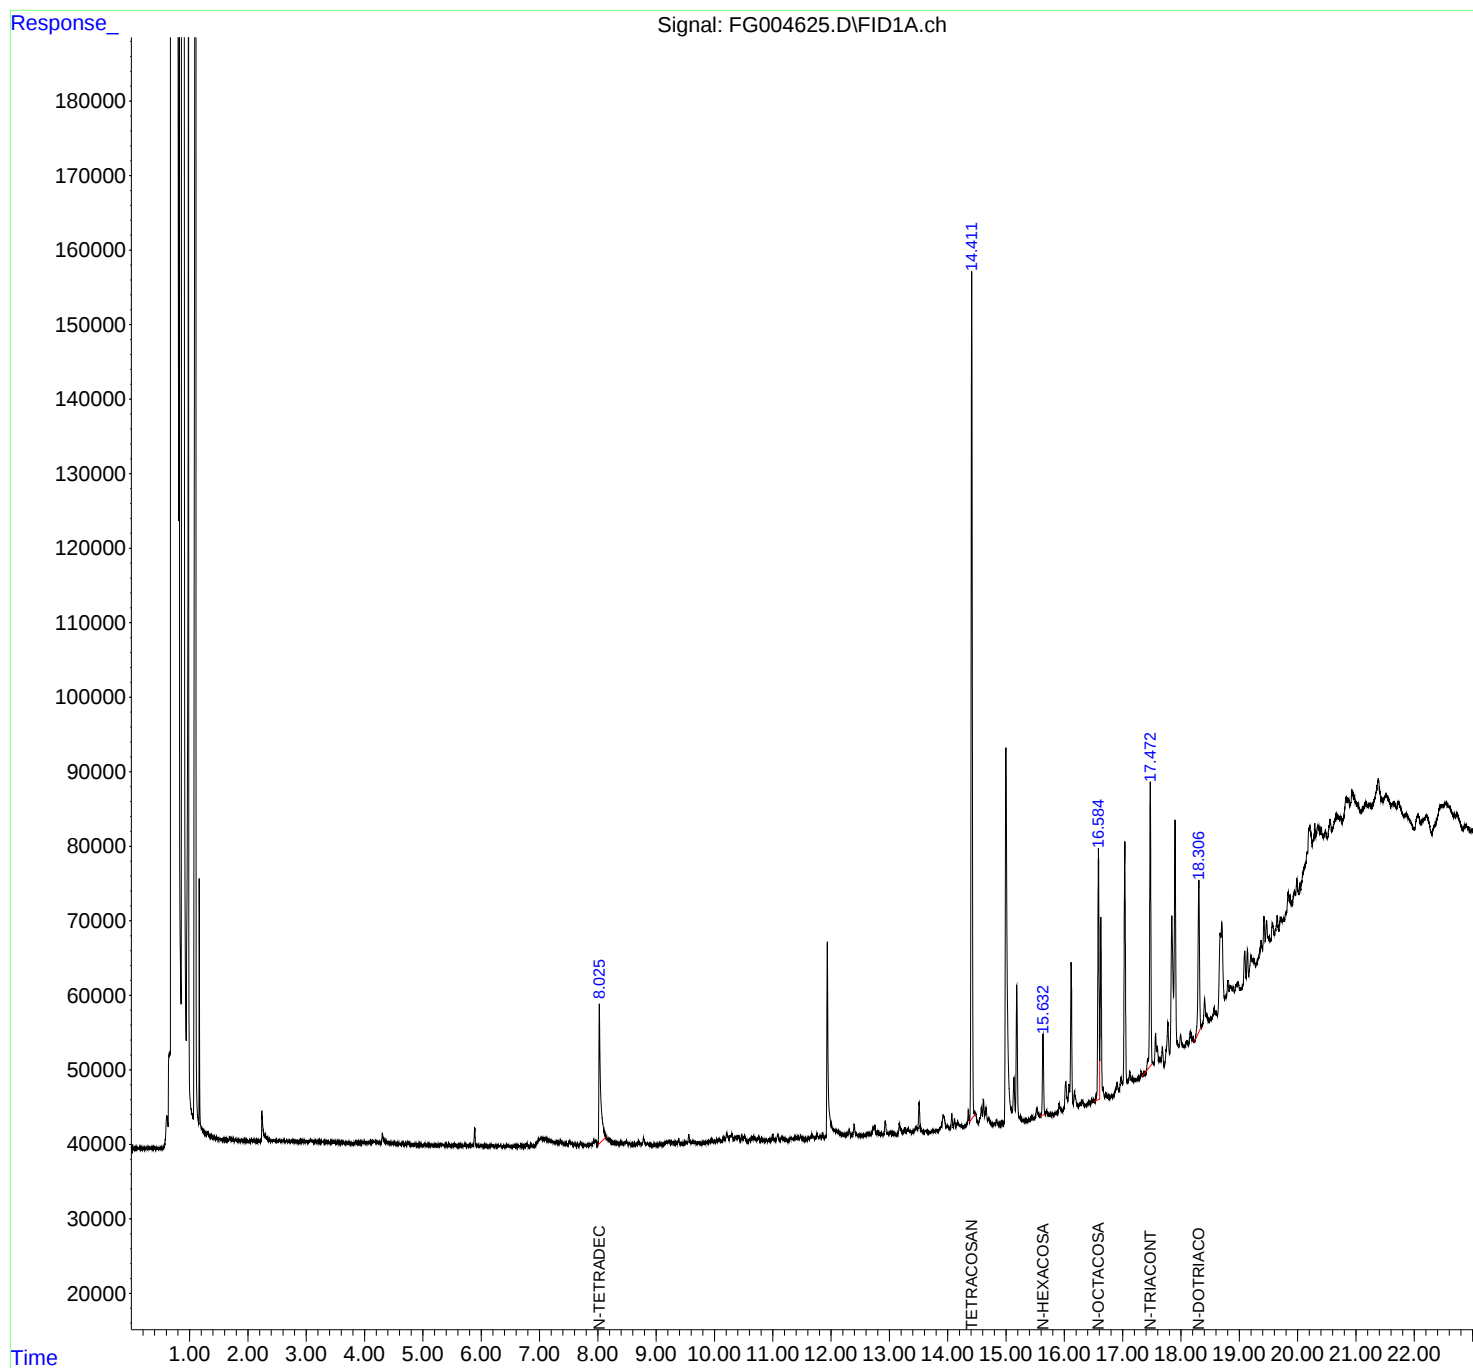


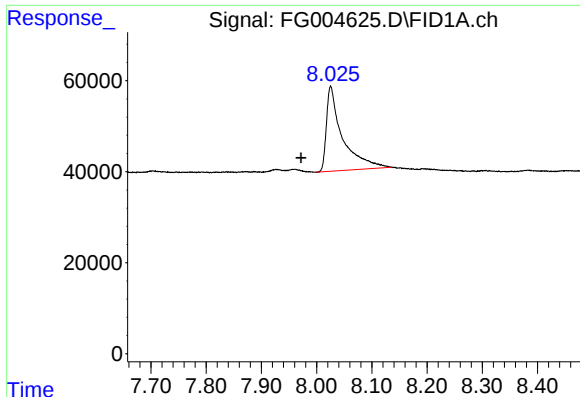

#4 N-TETRADECANE


R.T.: 8.026 min
Delta R.T.: 0.054 min
Response: 377142
Conc: 3.48 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-3-SHALLOW

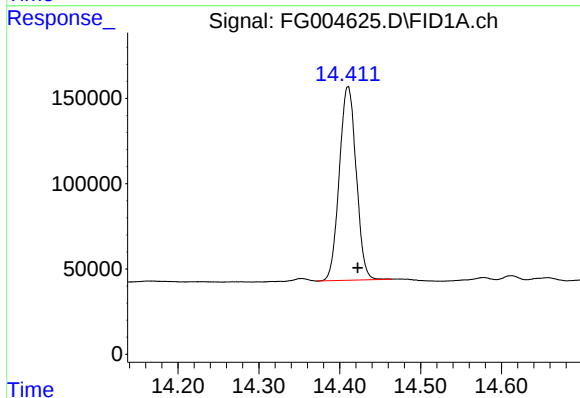


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.410 min
Delta R.T.: -0.012 min
Response: 1643732
Conc: 15.94 ug/ml

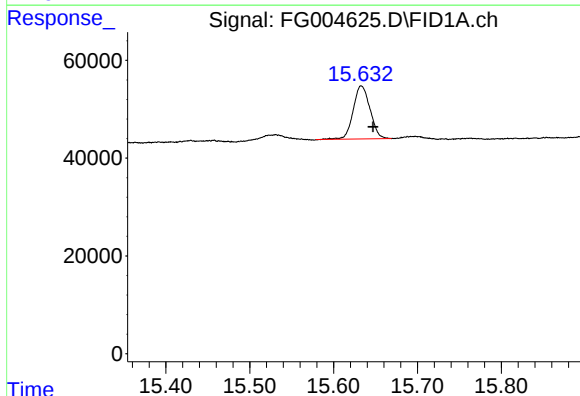


#11 N-HEXACOSANE

R.T.: 15.633 min
Delta R.T.: -0.014 min
Response: 150640
Conc: 1.31 ug/ml

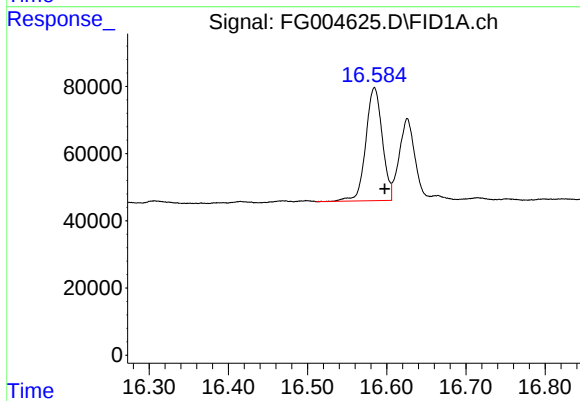

#12 N-OCTACOSANE


R.T.: 16.584 min
Delta R.T.: -0.013 min
Response: 485848
Conc: 4.20 ug/ml

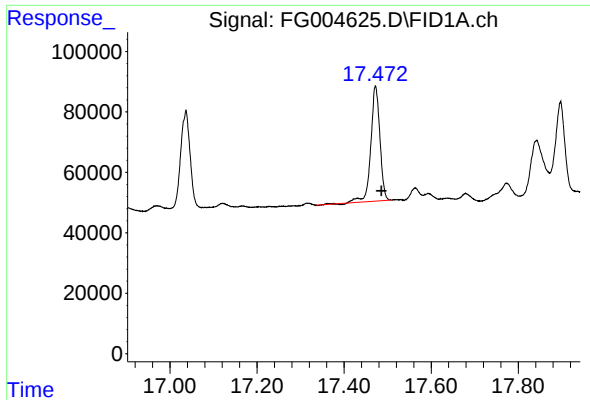

#13 N-TRIACONTANE

R.T.: 17.472 min
Delta R.T.: -0.014 min
Response: 551922
Conc: 4.65 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-3-SHALLOW

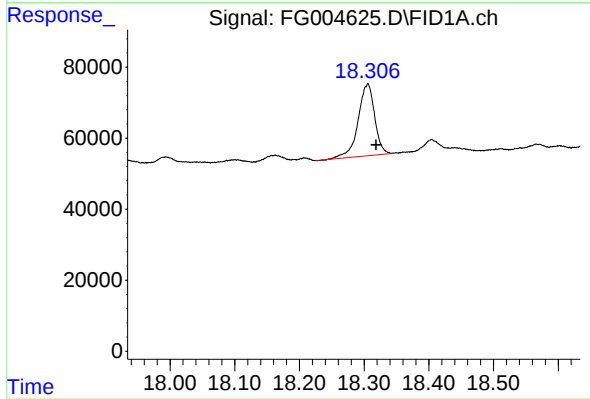

#14 N-DOTRIACONTANE

R.T.: 18.306 min
Delta R.T.: -0.013 min
Response: 357931
Conc: 3.05 ug/ml