

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
 Data File : FG004626.D
 Signal(s) : FID1A.ch
 Acq On : 09 Apr 2019 18:06
 Operator : AJ\SJ
 Sample : K2338-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 TP-3-SHALLOW

Integration File: autoint1.e
 Quant Time: Apr 10 00:44:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.409	1613716	15.645 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.027f	383194	3.537 ug/ml
11)	N-HEXACOSANE	15.634	151062	1.318 ug/ml
12)	N-OCTACOSANE	16.585	466530	4.033 ug/ml
13)	N-TRIACONTANE	17.473	556383	4.690 ug/ml
14)	N-DOTRIACONTANE	18.307	375007	3.198 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
Data File : FG004626.D
Signal(s) : FID1A.ch
Acq On : 09 Apr 2019 18:06
Operator : AJ\SJ
Sample : K2338-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-3-SHALLOW

Integration File: autoint1.e
Quant Time: Apr 10 00:44:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

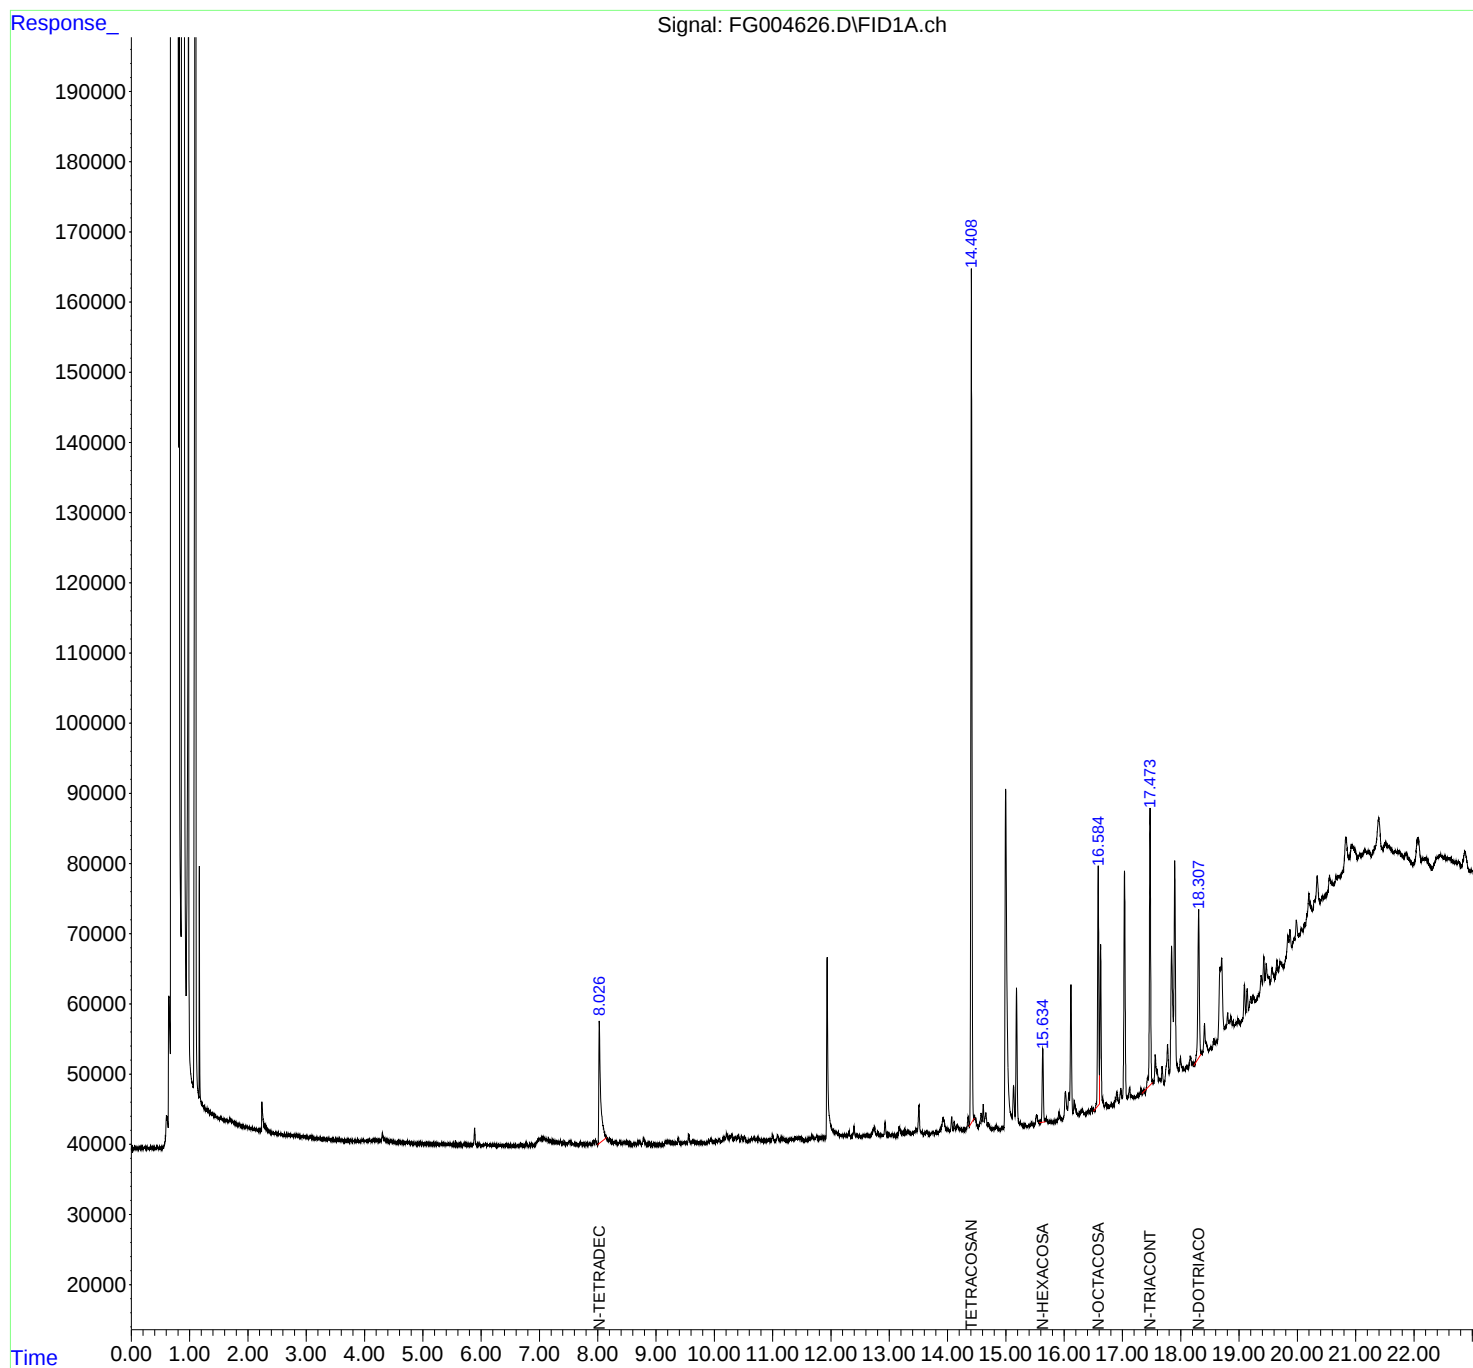


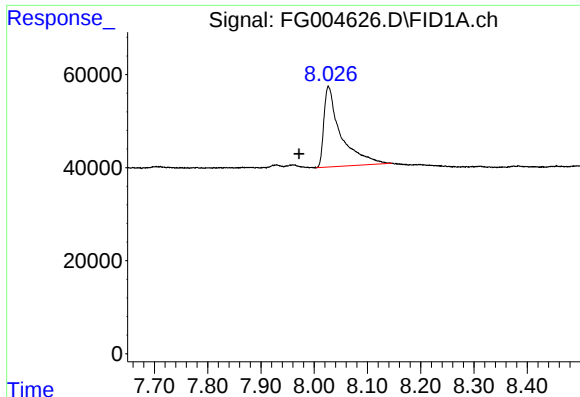

#4 N-TETRADECANE


R.T.: 8.027 min
Delta R.T.: 0.055 min
Response: 383194
Conc: 3.54 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-3-SHALLOW

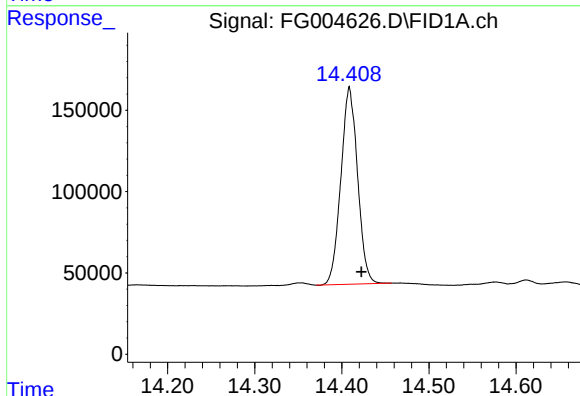


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.409 min
Delta R.T.: -0.014 min
Response: 1613716
Conc: 15.64 ug/ml

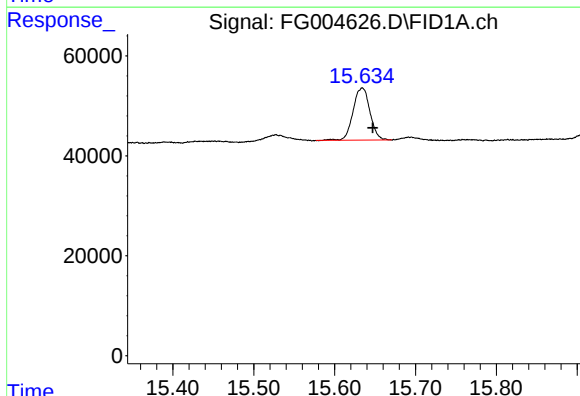


#11 N-HEXACOSANE

R.T.: 15.634 min
Delta R.T.: -0.013 min
Response: 151062
Conc: 1.32 ug/ml

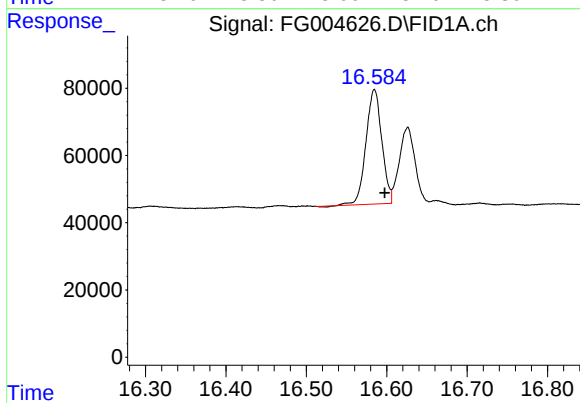

#12 N-OCTACOSANE


R.T.: 16.585 min
Delta R.T.: -0.013 min
Response: 466530
Conc: 4.03 ug/ml

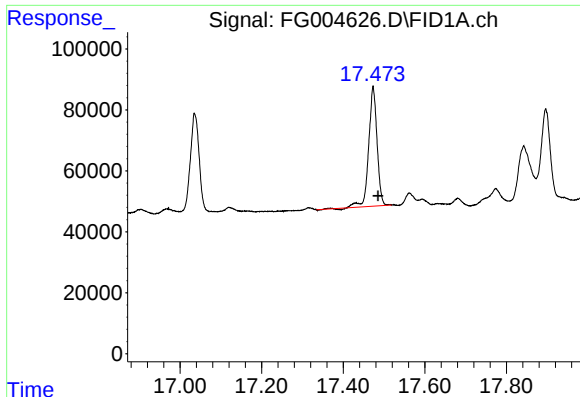

#13 N-TRIACONTANE

R.T.: 17.473 min
Delta R.T.: -0.013 min
Response: 556383
Conc: 4.69 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-3-SHALLOW

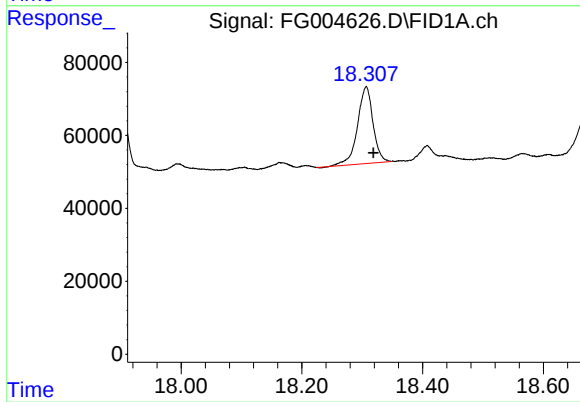

#14 N-DOTRIACONTANE

R.T.: 18.307 min
Delta R.T.: -0.012 min
Response: 375007
Conc: 3.20 ug/ml