

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
 Data File : FG004628.D
 Signal(s) : FID1A.ch
 Acq On : 09 Apr 2019 19:08
 Operator : AJ\SJ
 Sample : K2199-05 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 OR-03-040819-A

Integration File: autoint1.e
 Quant Time: Apr 10 00:45:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.409	124825	1.210 ug/ml
Target Compounds			
7) N-EICOSANE	12.287	139925	1.224 ug/ml
8) N-DOCOSANE	13.535	331160	2.897 ug/ml
10) N-TETRACOSANE	14.595	1469360	12.720 ug/ml
12) N-OCTACOSANE	16.583	108441	0.937 ug/ml
13) N-TRIACONTANE	17.474	116877	0.985 ug/ml
14) N-DOTRIACONTANE	18.309	241894	2.063 ug/ml
16) N-HEXATRIACONTANE	19.878	210206	1.886 ug/ml
18) N-TETRACONTANE	21.386	319903	2.957 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
Data File : FG004628.D
Signal(s) : FID1A.ch
Acq On : 09 Apr 2019 19:08
Operator : AJ\SJ
Sample : K2199-05 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OR-03-040819-A

Integration File: autoint1.e
Quant Time: Apr 10 00:45:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

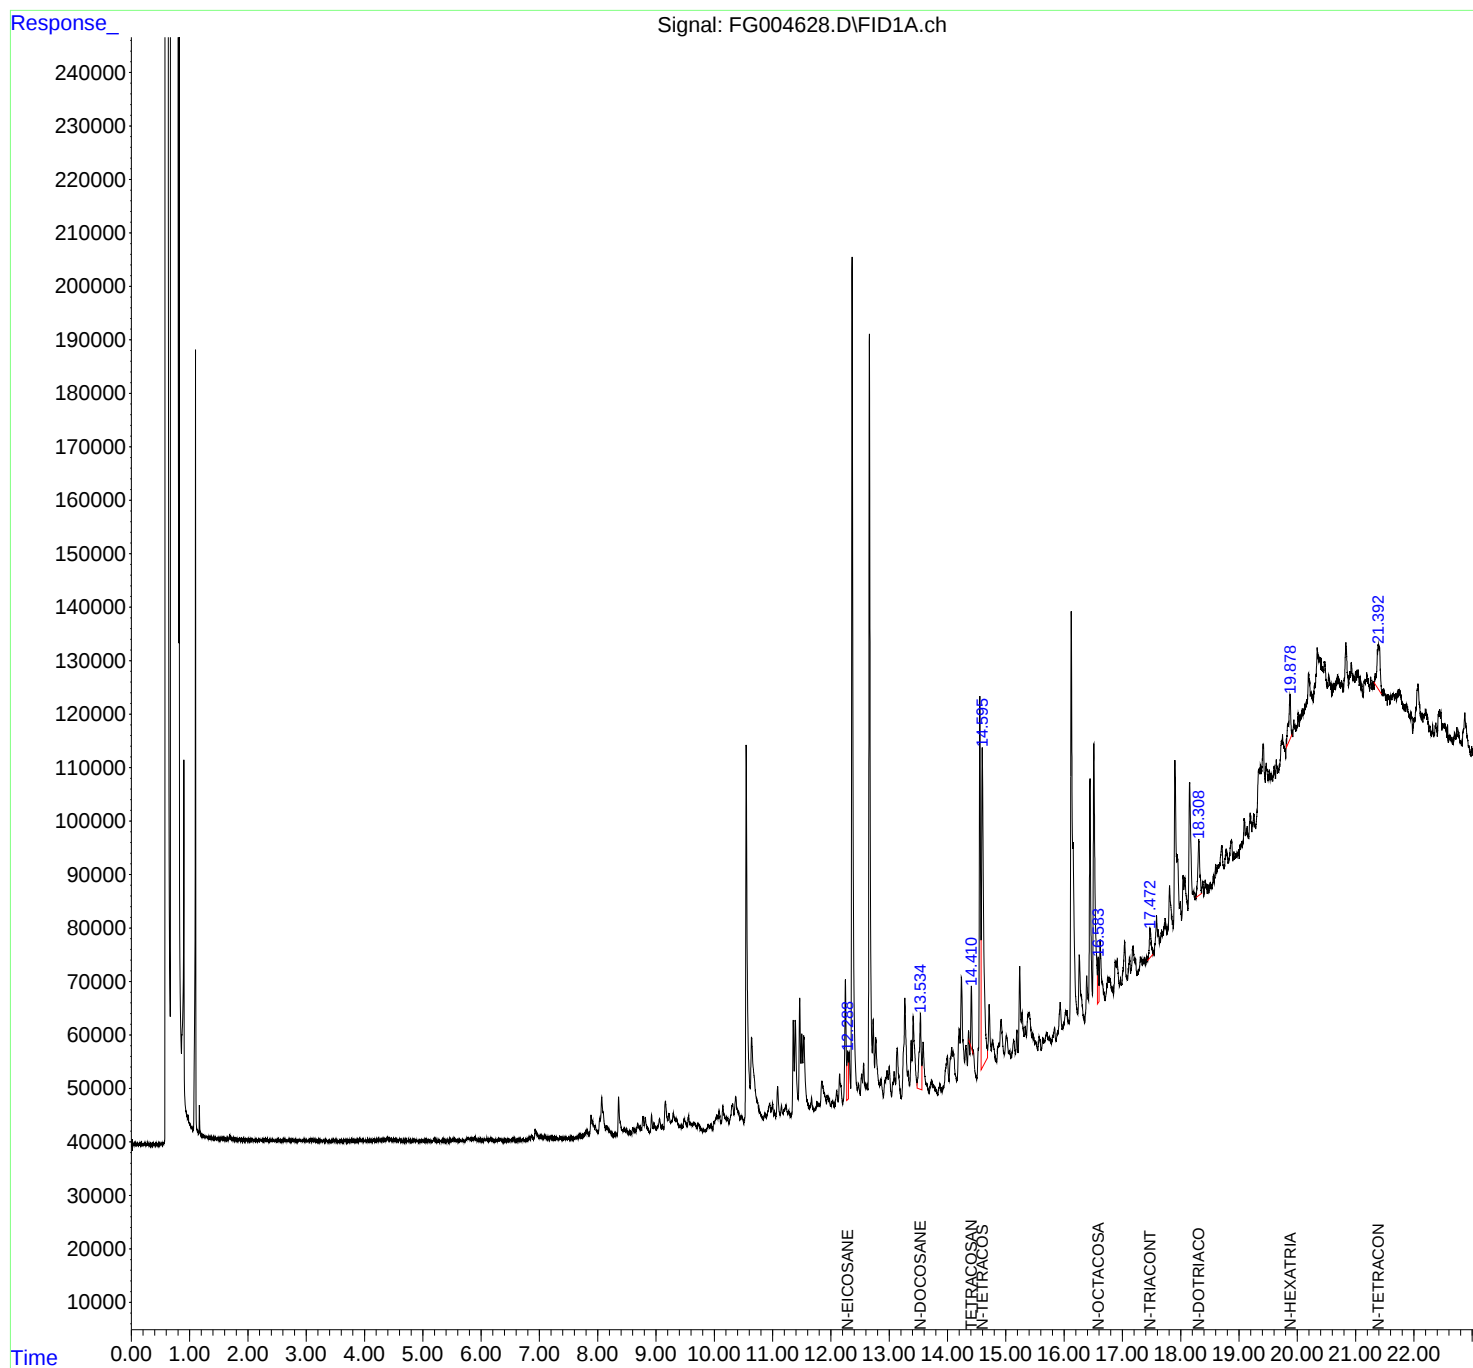


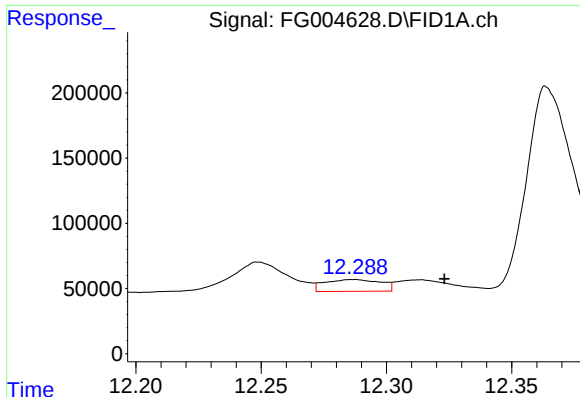

#7 N-EICOSANE


R.T.: 12.287 min
Delta R.T.: -0.036 min
Response: 139925
Conc: 1.22 ug/ml

Instrument :
FID_G
ClientSampleId :
OR-03-040819-A

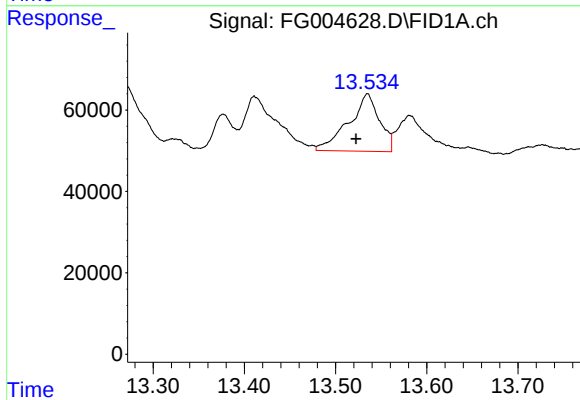


#8 N-DOCOSANE

R.T.: 13.535 min
Delta R.T.: 0.013 min
Response: 331160
Conc: 2.90 ug/ml

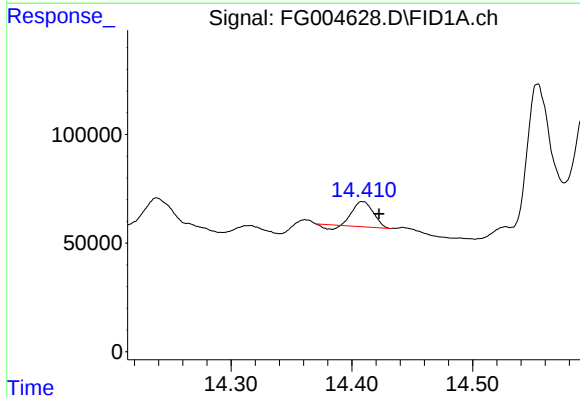


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.409 min
Delta R.T.: -0.013 min
Response: 124825
Conc: 1.21 ug/ml

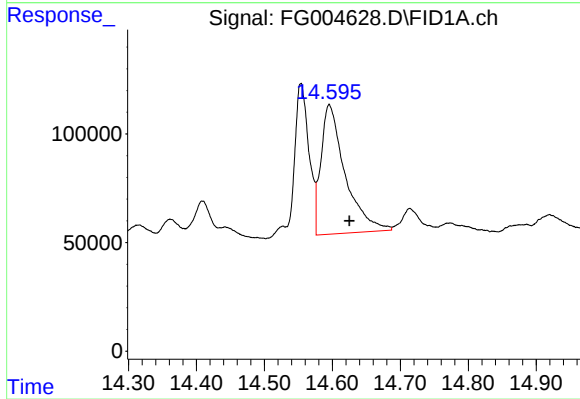

#10 N-TETRACOSANE


R.T.: 14.595 min
Delta R.T.: -0.030 min
Response: 1469360
Conc: 12.72 ug/ml

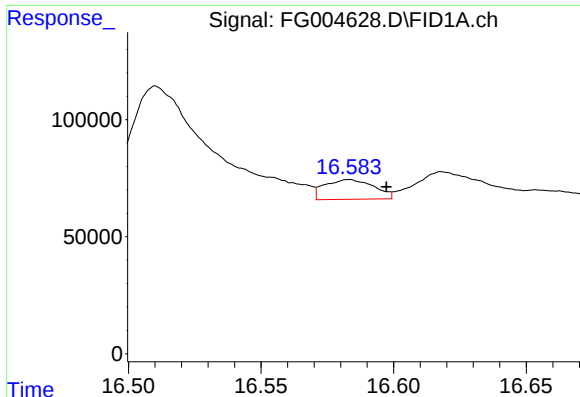

#12 N-OCTACOSANE


R.T.: 16.583 min
Delta R.T.: -0.014 min
Response: 108441
Conc: 0.94 ug/ml

Instrument :
FID_G
ClientSampleId :
OR-03-040819-A

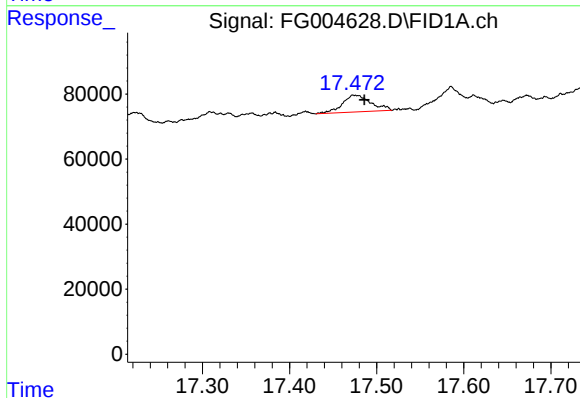


#13 N-TRIACONTANE

R.T.: 17.474 min
Delta R.T.: -0.012 min
Response: 116877
Conc: 0.99 ug/ml

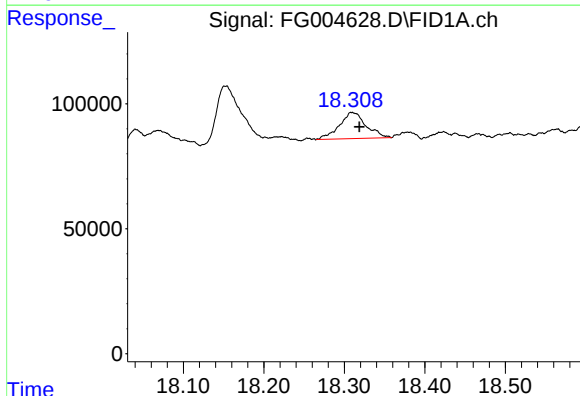


#14 N-DOTRIACONTANE

R.T.: 18.309 min
Delta R.T.: -0.009 min
Response: 241894
Conc: 2.06 ug/ml

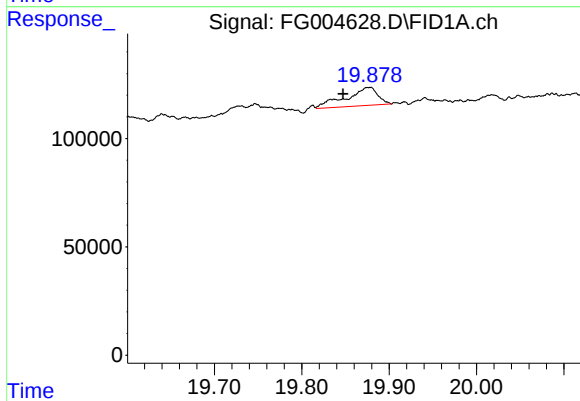

#16 N-HEXATRIACONTANE

R.T.: 19.878 min
Delta R.T.: 0.031 min
Response: 210206
Conc: 1.89 ug/ml

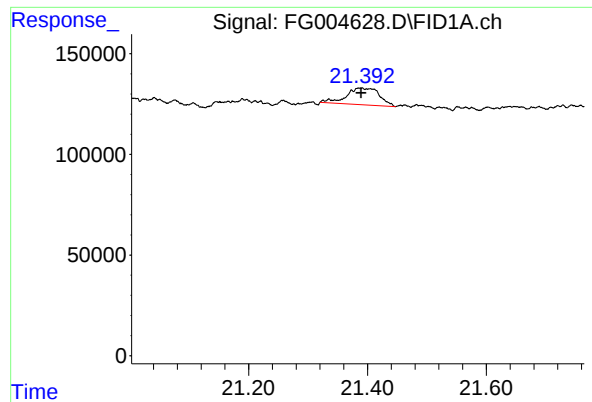

#18 N-TETRACONTANE

R.T.: 21.386 min
Delta R.T.: -0.003 min
Response: 319903
Conc: 2.96 ug/ml

Instrument :
FID_G
ClientSampleId :
OR-03-040819-A