

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
Data File : FG004625.D
Signal(s) : FID1A.ch
Acq On : 09 Apr 2019 17:35
Operator : AJ\SJ
Sample : K2338-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-3-SHALLOW

Integration File: autoint1.e
Quant Time: Apr 10 00:44:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.410	1643732	15.936 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040919\
Data File : FG004625.D
Signal(s) : FID1A.ch
Acq On : 09 Apr 2019 17:35
Operator : AJ\SJ
Sample : K2338-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-3-SHALLOW

Integration File: autoint1.e
Quant Time: Apr 10 00:44:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rx1-1ms
Signal Info : 20mx0.18mmx0.18um

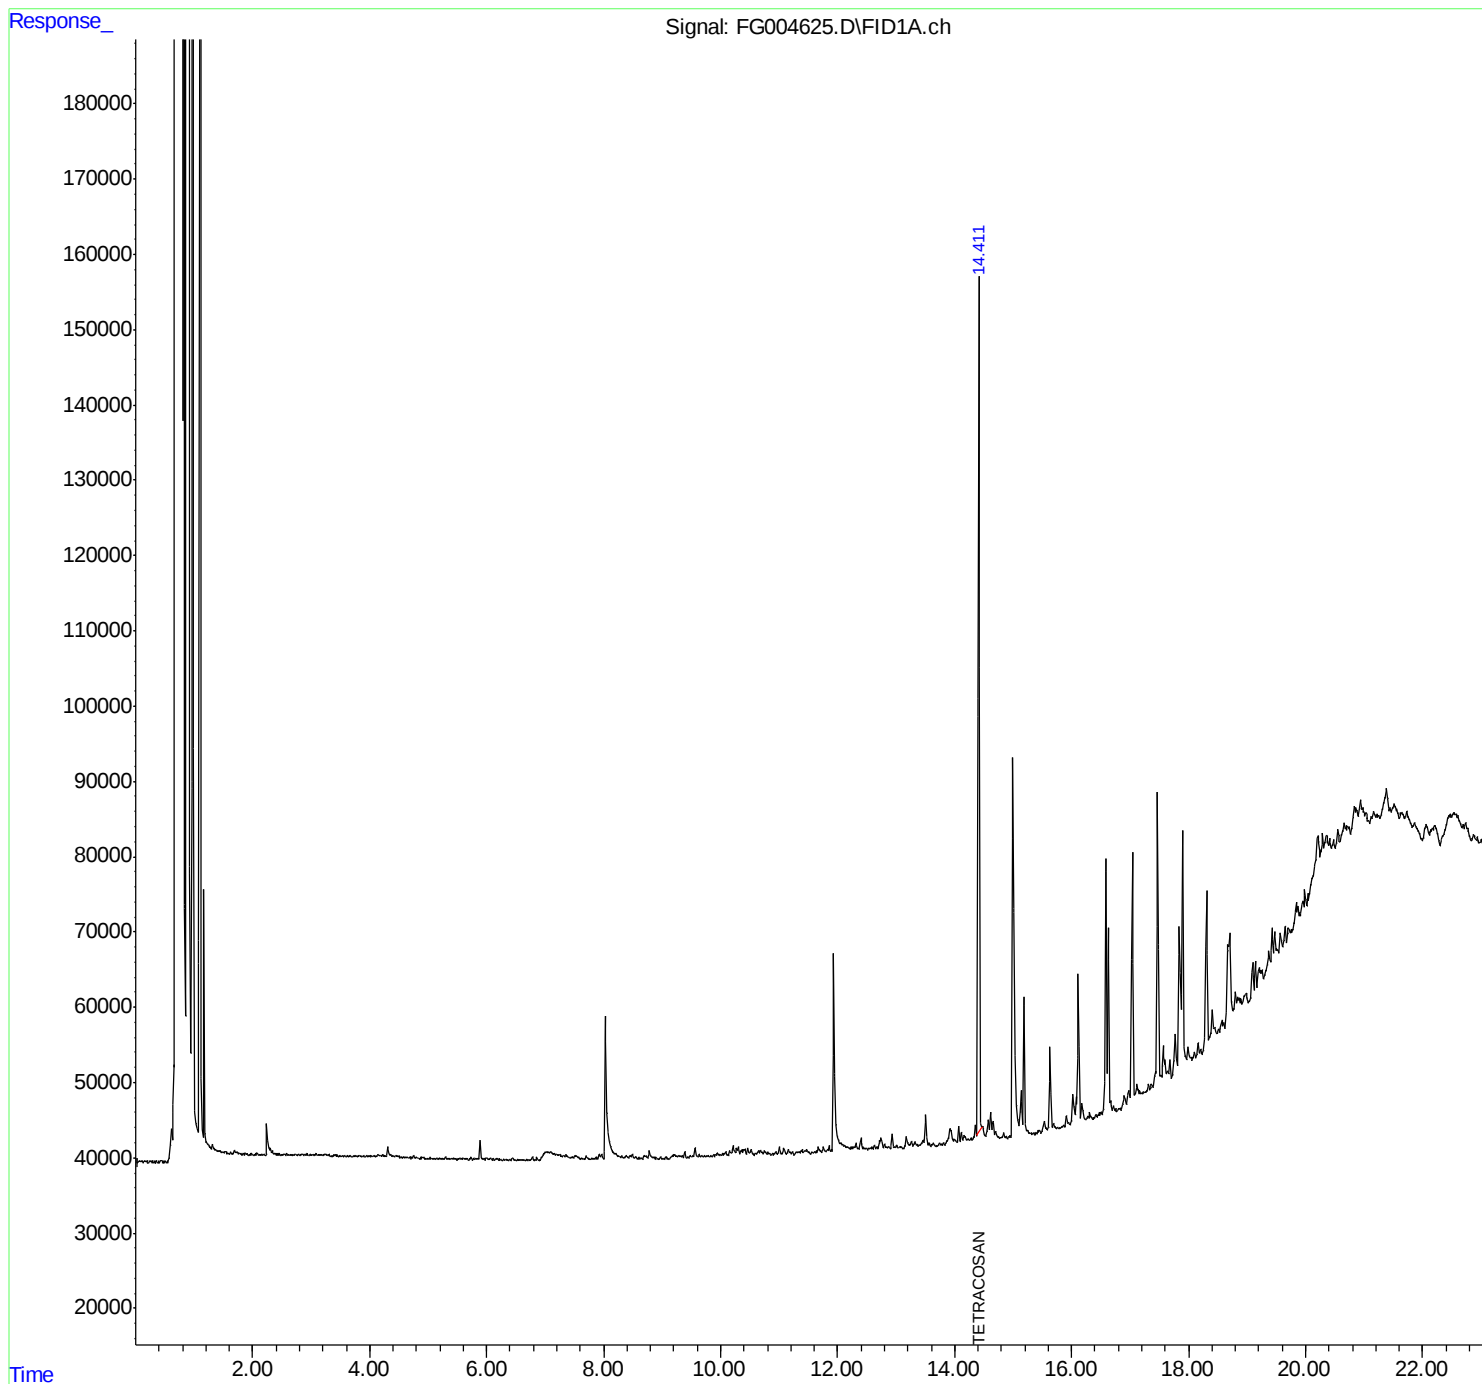

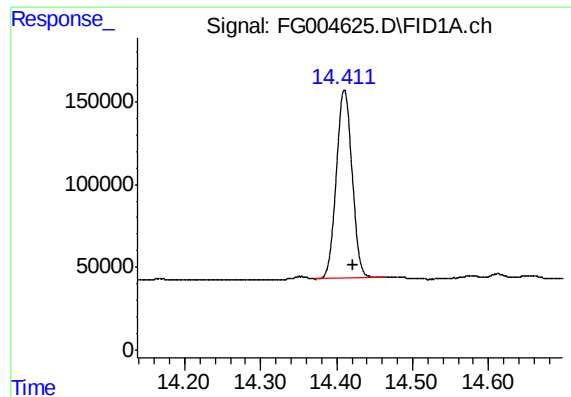

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.410 min
Delta R.T.: -0.012 min
Response: 1643732
Conc: 15.94 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-3-SHALLOW