

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041019\
 Data File : FG004648.D
 Signal(s) : FID1A.ch
 Acq On : 10 Apr 2019 16:16
 Operator : AJ\SJ
 Sample : K2200-05 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 11 01:31:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.408	337552	3.273 ug/ml
Target Compounds			
3) N-DODECANE	6.166	106717	1.013 ug/ml
4) N-TETRADECANE	7.957	521935	4.817 ug/ml
5) N-HEXADECANE	9.557	667292	5.964 ug/ml
6) N-OCTADECANE	10.999	703477	6.202 ug/ml
7) N-EICOSANE	12.309	689861	6.035 ug/ml
8) N-DOCOSANE	13.509	490118	4.288 ug/ml
10) N-TETRACOSANE	14.598	2239272	19.385 ug/ml
11) N-HEXACOSANE	15.635	290730	2.536 ug/ml
12) N-OCTACOSANE	16.586	434766	3.758 ug/ml
13) N-TRIACONTANE	17.478	582951	4.914 ug/ml
14) N-DOTRIACONTANE	18.306	951120	8.111 ug/ml
15) N-TETRATRIACONTANE	19.096	708255	6.357 ug/ml
16) N-HEXATRIACONTANE	19.842	637398	5.718 ug/ml
17) N-OCTATRIACONTANE	20.544	358184	3.604 ug/ml
18) N-TETRACONTANE	21.377	699068	6.463 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041019\
Data File : FG004648.D
Signal(s) : FID1A.ch
Acq On : 10 Apr 2019 16:16
Operator : AJ\SJ
Sample : K2200-05 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 11 01:31:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

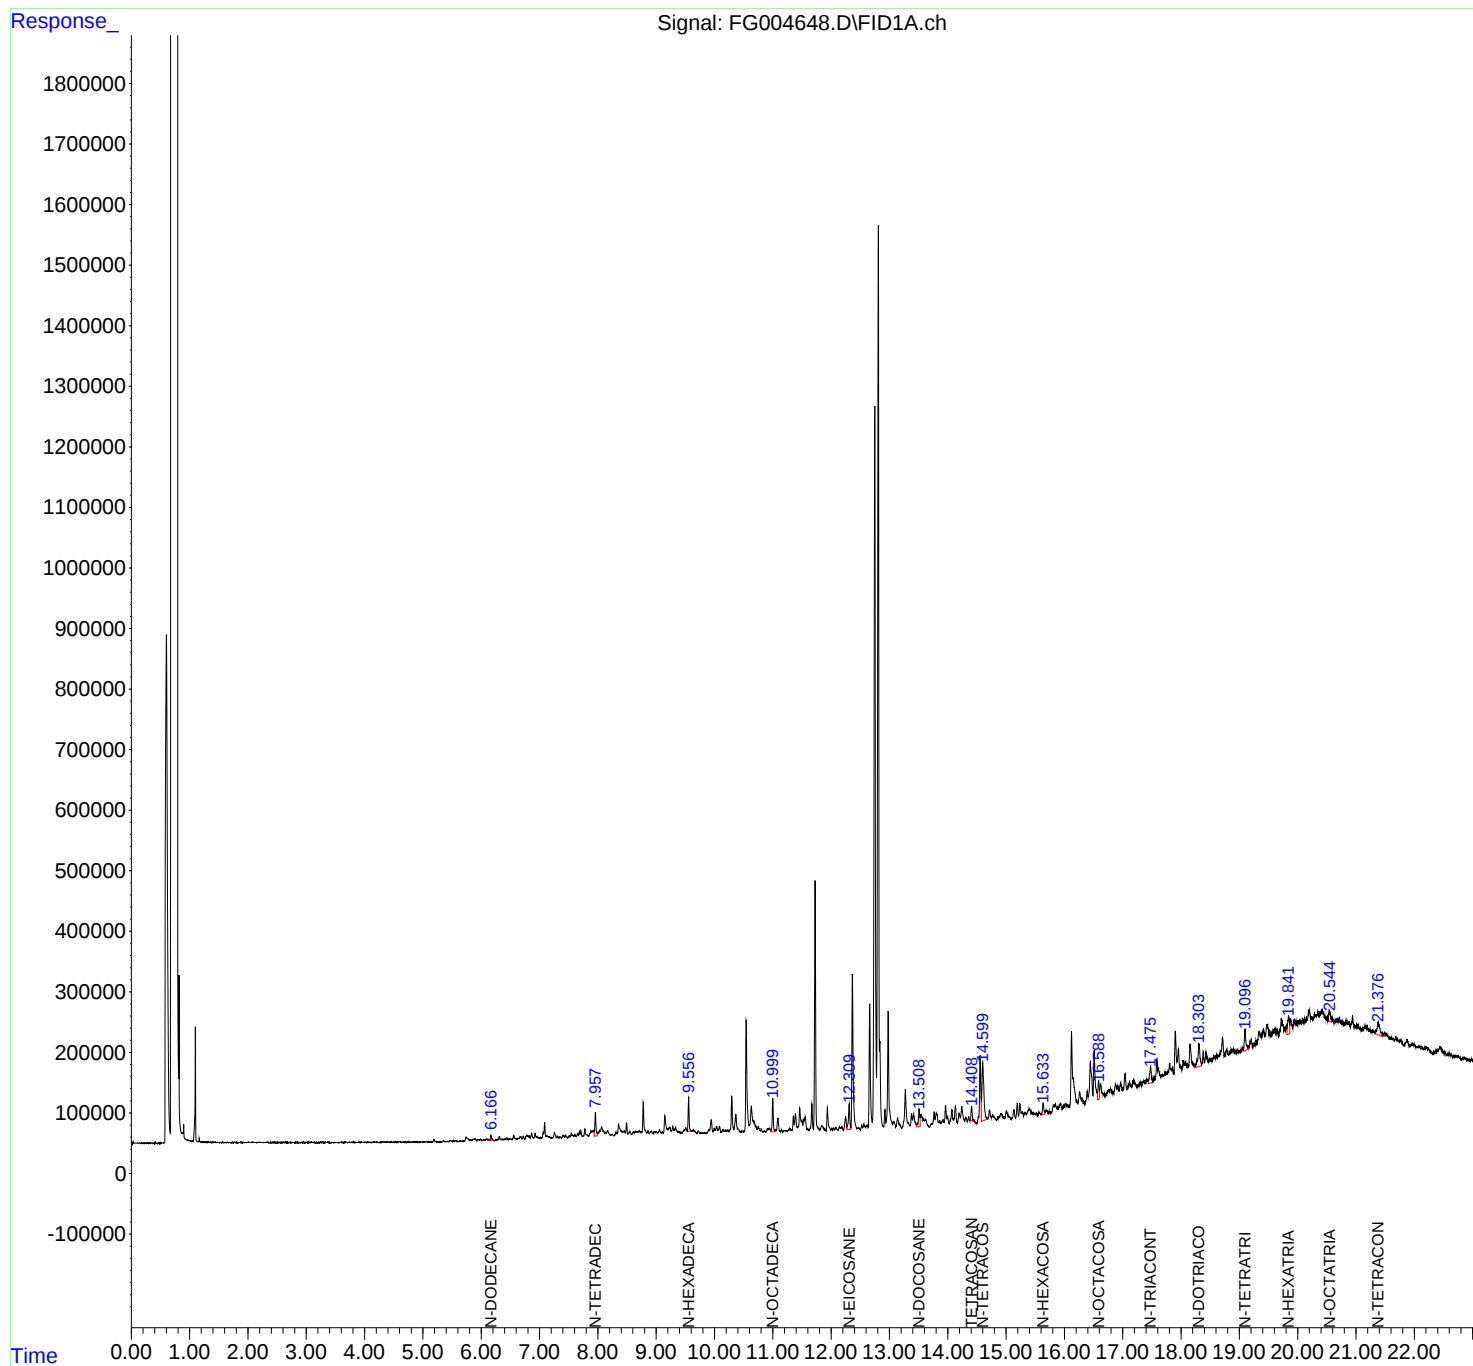

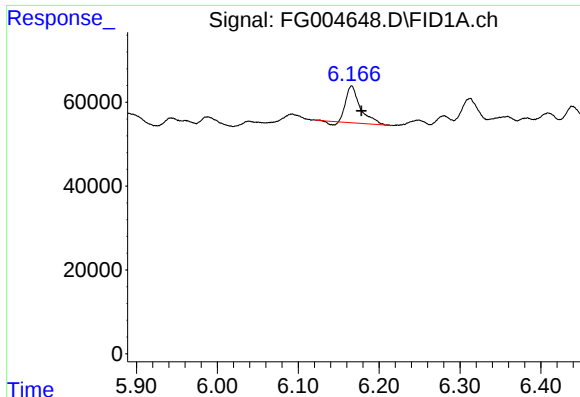


#3 N-DODECANE

R.T.: 6.166 min
Delta R.T.: -0.012 min
Response: 106717
Conc: 1.01 ug/ml

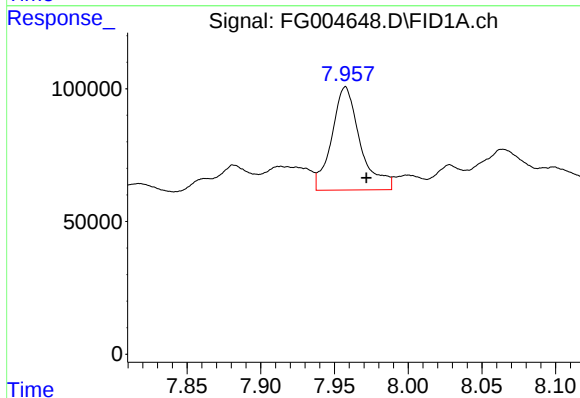


#4 N-TETRADECANE

R.T.: 7.957 min
Delta R.T.: -0.014 min
Response: 521935
Conc: 4.82 ug/ml

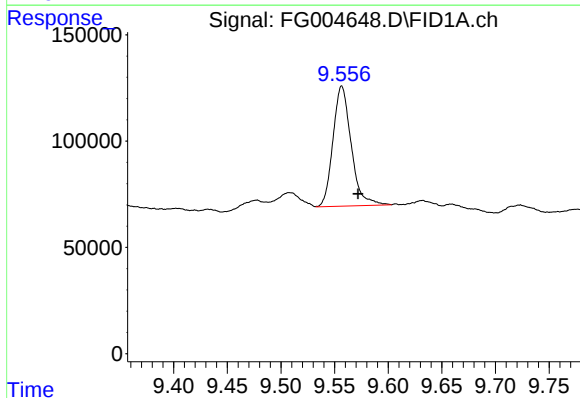


#5 N-HEXADECANE

R.T.: 9.557 min
Delta R.T.: -0.015 min
Response: 667292
Conc: 5.96 ug/ml

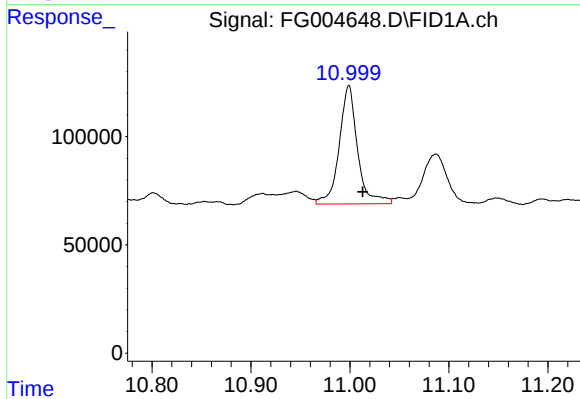


#6 N-OCTADECANE

R.T.: 10.999 min
Delta R.T.: -0.014 min
Response: 703477
Conc: 6.20 ug/ml

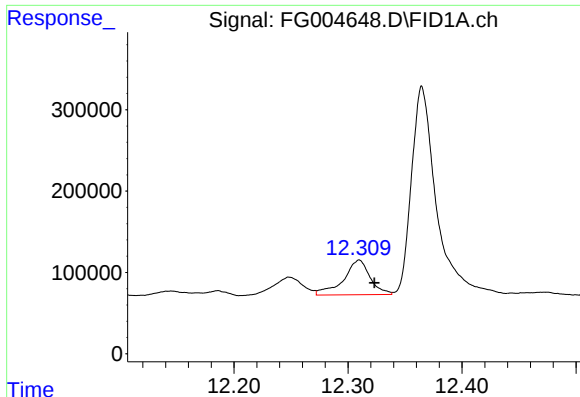


#7 N-EICOSANE

R.T.: 12.309 min
Delta R.T.: -0.014 min
Response: 689861
Conc: 6.03 ug/ml

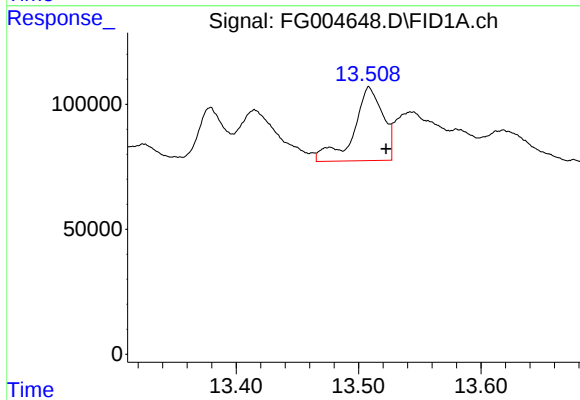


#8 N-DOCOSANE

R.T.: 13.509 min
Delta R.T.: -0.014 min
Response: 490118
Conc: 4.29 ug/ml

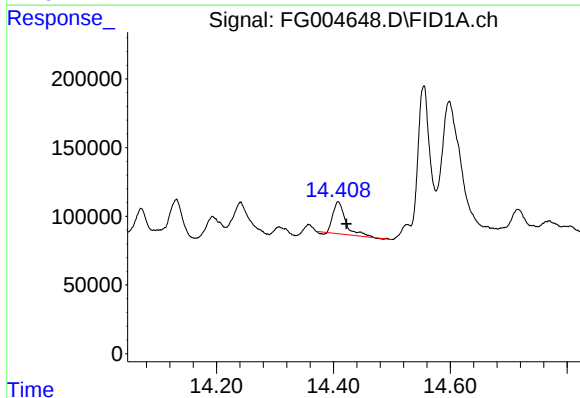


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.408 min
Delta R.T.: -0.014 min
Response: 337552
Conc: 3.27 ug/ml

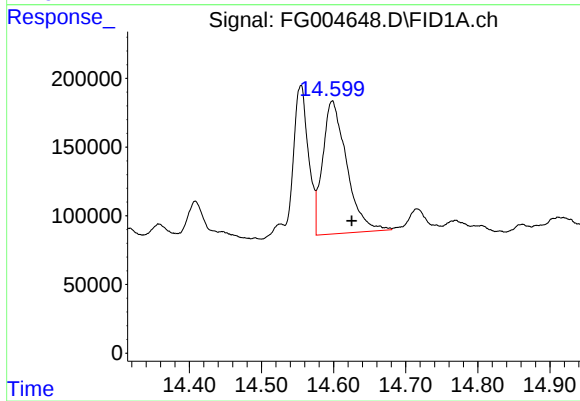


#10 N-TETRACOSANE

R.T.: 14.598 min
Delta R.T.: -0.027 min
Response: 2239272
Conc: 19.38 ug/ml

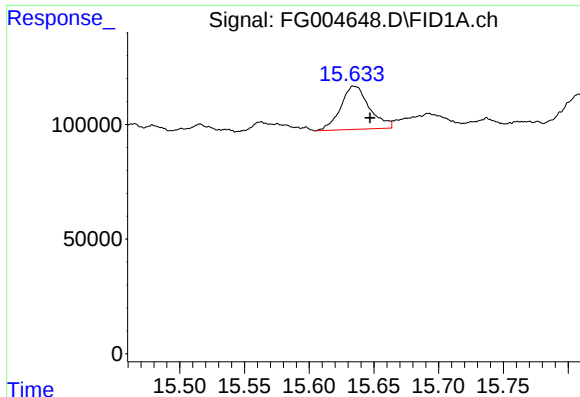


#11 N-HEXACOSANE

R.T.: 15.635 min
Delta R.T.: -0.012 min
Response: 290730
Conc: 2.54 ug/ml

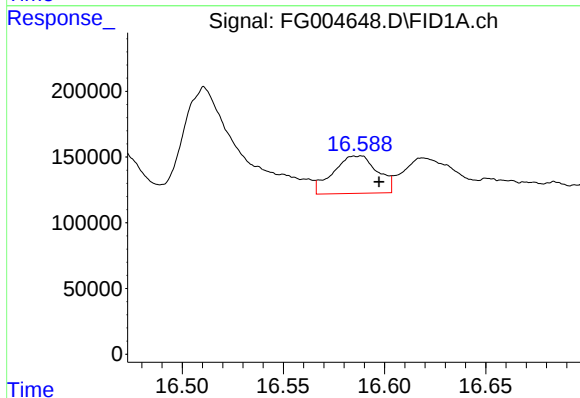


#12 N-OCTACOSANE

R.T.: 16.586 min
Delta R.T.: -0.011 min
Response: 434766
Conc: 3.76 ug/ml

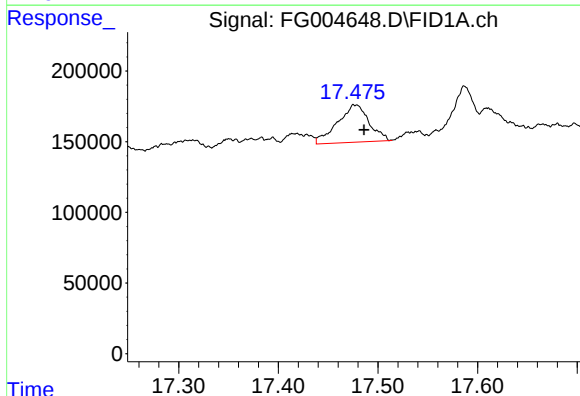


#13 N-TRIACONTANE

R.T.: 17.478 min
Delta R.T.: -0.008 min
Response: 582951
Conc: 4.91 ug/ml

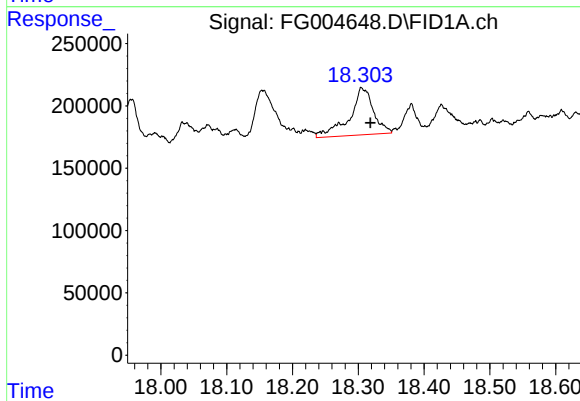

#14 N-DOTRIACONTANE

R.T.: 18.306 min
Delta R.T.: -0.012 min
Response: 951120
Conc: 8.11 ug/ml

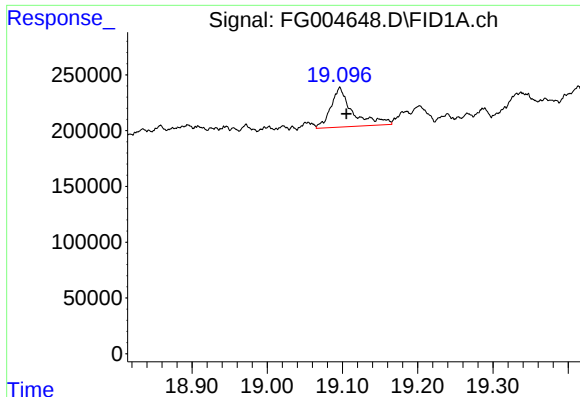


#15 N-TETRATRIACONTANE

R.T.: 19.096 min

Delta R.T.: -0.009 min

Response: 708255

Conc: 6.36 ug/ml

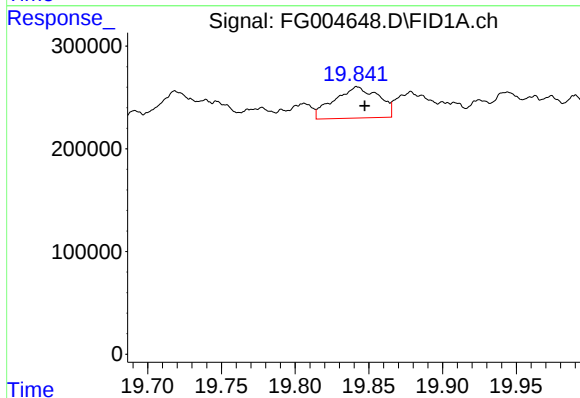


#16 N-HEXATRIACONTANE

R.T.: 19.842 min

Delta R.T.: -0.005 min

Response: 637398

Conc: 5.72 ug/ml

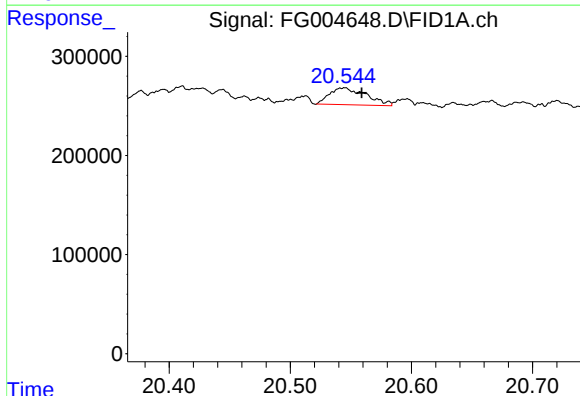


#17 N-OCTATRIACONTANE

R.T.: 20.544 min

Delta R.T.: -0.015 min

Response: 358184

Conc: 3.60 ug/ml

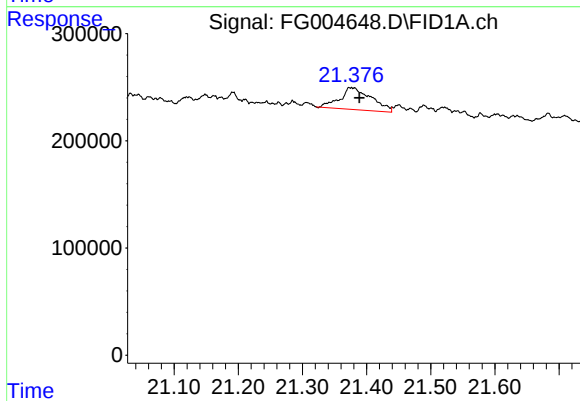

#18 N-TETRACONTANE

R.T.: 21.377 min

Delta R.T.: -0.012 min

Response: 699068

Conc: 6.46 ug/ml