

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041122\
Data File : FG009575.D
Signal(s) : FID1A.ch
Acq On : 11 Apr 2022 12:15
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 11 13:24:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.355	3372086	22.374 ug/ml
12)	N-OCTACOSANE	16.820	2837564	21.742 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041122\
Data File : FG009575.D
Signal(s) : FID1A.ch
Acq On : 11 Apr 2022 12:15
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 11 13:24:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

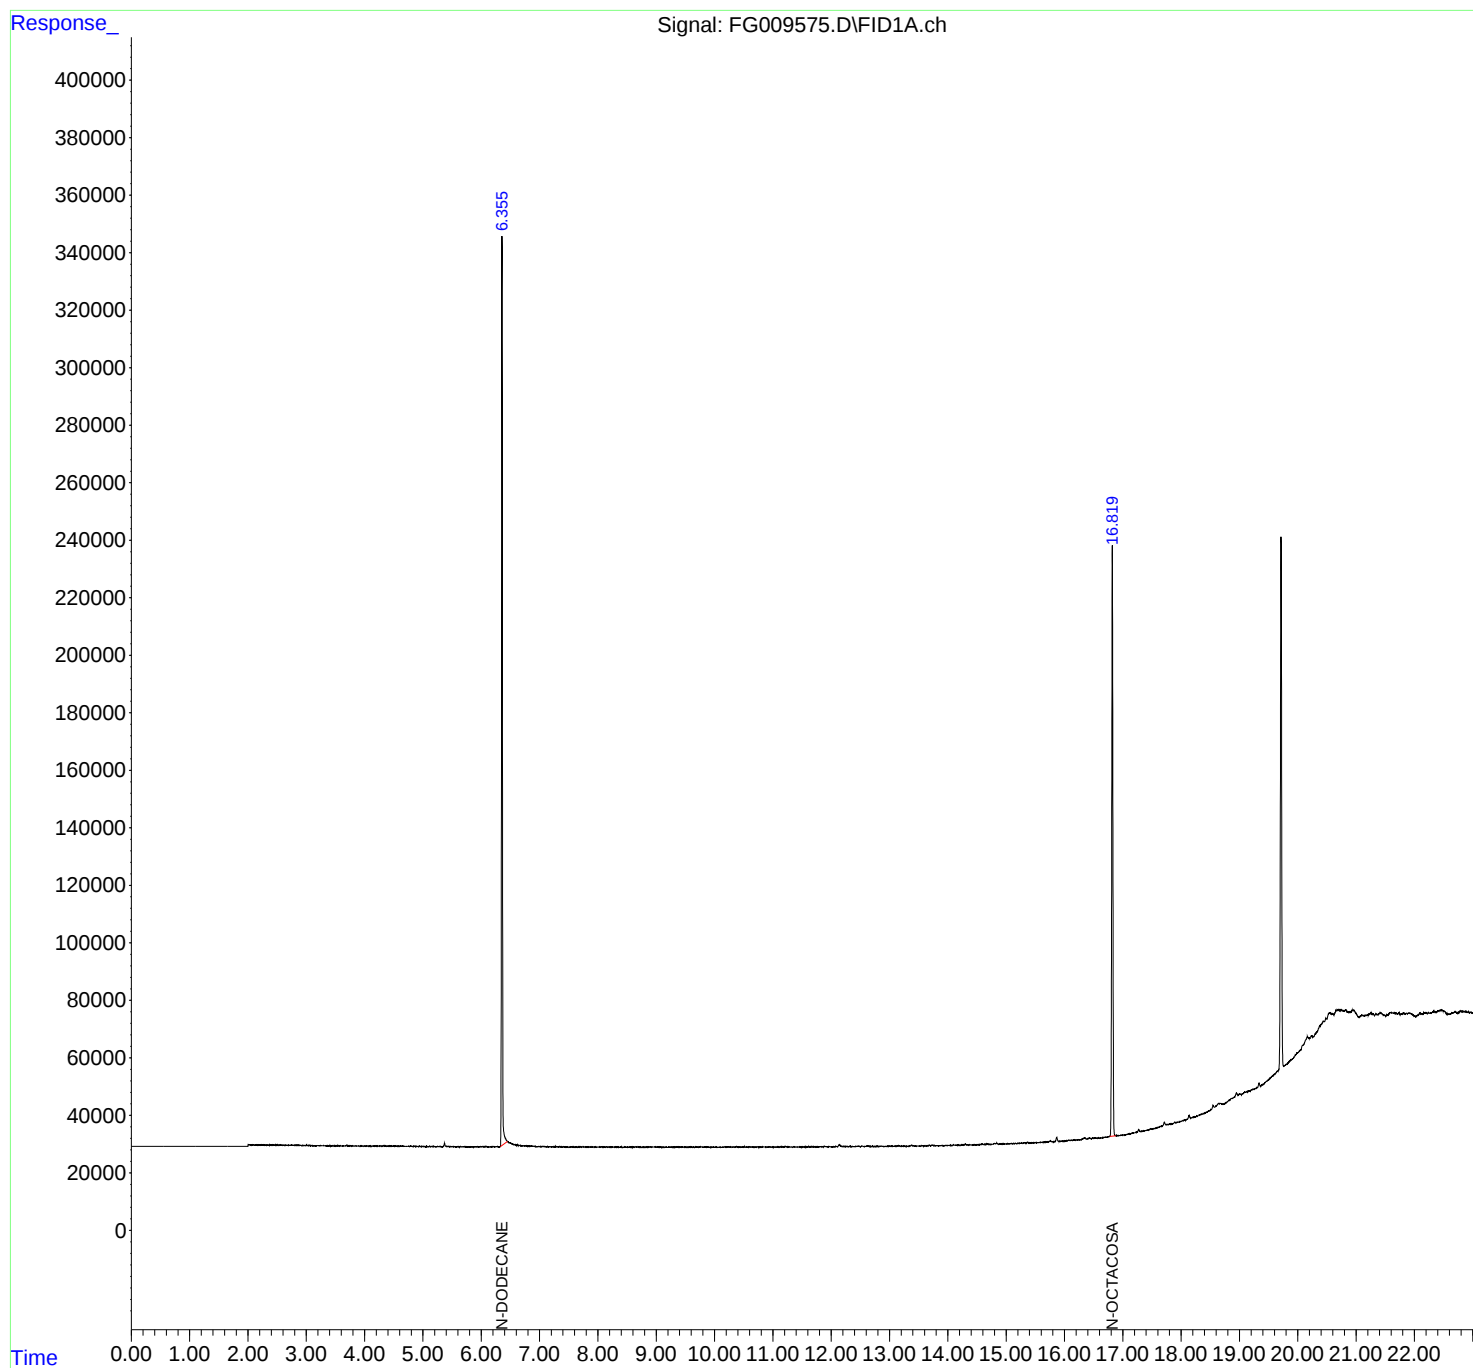


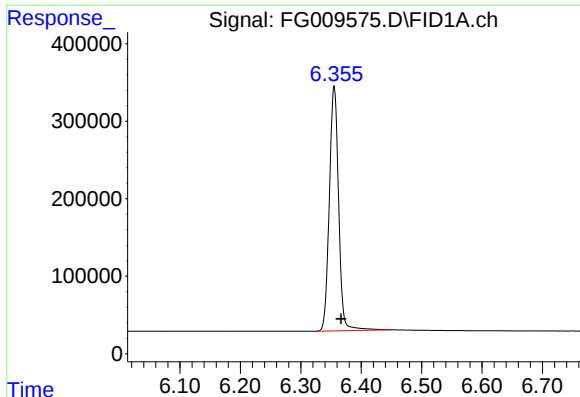

#3 N-DODECANE


R.T.: 6.355 min
Delta R.T.: -0.011 min
Response: 3372086
Conc: 22.37 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

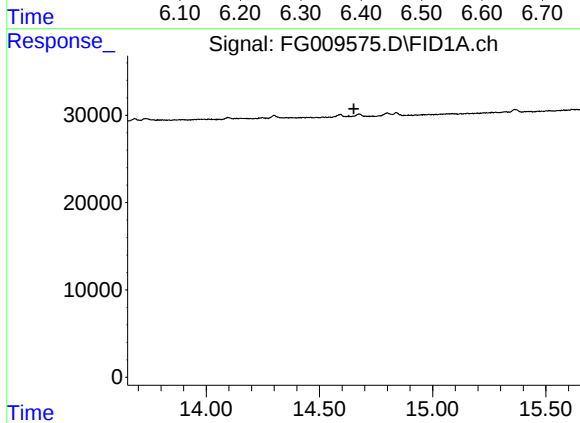

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.652 min
Response: 0
Conc: N.D.

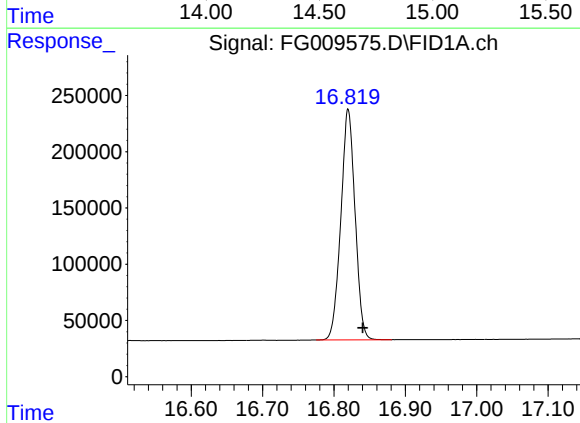

#12 N-OCTACOSANE

R.T.: 16.820 min
Delta R.T.: -0.021 min
Response: 2837564
Conc: 21.74 ug/ml