

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG041122\  
 Data File : FG009576.D  
 Signal(s) : FID1A.ch  
 Acq On : 11 Apr 2022 12:45  
 Operator : AJ\MA  
 Sample : N2301-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :  
 WC-14A-1A-4-GR-7

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 04/11/2022  
 Supervised By :mohammad ahmed 04/13/2022

Integration File: autoint1.e  
 Quant Time: Apr 11 13:32:11 2022  
 Quant Title :  
 QLast Update : Fri Apr 08 10:19:35 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.657 | 1766927  | 13.716 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG041122\  
Data File : FG009576.D  
Signal(s) : FID1A.ch  
Acq On : 11 Apr 2022 12:45  
Operator : AJ\MA  
Sample : N2301-07  
Misc :  
ALS Vial : 5 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
WC-14A-1A-4-GR-7


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/11/2022  
Supervised By :mohammad ahmed 04/13/2022

Integration File: autoint1.e  
Quant Time: Apr 11 13:32:11 2022  
Quant Title :  
QLast Update : Fri Apr 08 10:19:35 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

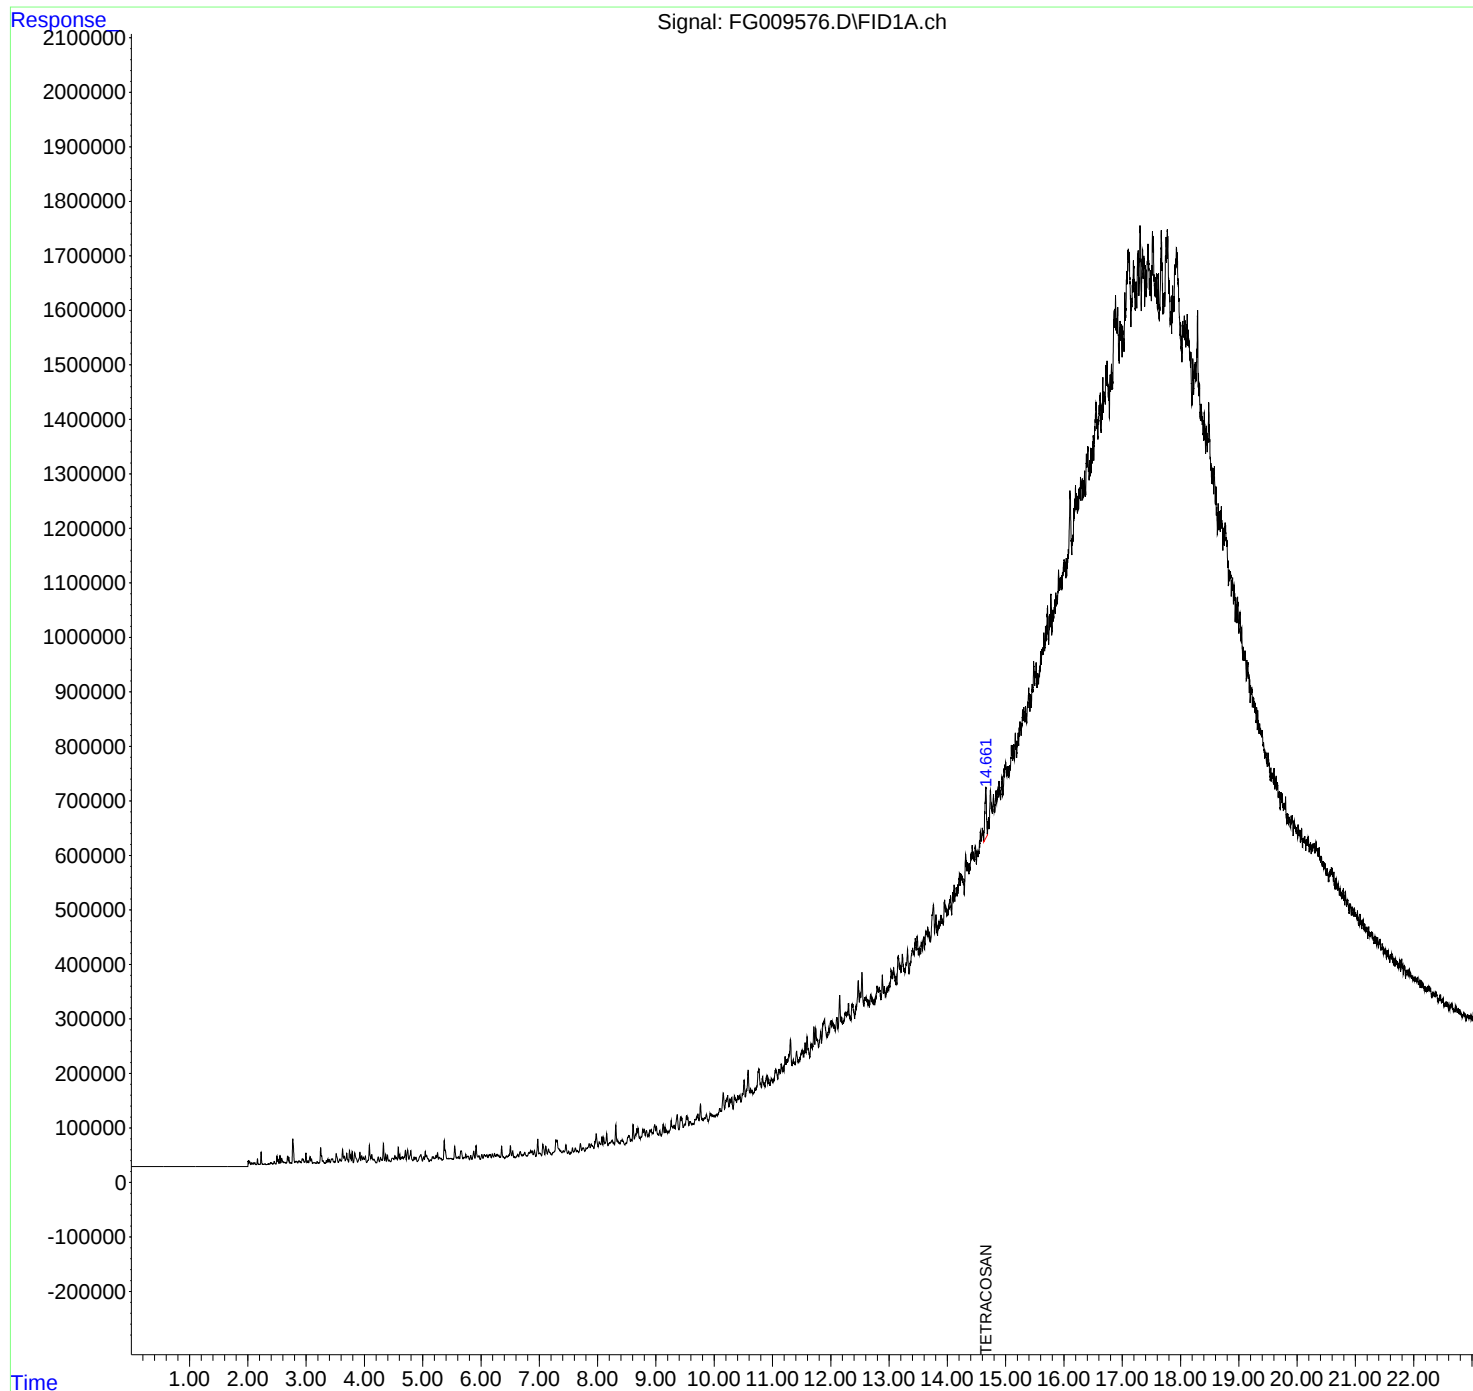

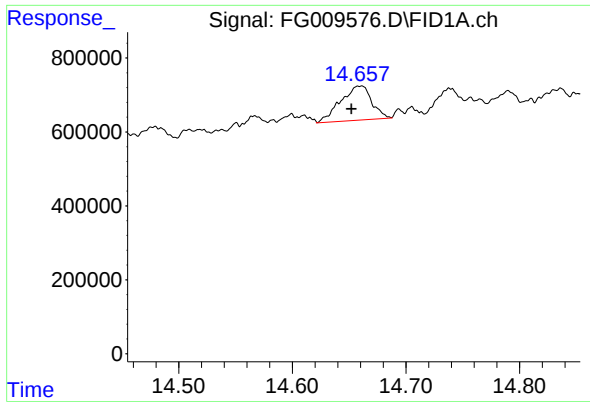

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.657 min  
Delta R.T.: 0.005 min  
Response: 1766927  
Conc: 13.72 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
WC-14A-1A-4-GR-7

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/11/2022  
Supervised By :mohammad ahmed 04/13/2022