

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041422\
 Data File : FG009623.D
 Signal(s) : FID1A.ch
 Acq On : 14 Apr 2022 14:27
 Operator : AJ\MA
 Sample : PB144021BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 15 01:12:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG041322.M
 Quant Title :
 QLast Update : Wed Apr 13 15:22:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.631	1990907	12.238 ug/ml
Target Compounds			
11) N-OCTACOSANE	16.809	1249626	10.193 ug/ml
12) N-DOTRIACONTANE	18.559	235179	1.988 ug/ml
14) N-HEXATRIACONTANE	20.066	1656539	14.154 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041422\
Data File : FG009623.D
Signal(s) : FID1A.ch
Acq On : 14 Apr 2022 14:27
Operator : AJ\MA
Sample : PB144021BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 15 01:12:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG041322.M
Quant Title :
QLast Update : Wed Apr 13 15:22:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

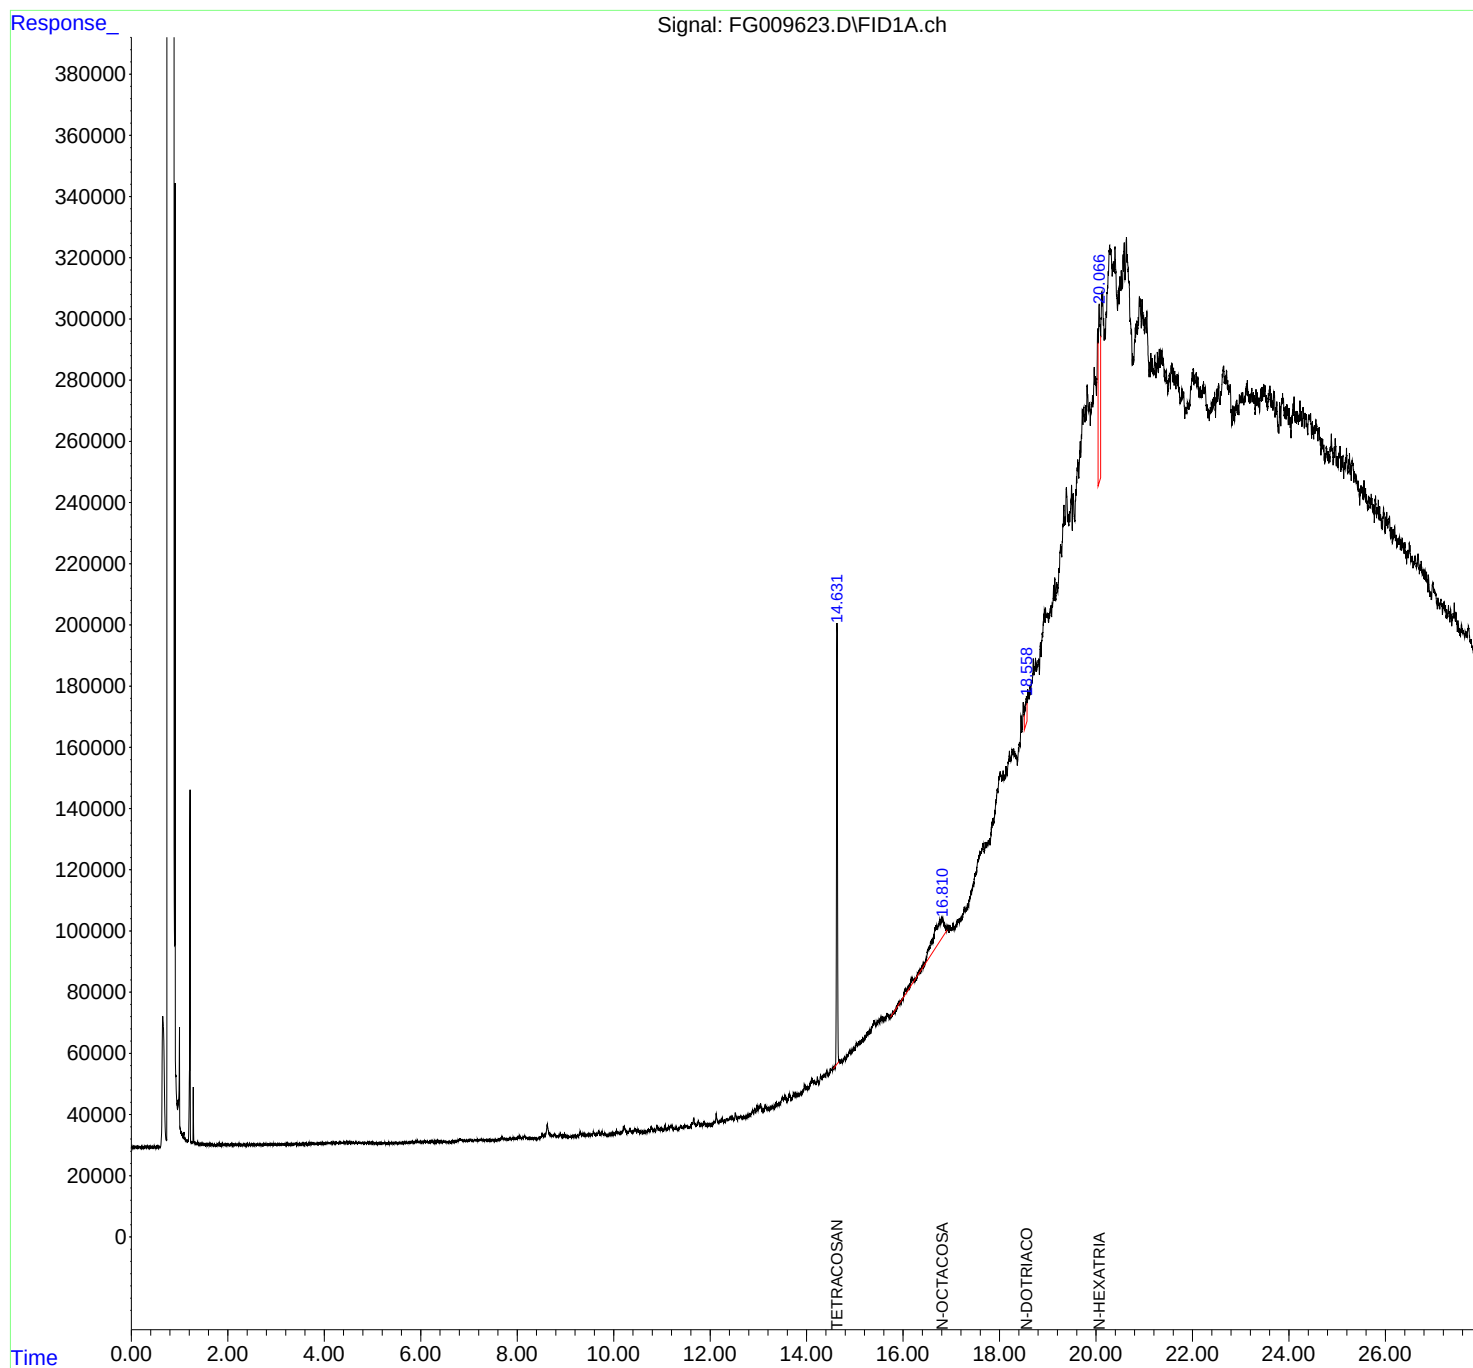


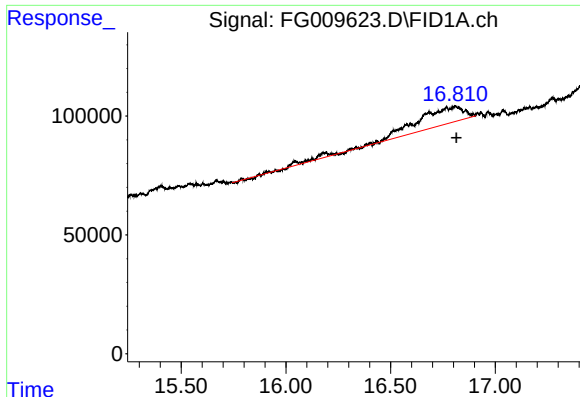

#11 N-OCTACOSANE


R.T.: 16.809 min
Delta R.T.: -0.004 min
Response: 1249626
Conc: 10.19 ug/ml

Instrument :
FID_G
ClientSampleId :

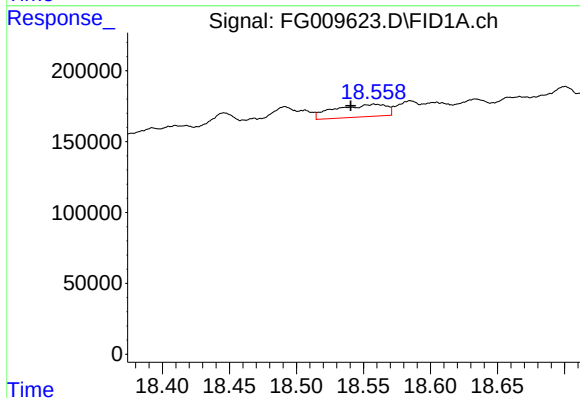


#12 N-DOTRIACONTANE

R.T.: 18.559 min
Delta R.T.: 0.018 min
Response: 235179
Conc: 1.99 ug/ml

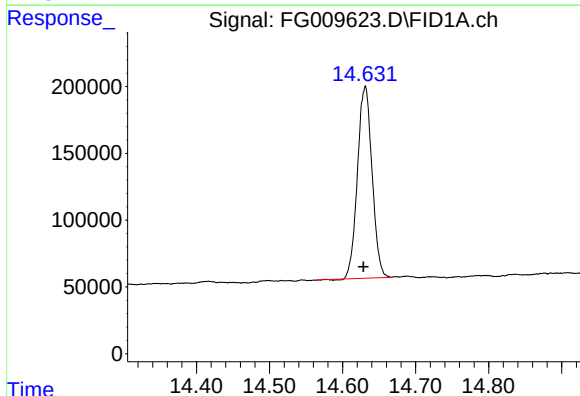

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.631 min
Delta R.T.: 0.002 min
Response: 1990907
Conc: 12.24 ug/ml

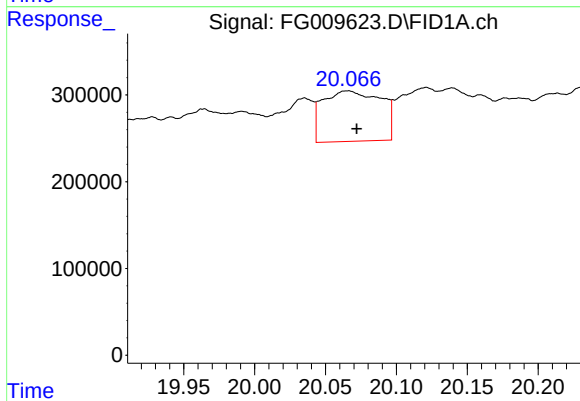

#14 N-HEXATRIACONTANE

R.T.: 20.066 min
Delta R.T.: -0.006 min
Response: 1656539
Conc: 14.15 ug/ml