

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041422\
 Data File : FG009627.D
 Signal(s) : FID1A.ch
 Acq On : 14 Apr 2022 16:51
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2022
 Supervised By :mohammad ahmed 04/18/2022

Integration File: sample.e
 Quant Time: Apr 15 01:13:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG041322.M
 Quant Title :
 QLast Update : Wed Apr 13 15:22:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.627	2202597	13.540 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041422\
Data File : FG009627.D
Signal(s) : FID1A.ch
Acq On : 14 Apr 2022 16:51
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2022
Supervised By :mohammad ahmed 04/18/2022

Integration File: sample.e
Quant Time: Apr 15 01:13:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG041322.M
Quant Title :
QLast Update : Wed Apr 13 15:22:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

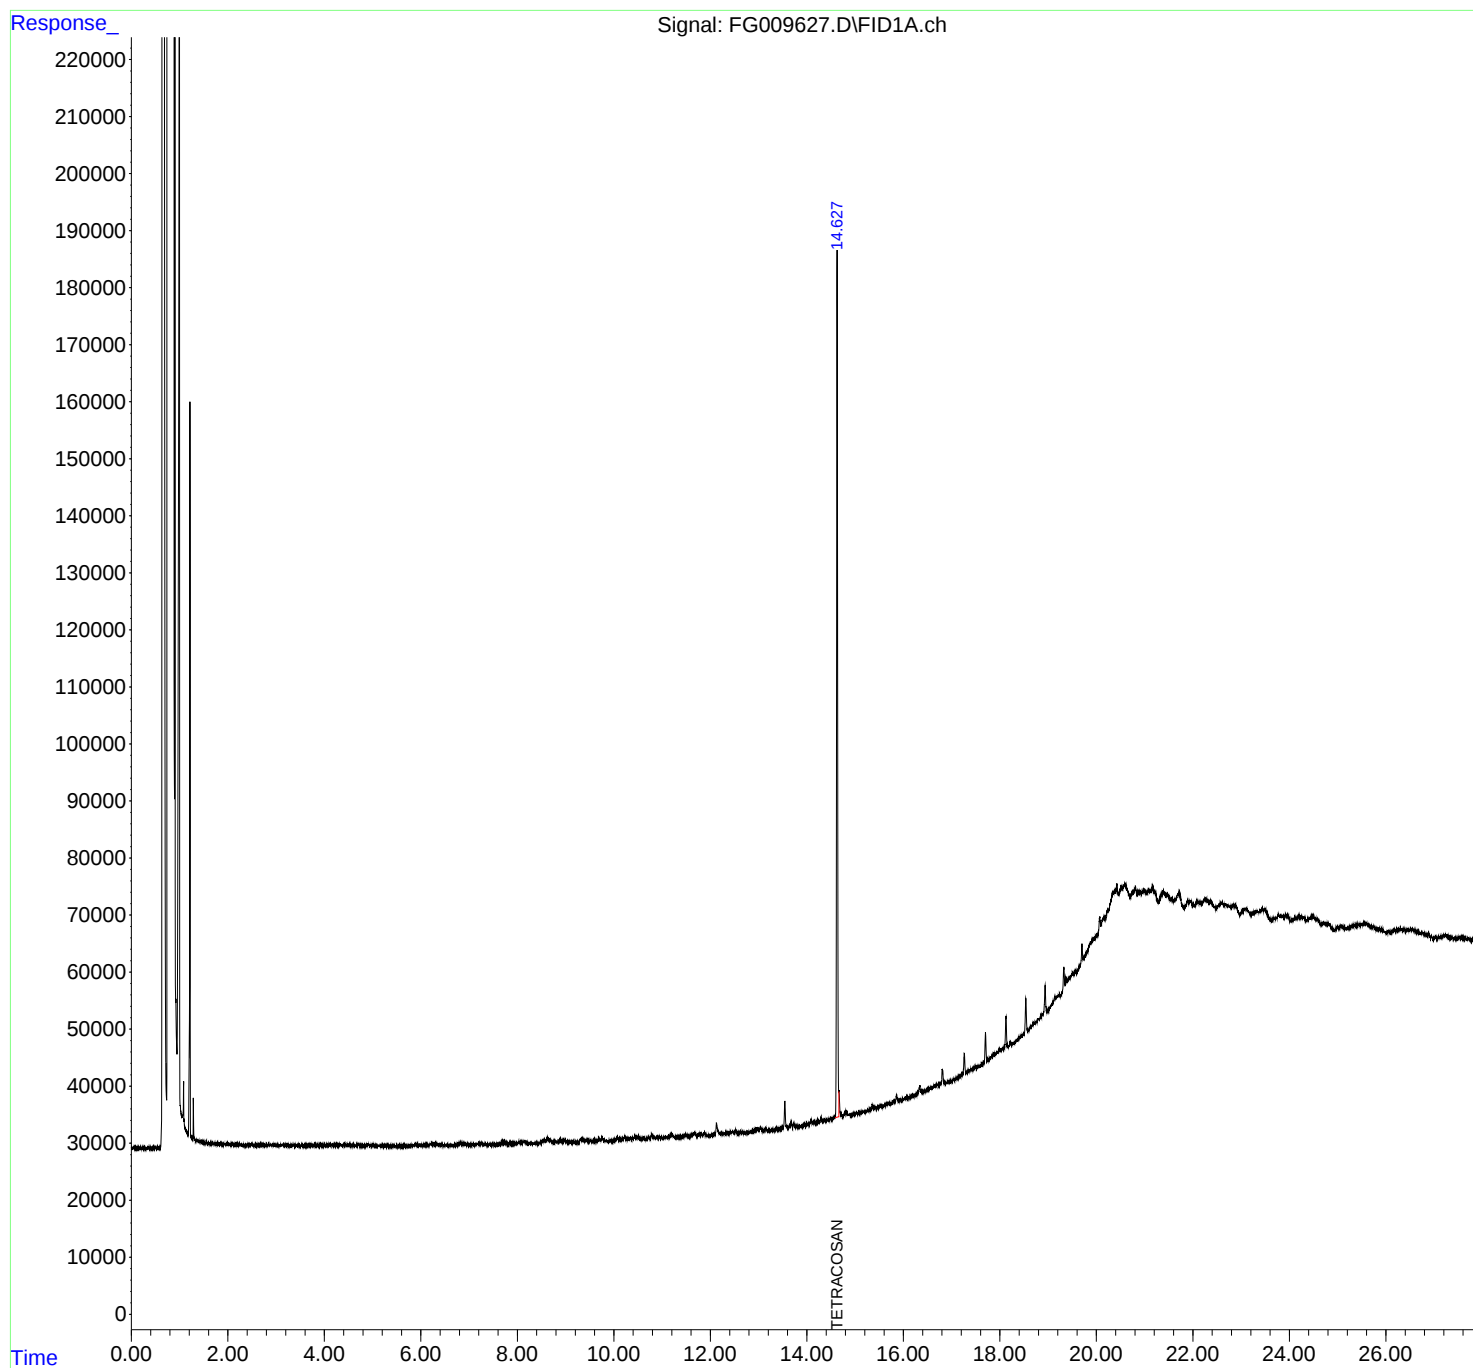

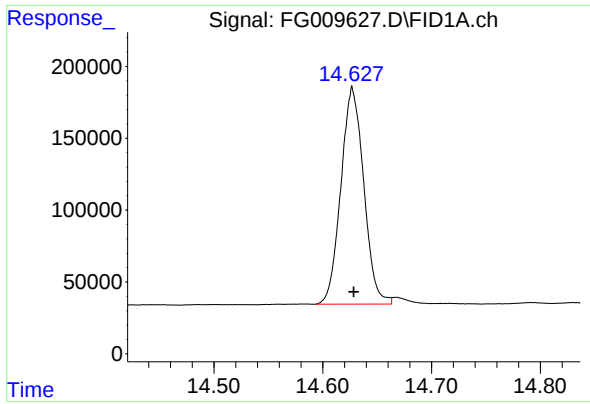

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: -0.002 min
Response: 2202597
Conc: 13.54 ug/ml

Instrument :

FID_G

ClientSampleId :

I.BLK

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/15/2022

Supervised By :mohammad ahmed 04/18/2022