

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041625\
 Data File : FG015673.D
 Signal(s) : FID1A.ch
 Acq On : 16 Apr 2025 15:44
 Operator : YP\AJ
 Sample : PB167614BS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 17 02:17:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032725.M
 Quant Title :
 QLast Update : Thu Mar 27 11:04:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.008	1862173	16.254 ug/ml
Target Compounds			
1) N-OCTANE	1.983	1700589	14.631 ug/ml
2) N-DECANE	4.509	1973485	16.705 ug/ml
3) N-DODECANE	6.691	2084713	17.169 ug/ml
4) N-TETRADECANE	8.527	2085598	16.539 ug/ml
5) N-HEXADECANE	10.141	2152789	16.720 ug/ml
6) N-OCTADECANE	11.588	2229141	16.921 ug/ml
7) N-EICOSANE	12.903	2172633	16.226 ug/ml
8) N-DOCOSANE	14.105	2130686	16.397 ug/ml
10) N-TETRACOSANE	15.212	2118911	16.359 ug/ml
11) N-HEXACOSANE	16.237	2046755	16.081 ug/ml
12) N-OCTACOSANE	17.188	1997631	15.981 ug/ml
13) N-TRIACONTANE	18.078	1903779	15.209 ug/ml
14) N-DOTRIACONTANE	18.914	1515742	12.772 ug/ml
15) N-TETRATRIACONTANE	19.698	845487	8.100 ug/ml
16) N-HEXATRIACONTANE	20.439	453895	5.179 ug/ml
17) N-OCTATRIACONTANE	21.181	296367	3.971 ug/ml
18) N-TETRACONTANE	22.106	211135	3.188 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041625\
Data File : FG015673.D
Signal(s) : FID1A.ch
Acq On : 16 Apr 2025 15:44
Operator : YP\AJ
Sample : PB167614BS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 17 02:17:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032725.M
Quant Title :
QLast Update : Thu Mar 27 11:04:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

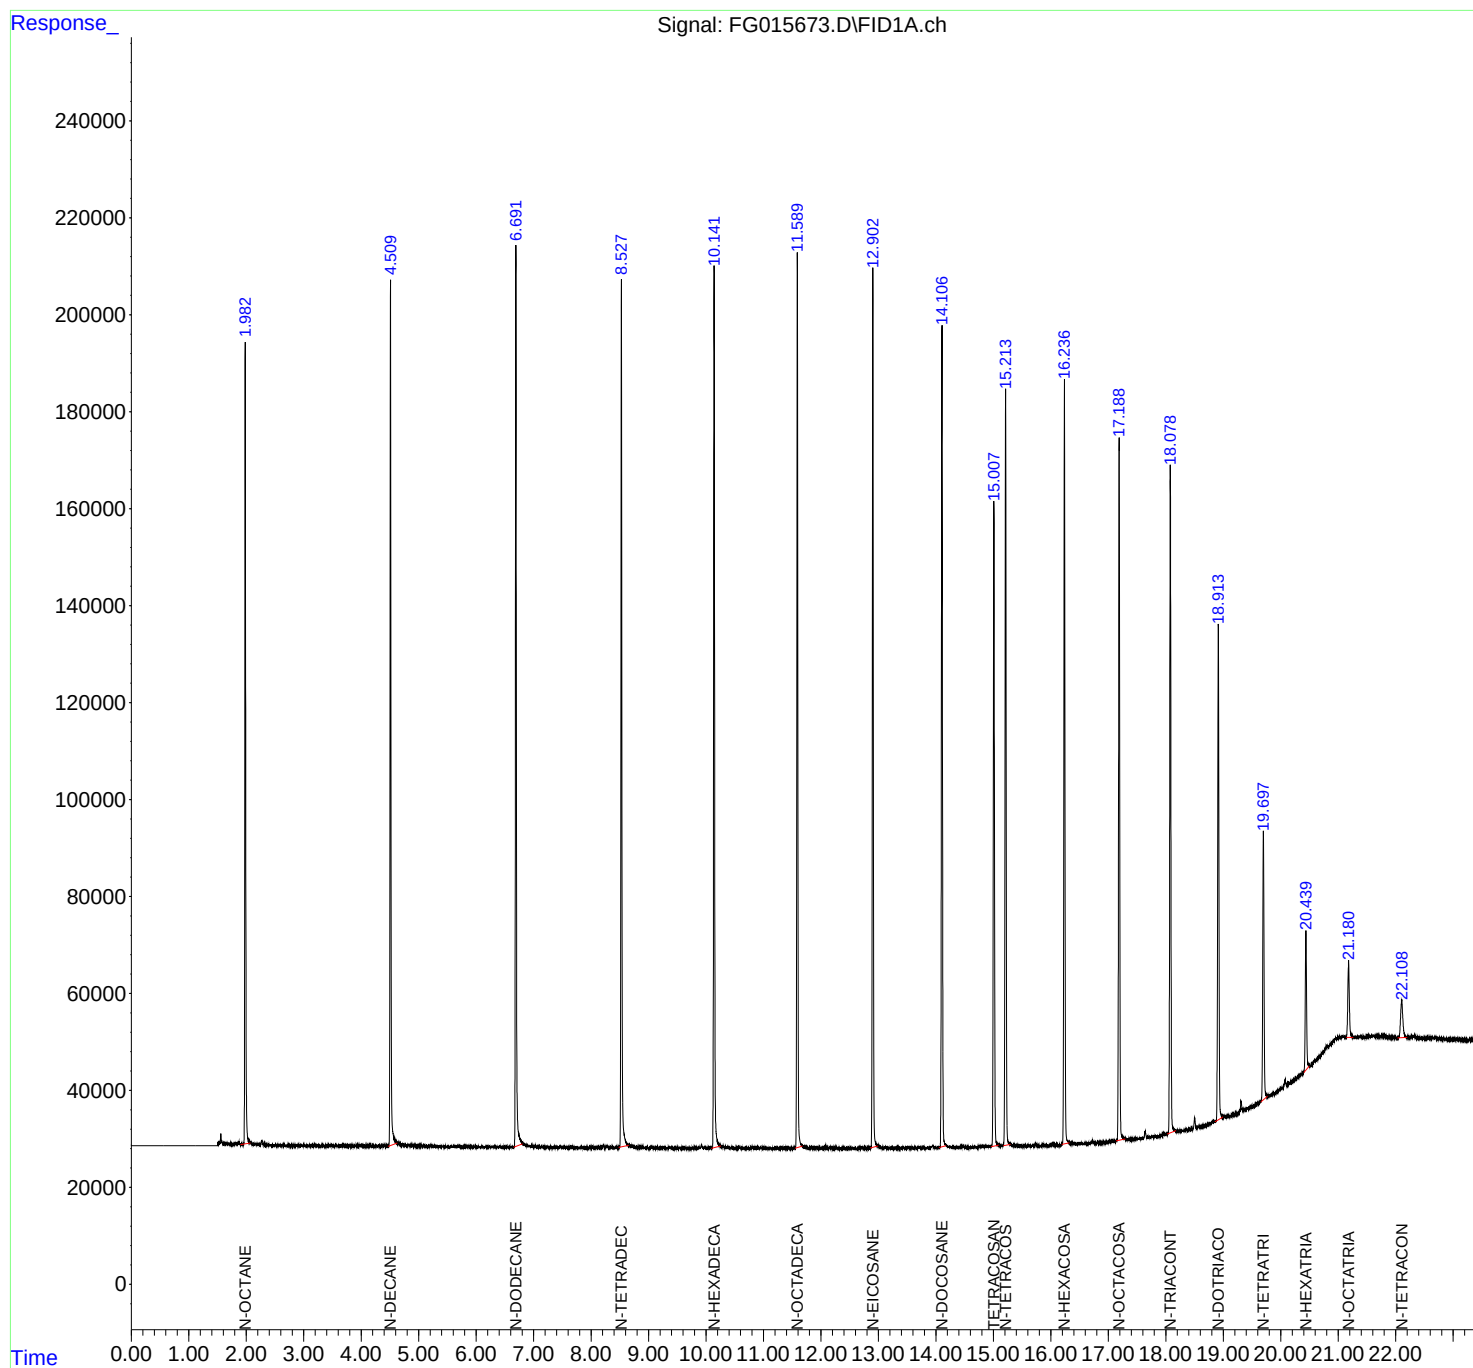


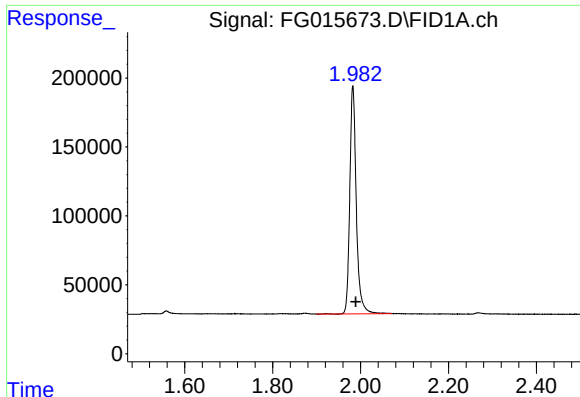

#1 N-OCTANE


R.T.: 1.983 min
Delta R.T.: -0.006 min
Response: 1700589
Conc: 14.63 ug/ml

Instrument :
FID_G
ClientSampleId :

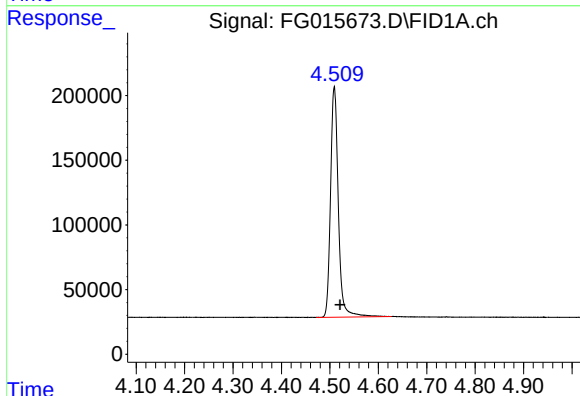


#2 N-DECANE

R.T.: 4.509 min
Delta R.T.: -0.012 min
Response: 1973485
Conc: 16.71 ug/ml

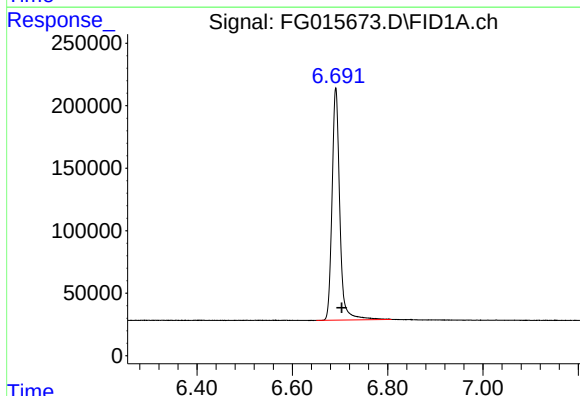


#3 N-DODECANE

R.T.: 6.691 min
Delta R.T.: -0.013 min
Response: 2084713
Conc: 17.17 ug/ml

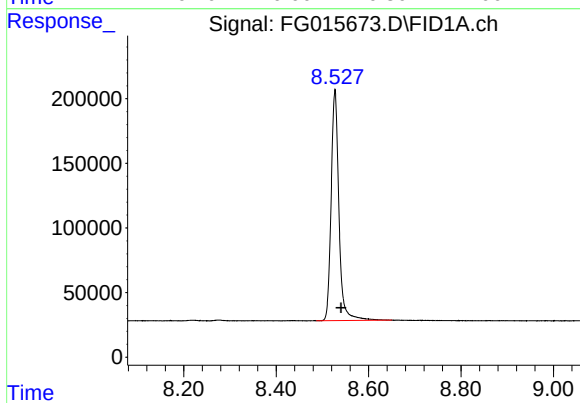

#4 N-TETRADECANE


R.T.: 8.527 min
Delta R.T.: -0.013 min
Response: 2085598
Conc: 16.54 ug/ml

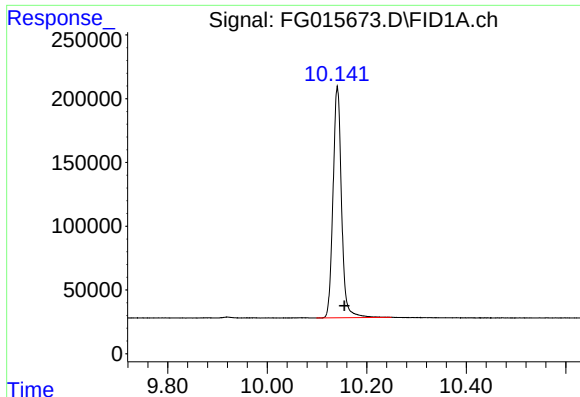

#5 N-HEXADECANE


R.T.: 10.141 min
Delta R.T.: -0.014 min
Response: 2152789
Conc: 16.72 ug/ml

Instrument :
FID_G
ClientSampleId :

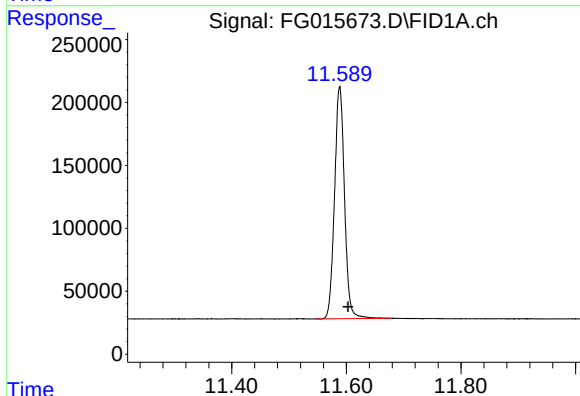


#6 N-OCTADECANE

R.T.: 11.588 min
Delta R.T.: -0.015 min
Response: 2229141
Conc: 16.92 ug/ml

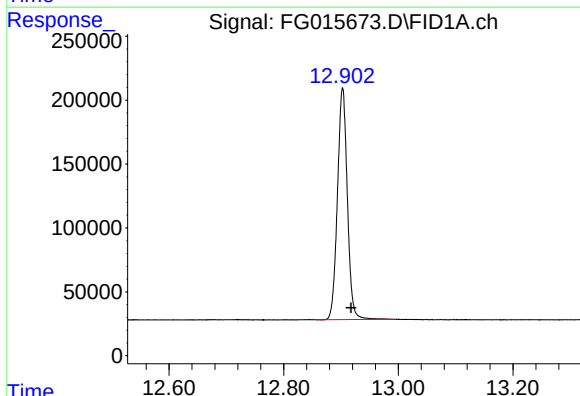


#7 N-EICOSANE

R.T.: 12.903 min
Delta R.T.: -0.015 min
Response: 2172633
Conc: 16.23 ug/ml

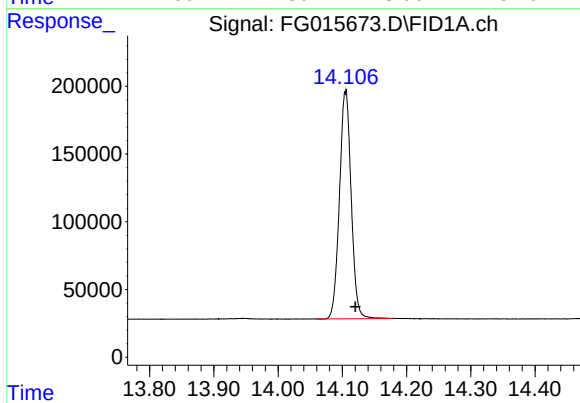

#8 N-DOCOSANE


R.T.: 14.105 min
Delta R.T.: -0.015 min
Response: 2130686
Conc: 16.40 ug/ml

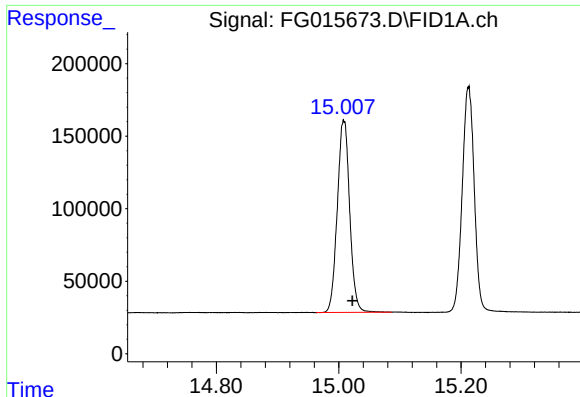

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.008 min
Delta R.T.: -0.014 min
Response: 1862173
Conc: 16.25 ug/ml

Instrument :
FID_G
ClientSampleId :

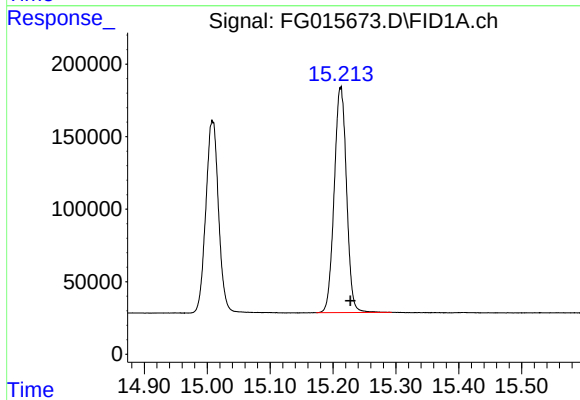


#10 N-TETRACOSANE

R.T.: 15.212 min
Delta R.T.: -0.016 min
Response: 2118911
Conc: 16.36 ug/ml

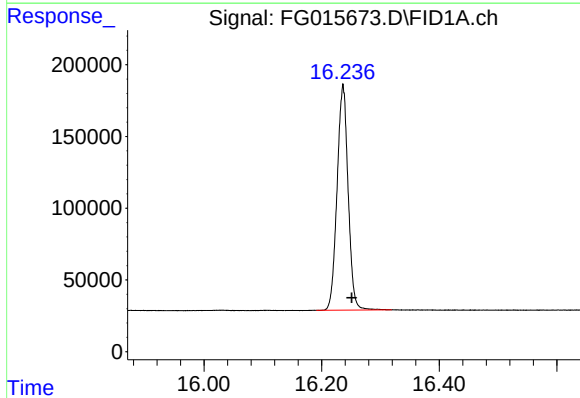


#11 N-HEXACOSANE

R.T.: 16.237 min
Delta R.T.: -0.015 min
Response: 2046755
Conc: 16.08 ug/ml

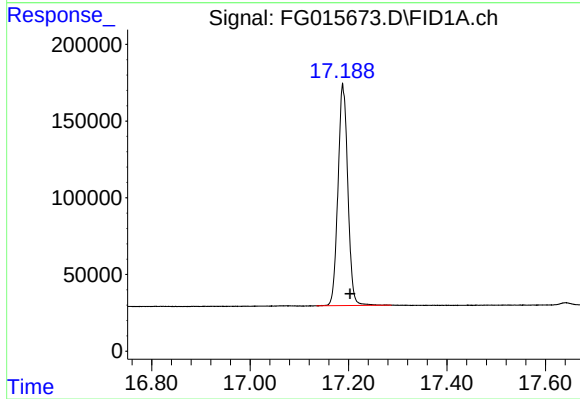

#12 N-OCTACOSANE


R.T.: 17.188 min
Delta R.T.: -0.015 min
Response: 1997631
Conc: 15.98 ug/ml

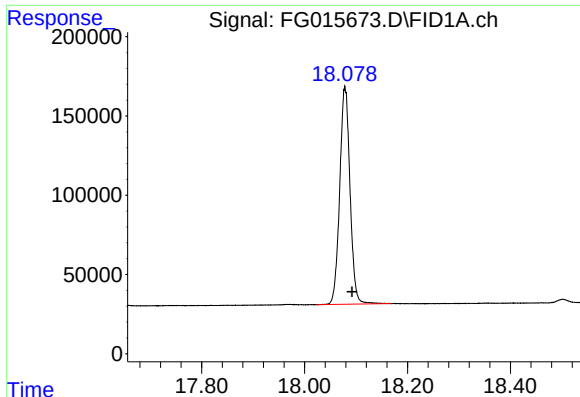

#13 N-TRIACONTANE


R.T.: 18.078 min
Delta R.T.: -0.014 min
Response: 1903779
Conc: 15.21 ug/ml

Instrument :
FID_G
ClientSampleId :

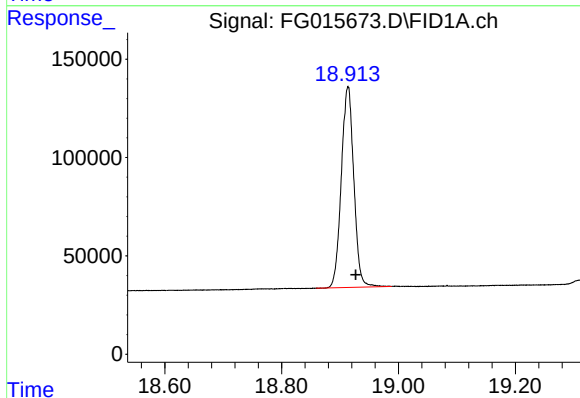


#14 N-DOTRIACONTANE

R.T.: 18.914 min
Delta R.T.: -0.013 min
Response: 1515742
Conc: 12.77 ug/ml

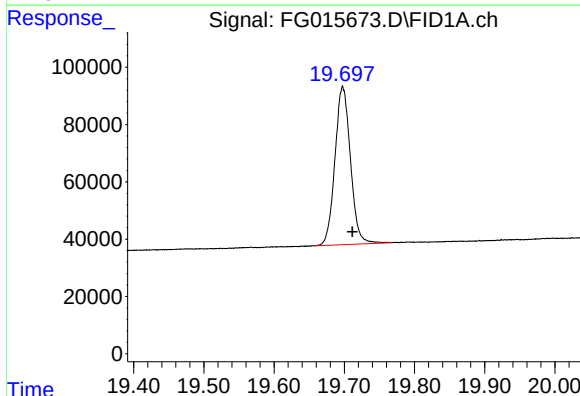


#15 N-TETRATRIACONTANE

R.T.: 19.698 min
Delta R.T.: -0.014 min
Response: 845487
Conc: 8.10 ug/ml

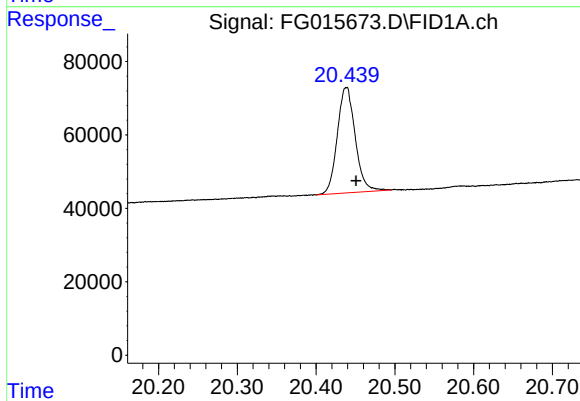

#16 N-HEXATRIACONTANE


R.T.: 20.439 min
Delta R.T.: -0.012 min
Response: 453895
Conc: 5.18 ug/ml

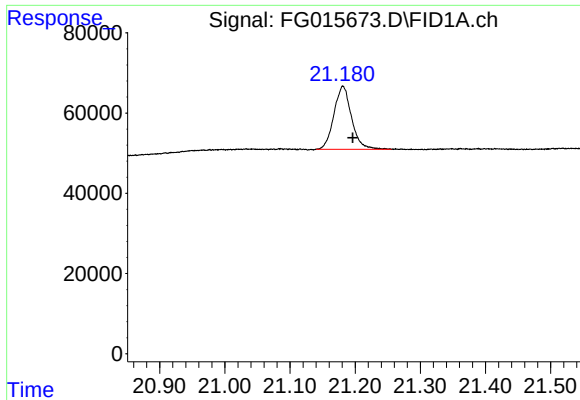

#17 N-OCTATRIACONTANE

R.T.: 21.181 min
Delta R.T.: -0.015 min
Response: 296367
Conc: 3.97 ug/ml

Instrument :
FID_G
ClientSampleId :

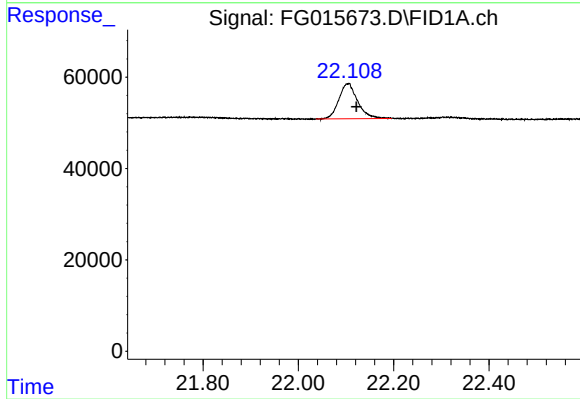

#18 N-TETRACONTANE

R.T.: 22.106 min
Delta R.T.: -0.016 min
Response: 211135
Conc: 3.19 ug/ml