

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041625\
Data File : FG015676.D
Signal(s) : FID1A.ch
Acq On : 16 Apr 2025 17:12
Operator : YP\AJ
Sample : Q1812-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RINSE-EB-PUMP-041525

Integration File: autoint1.e
Quant Time: Apr 17 02:18:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032725.M
Quant Title :
QLast Update : Thu Mar 27 11:04:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.007	1800028	15.712 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041625\
Data File : FG015676.D
Signal(s) : FID1A.ch
Acq On : 16 Apr 2025 17:12
Operator : YP\AJ
Sample : Q1812-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RINSE-EB-PUMP-041525

Integration File: autoint1.e
Quant Time: Apr 17 02:18:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032725.M
Quant Title :
QLast Update : Thu Mar 27 11:04:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

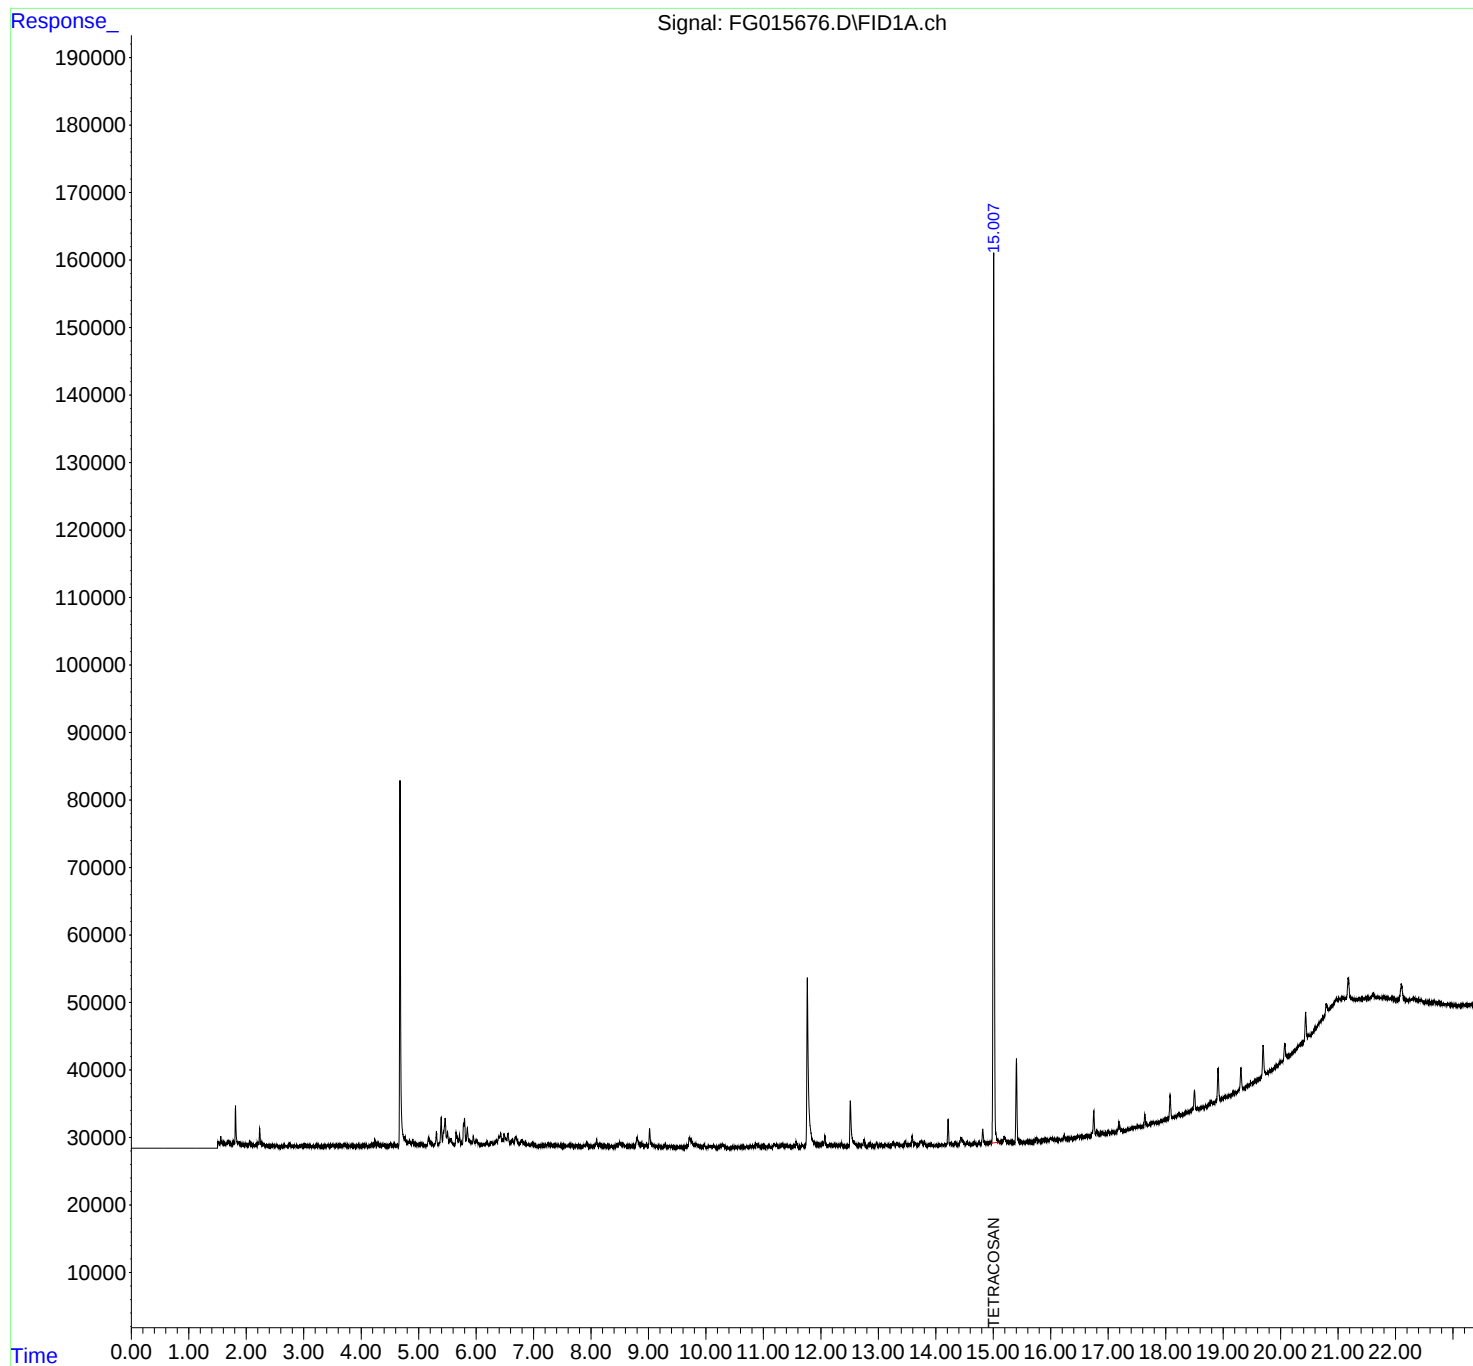

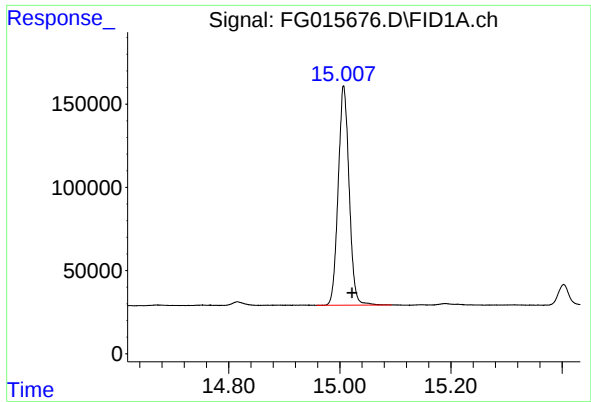

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.007 min
Delta R.T.: -0.015 min
Response: 1800028
Conc: 15.71 ug/ml

Instrument :
FID_G
ClientSampleId :
RINSE-EB-PUMP-041525