

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041919\
 Data File : FG004752.D
 Signal(s) : FID1A.ch
 Acq On : 19 Apr 2019 15:44
 Operator : AJ\SJ
 Sample : K2484-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 19 22:38:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.404	2018490	19.569 ug/ml
Target Compounds			
4) N-TETRADECANE	8.020	326291	3.012 ug/ml
8) N-DOCOSANE	13.502	127899	1.119 ug/ml
10) N-TETRACOSANE	14.606	95138	0.824 ug/ml
11) N-HEXACOSANE	15.629	437700	3.818 ug/ml
12) N-OCTACOSANE	16.582	1442866	12.472 ug/ml
13) N-TRIACONTANE	17.472	2121664	17.884 ug/ml
14) N-DOTRIACONTANE	18.307	1236893	10.548 ug/ml
15) N-TETRATRIACONTANE	19.096	196905	1.767 ug/ml
16) N-HEXATRIACONTANE	19.842	117192	1.051 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041919\
Data File : FG004752.D
Signal(s) : FID1A.ch
Acq On : 19 Apr 2019 15:44
Operator : AJ\SJ
Sample : K2484-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 19 22:38:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

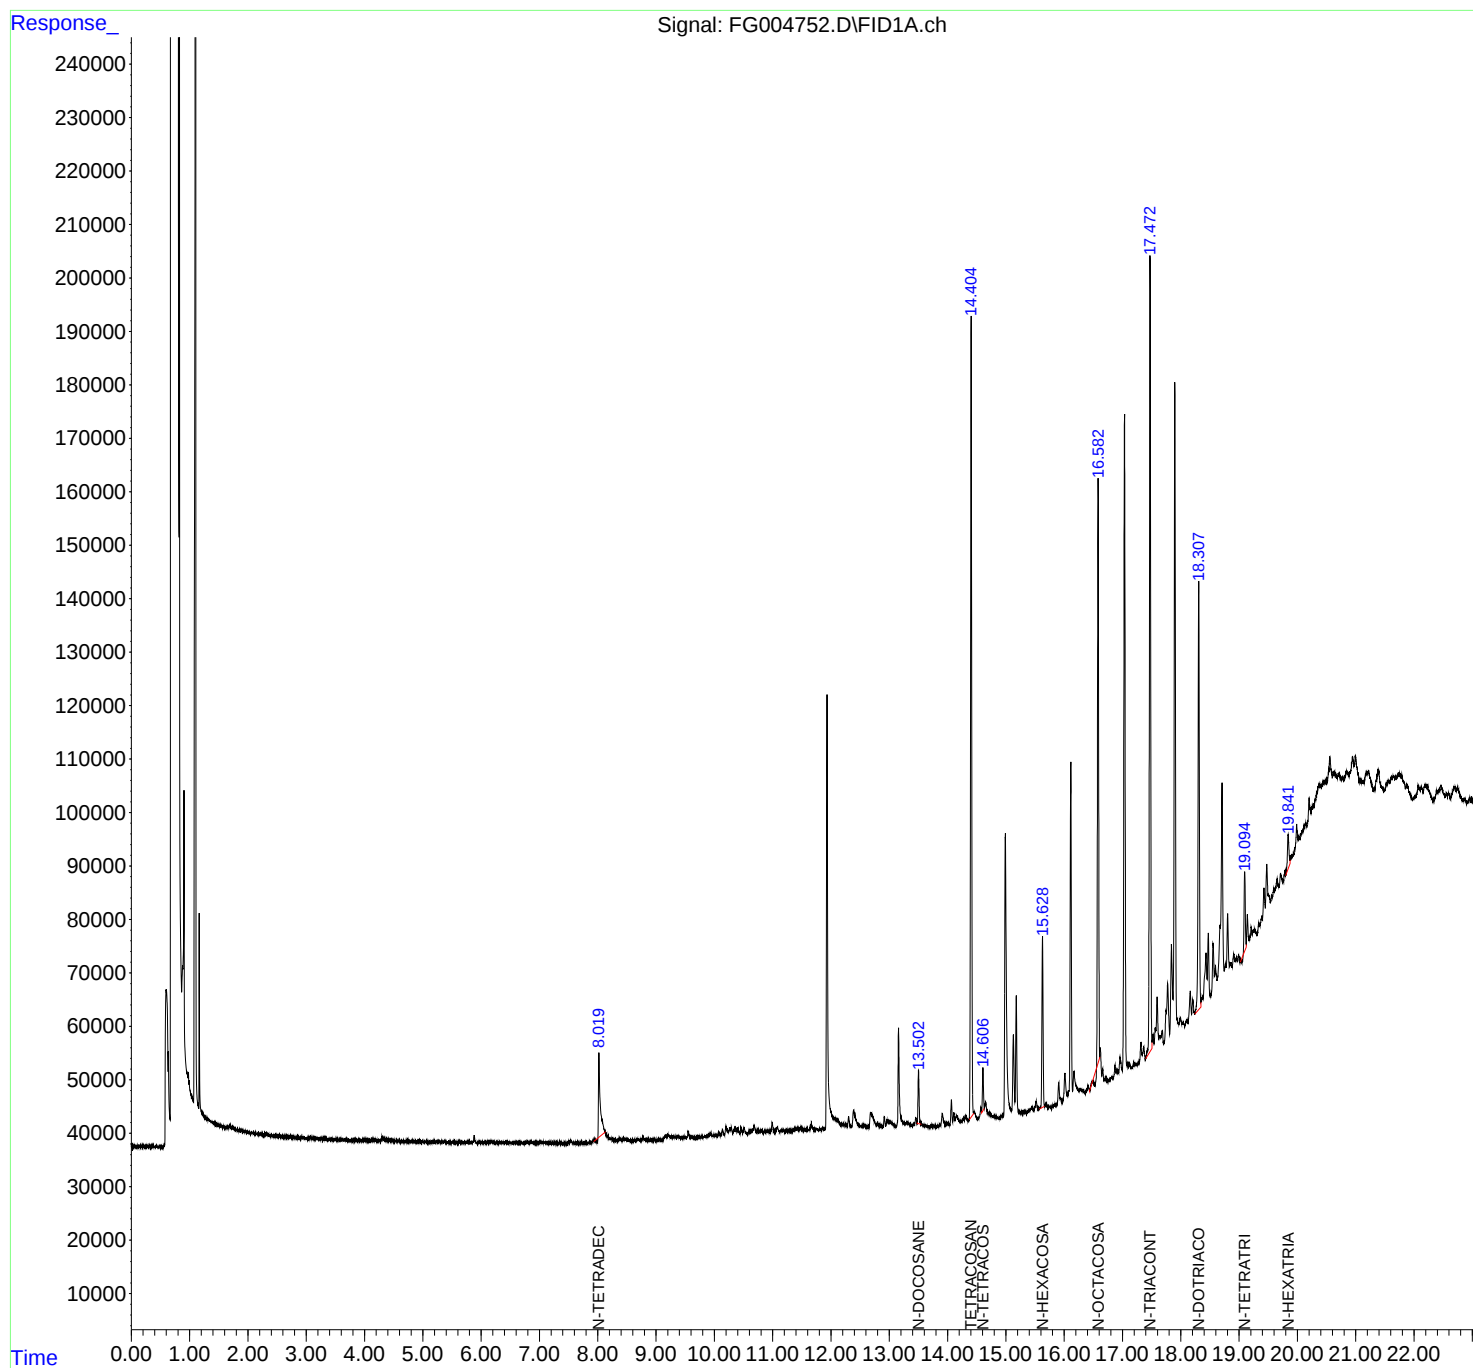

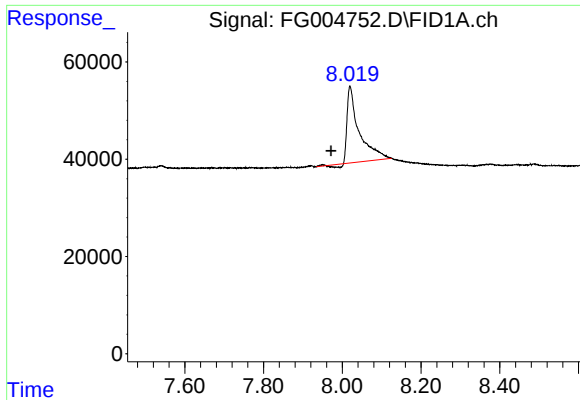


#4 N-TETRADECANE

R.T.: 8.020 min
Delta R.T.: 0.048 min
Response: 326291
Conc: 3.01 ug/ml

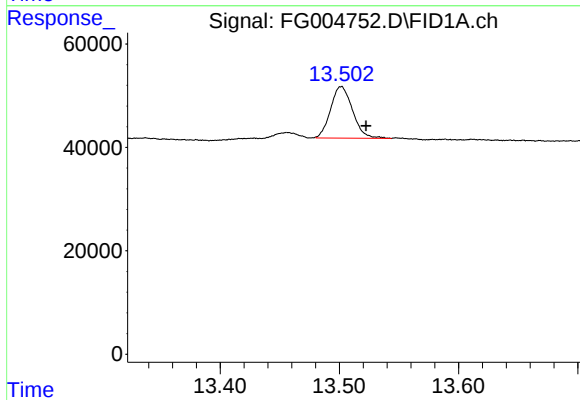


#8 N-DOCOSANE

R.T.: 13.502 min
Delta R.T.: -0.021 min
Response: 127899
Conc: 1.12 ug/ml

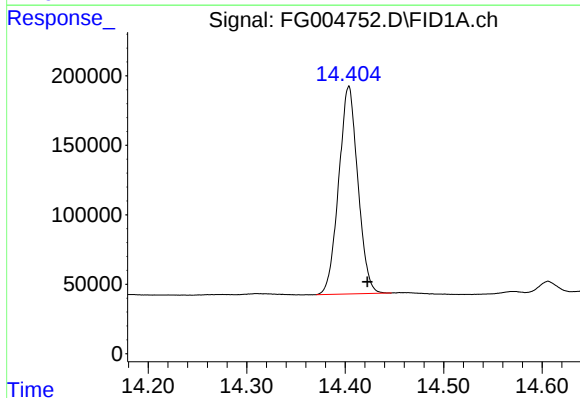


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.404 min
Delta R.T.: -0.019 min
Response: 2018490
Conc: 19.57 ug/ml

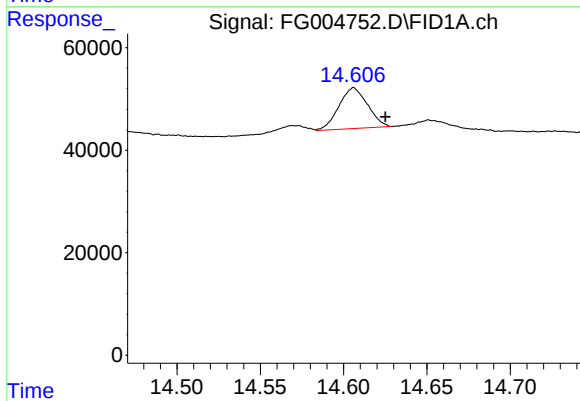


#10 N-TETRACOSANE

R.T.: 14.606 min
Delta R.T.: -0.019 min
Response: 95138
Conc: 0.82 ug/ml

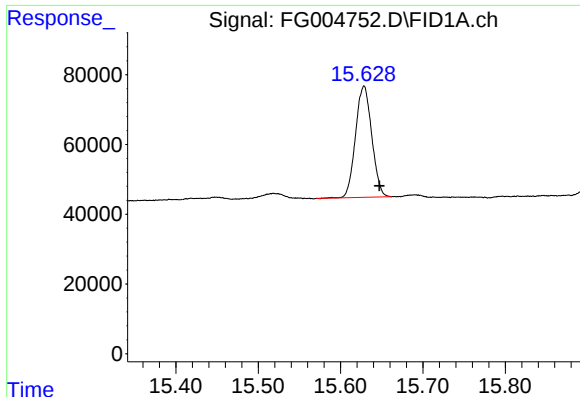


#11 N-HEXACOSANE

R.T.: 15.629 min
Delta R.T.: -0.018 min
Response: 437700
Conc: 3.82 ug/ml

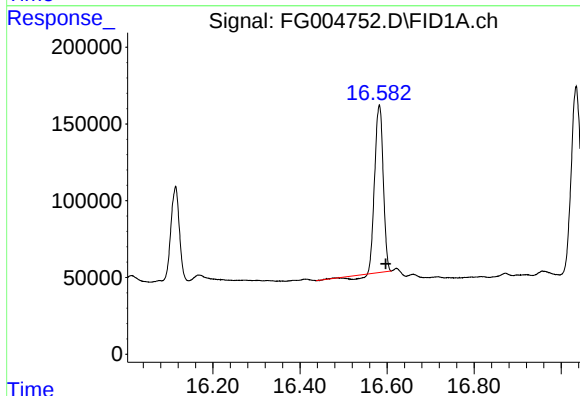


#12 N-OCTACOSANE

R.T.: 16.582 min
Delta R.T.: -0.015 min
Response: 1442866
Conc: 12.47 ug/ml

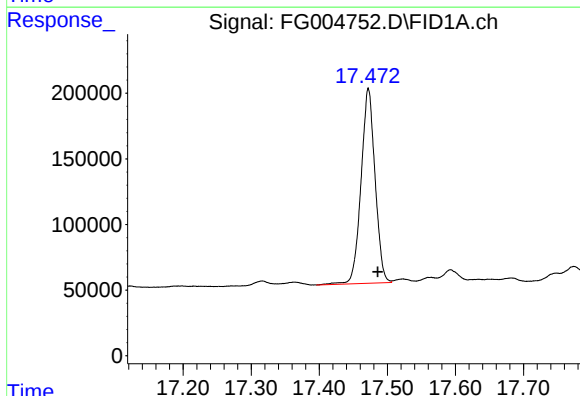


#13 N-TRIACONTANE

R.T.: 17.472 min
Delta R.T.: -0.014 min
Response: 2121664
Conc: 17.88 ug/ml

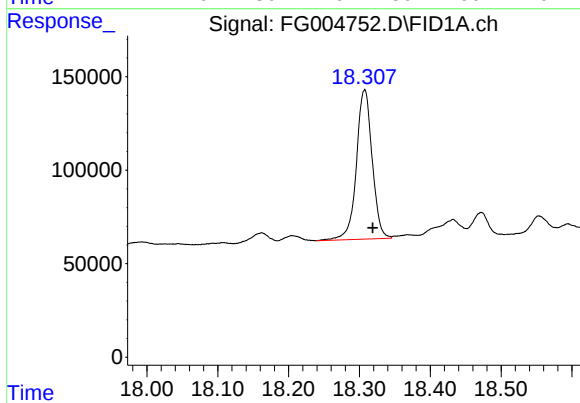


#14 N-DOTRIACONTANE

R.T.: 18.307 min
Delta R.T.: -0.011 min
Response: 1236893
Conc: 10.55 ug/ml

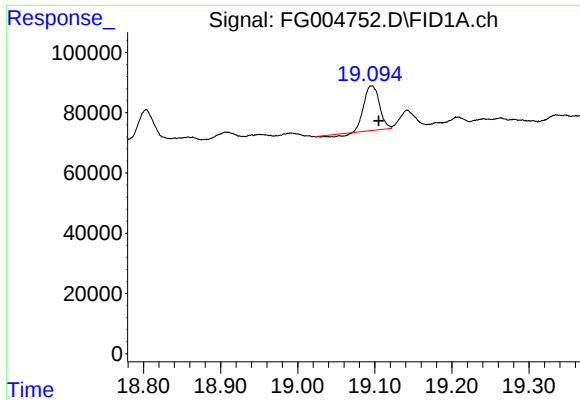

#15 N-TETRATRIACONTANE

R.T.: 19.096 min
Delta R.T.: -0.009 min
Response: 196905
Conc: 1.77 ug/ml

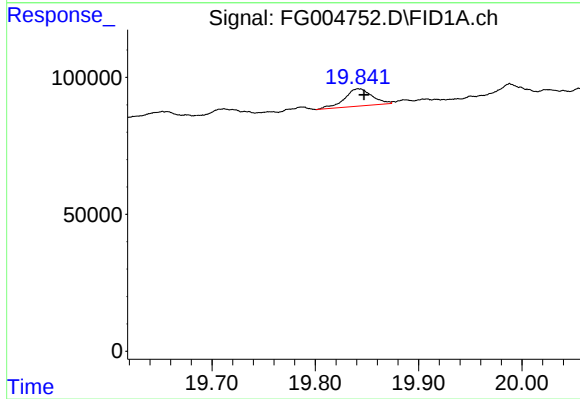

#16 N-HEXATRIACONTANE

R.T.: 19.842 min
Delta R.T.: -0.005 min
Response: 117192
Conc: 1.05 ug/ml