

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041919\
 Data File : FG004755.D
 Signal(s) : FID1A.ch
 Acq On : 19 Apr 2019 17:14
 Operator : AJ\SJ
 Sample : K2484-05MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 19 22:39:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.404	2109112	20.448 ug/ml
Target Compounds			
2) N-DECANE	4.135	2255897	21.372 ug/ml
3) N-DODECANE	6.156	2369454	22.490 ug/ml
4) N-TETRADECANE	7.950	2485764	22.942 ug/ml
5) N-HEXADECANE	9.550	2541266	22.714 ug/ml
6) N-OCTADECANE	10.993	2523213	22.246 ug/ml
7) N-EICOSANE	12.302	2514610	21.997 ug/ml
8) N-DOCOSANE	13.503	2559421	22.390 ug/ml
10) N-TETRACOSANE	14.609	2663609	23.058 ug/ml
11) N-HEXACOSANE	15.631	2742564	23.925 ug/ml
12) N-OCTACOSANE	16.583	3411354	29.488 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041919\
Data File : FG004755.D
Signal(s) : FID1A.ch
Acq On : 19 Apr 2019 17:14
Operator : AJ\SJ
Sample : K2484-05MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 19 22:39:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

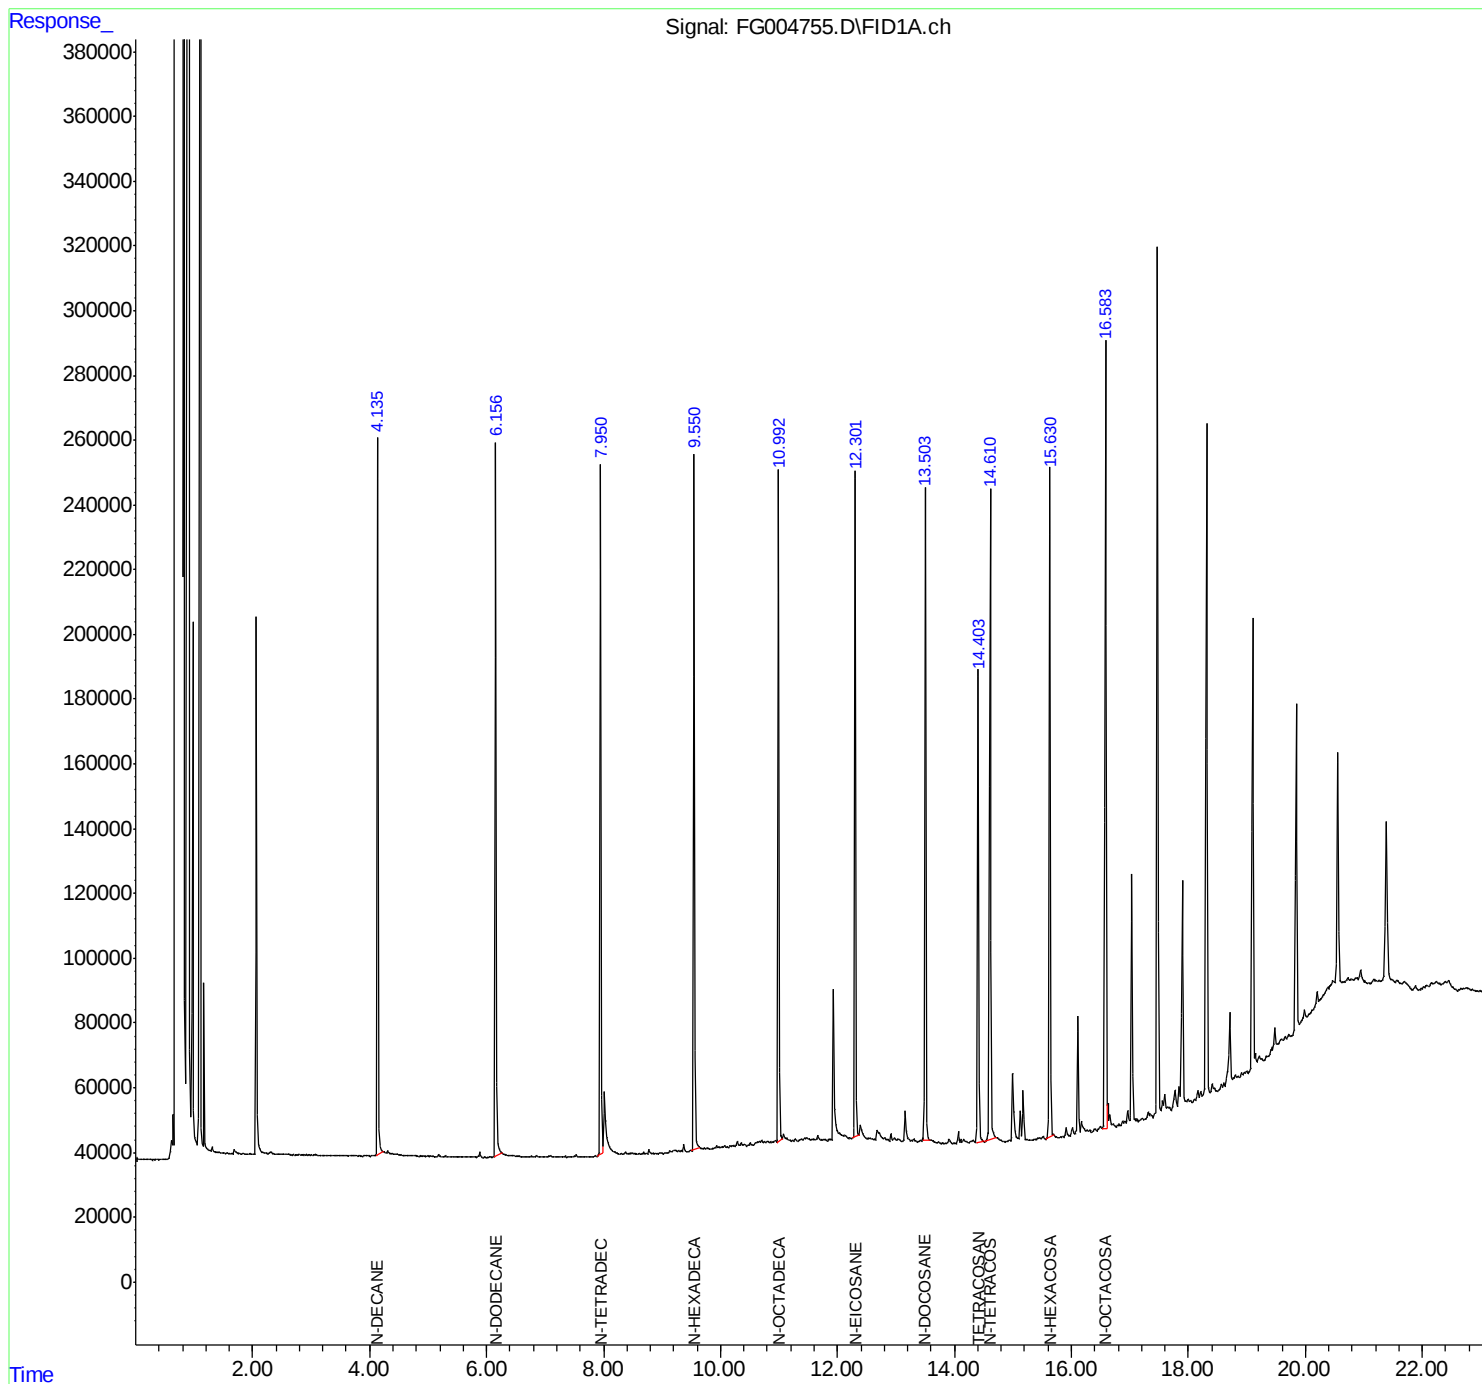

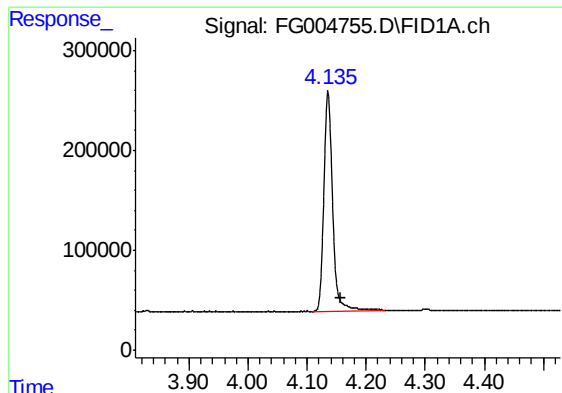


#2 N-DECANE

R.T.: 4.135 min
Delta R.T.: -0.021 min
Response: 2255897
Conc: 21.37 ug/ml

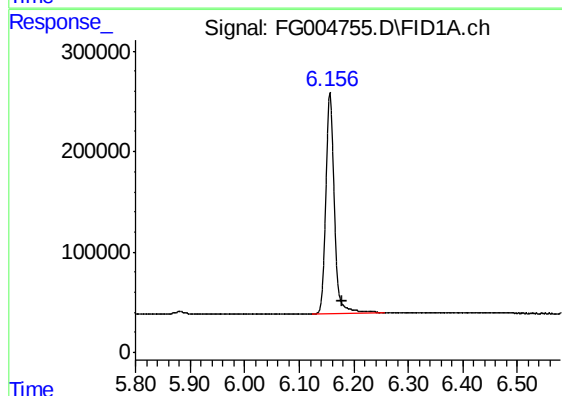


#3 N-DODECANE

R.T.: 6.156 min
Delta R.T.: -0.022 min
Response: 2369454
Conc: 22.49 ug/ml

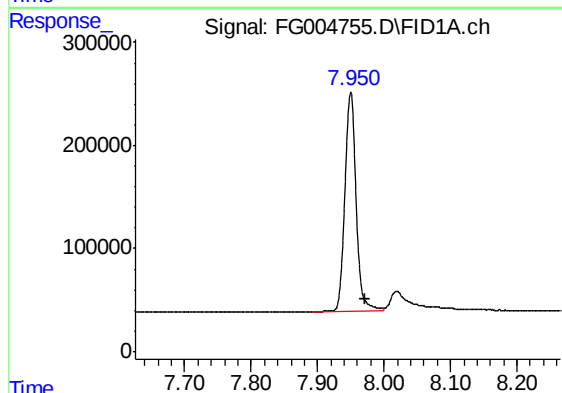


#4 N-TETRADECANE

R.T.: 7.950 min
Delta R.T.: -0.021 min
Response: 2485764
Conc: 22.94 ug/ml

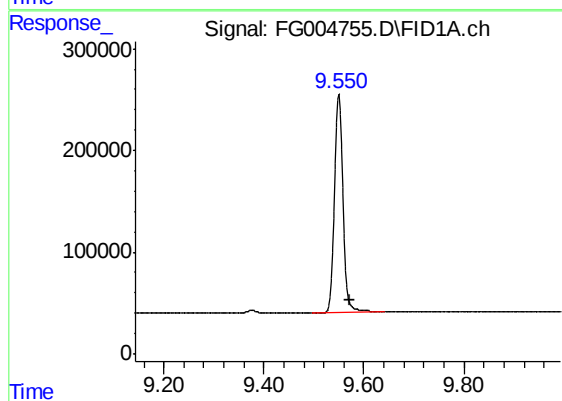


#5 N-HEXADECANE

R.T.: 9.550 min
Delta R.T.: -0.022 min
Response: 2541266
Conc: 22.71 ug/ml

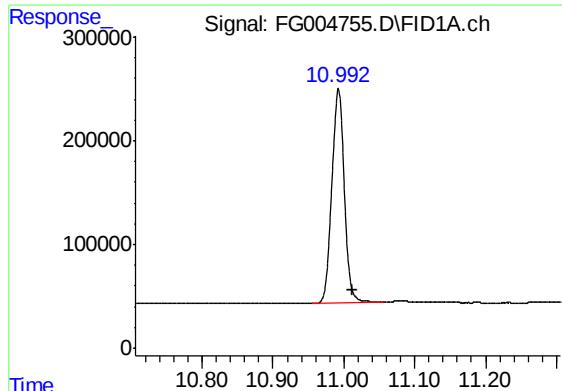


#6 N-OCTADECANE

R.T.: 10.993 min
Delta R.T.: -0.020 min
Response: 2523213
Conc: 22.25 ug/ml

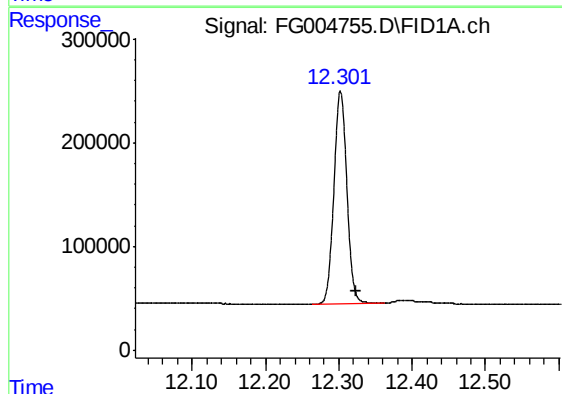


#7 N-EICOSANE

R.T.: 12.302 min
Delta R.T.: -0.021 min
Response: 2514610
Conc: 22.00 ug/ml

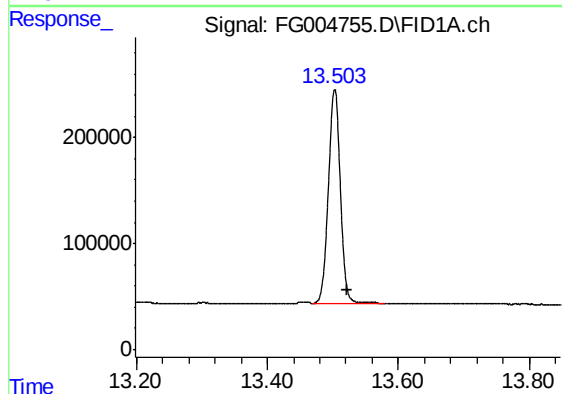


#8 N-DOCOSANE

R.T.: 13.503 min
Delta R.T.: -0.019 min
Response: 2559421
Conc: 22.39 ug/ml

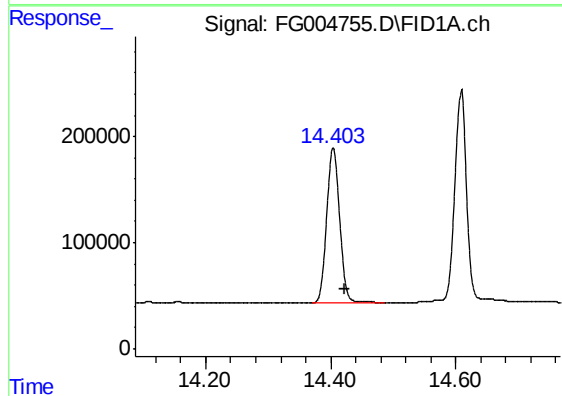


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.404 min
Delta R.T.: -0.019 min
Response: 2109112
Conc: 20.45 ug/ml

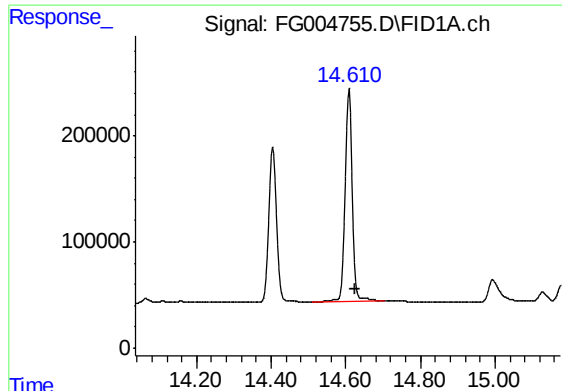


#10 N-TETRACOSANE

R.T.: 14.609 min
Delta R.T.: -0.016 min
Response: 2663609
Conc: 23.06 ug/ml

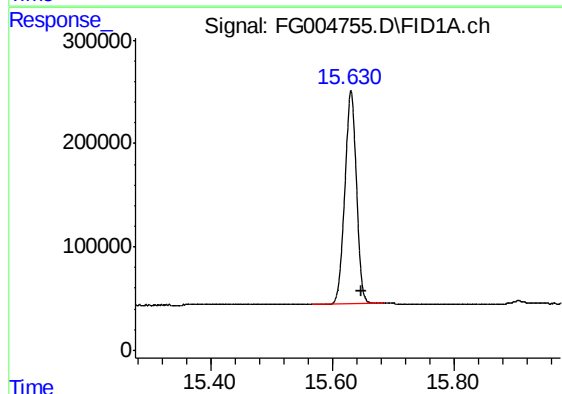

#11 N-HEXACOSANE

R.T.: 15.631 min
Delta R.T.: -0.016 min
Response: 2742564
Conc: 23.92 ug/ml

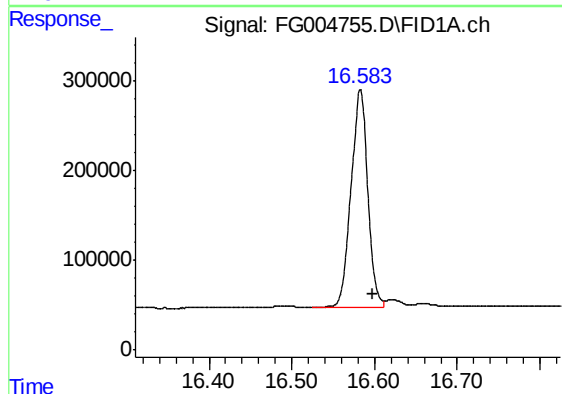

#12 N-OCTACOSANE

R.T.: 16.583 min
Delta R.T.: -0.014 min
Response: 3411354
Conc: 29.49 ug/ml m