

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041921\
Data File : FG007871.D
Signal(s) : FID1A.ch
Acq On : 19 Apr 2021 13:43
Operator : DD\AJ
Sample : M2077-07 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-21-COMP

Integration File: autoint1.e
Quant Time: Apr 20 01:52:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040521.M
Quant Title :
QLast Update : Tue Apr 06 03:05:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.788	778919	5.216 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041921\
Data File : FG007871.D
Signal(s) : FID1A.ch
Acq On : 19 Apr 2021 13:43
Operator : DD\AJ
Sample : M2077-07 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-21-COMP

Integration File: autoint1.e
Quant Time: Apr 20 01:52:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040521.M
Quant Title :
QLast Update : Tue Apr 06 03:05:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

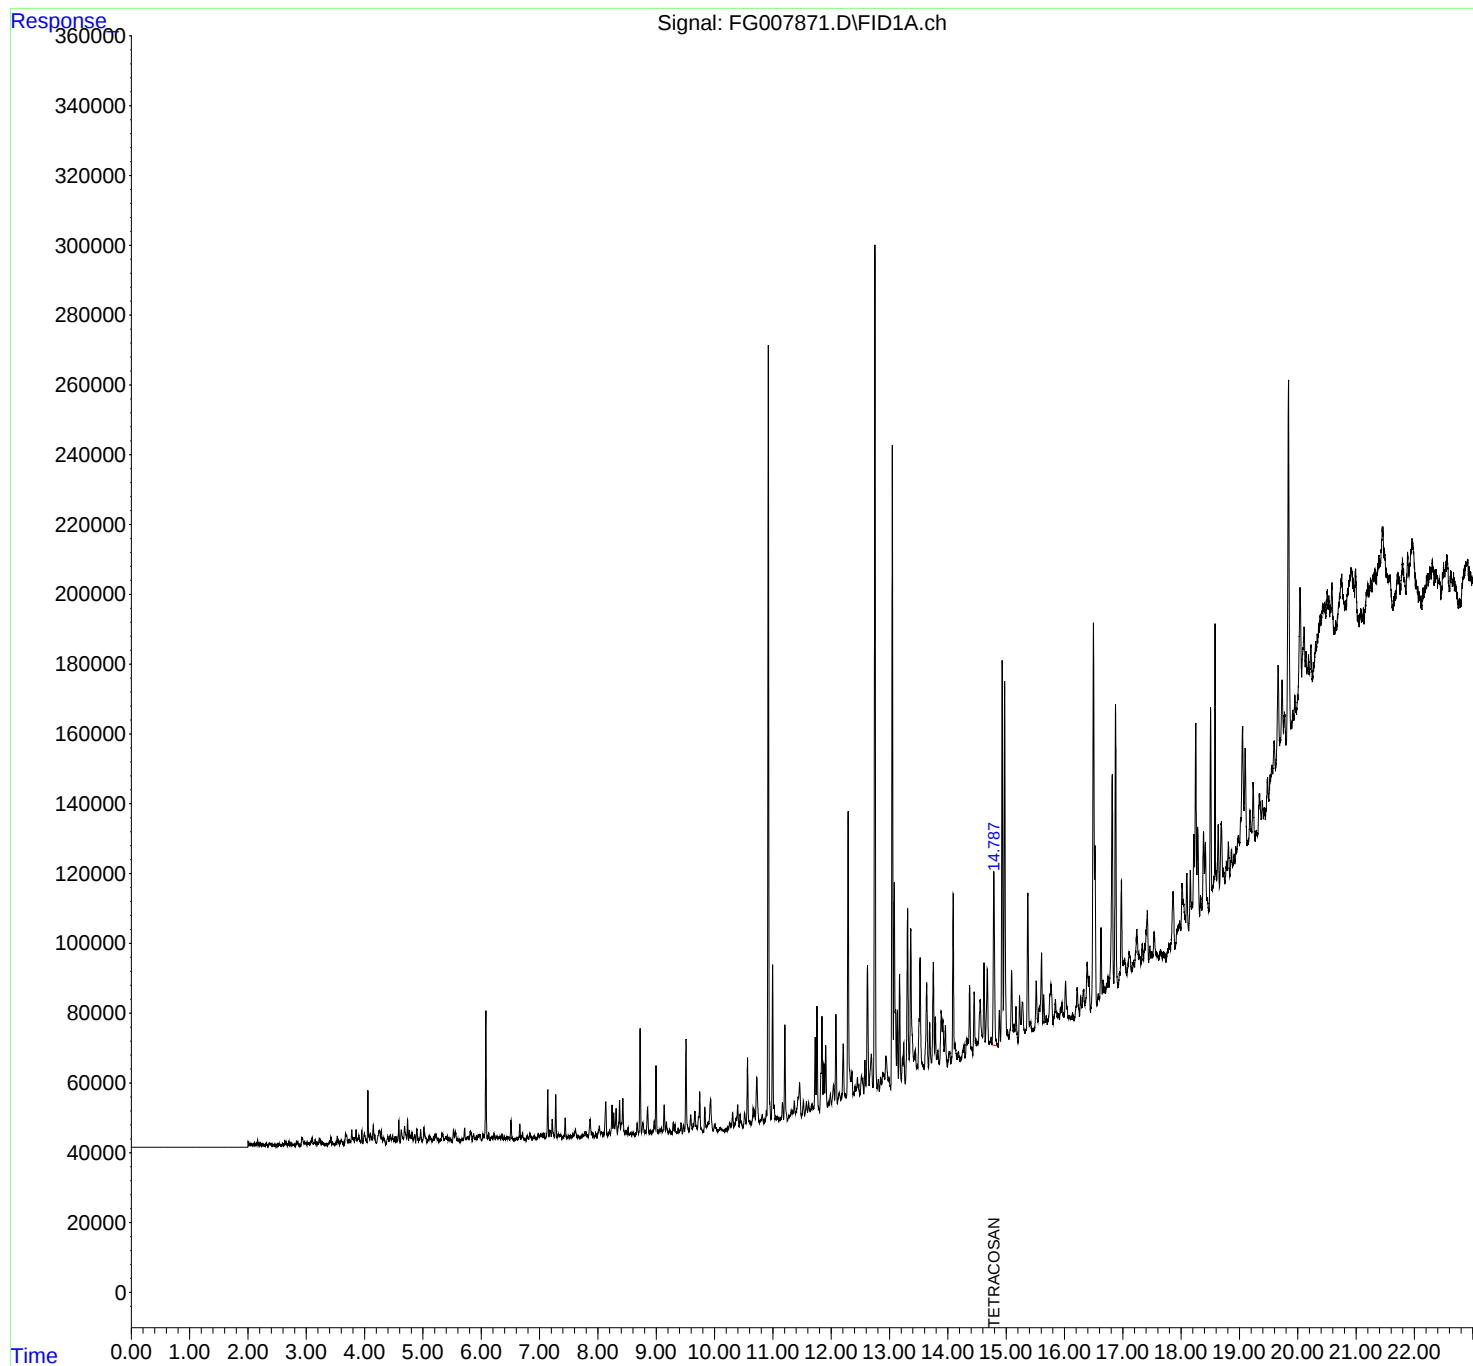

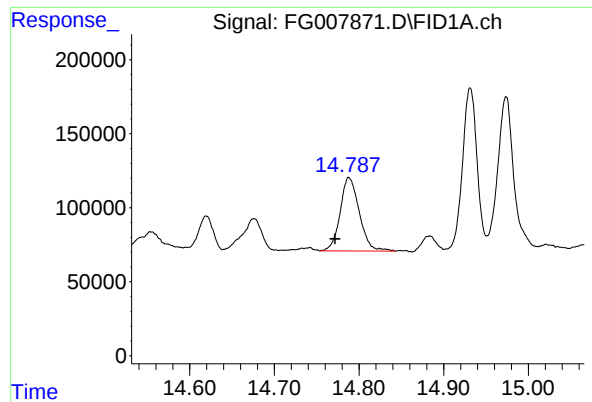

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.788 min
Delta R.T.: 0.016 min
Response: 778919
Conc: 5.22 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-21-COMP