

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042121\
Data File : FG007875.D
Signal(s) : FID1A.ch
Acq On : 21 Apr 2021 18:35
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 22 01:55:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.854	100172	0.701 ug/ml
14) N-DOTRIACONTANE	18.690	176794	1.296 ug/ml
15) N-TETRATRIACONTANE	19.475	98028	0.763 ug/ml
16) N-HEXATRIACONTANE	20.263	182431	1.559 ug/ml
18) N-TETRACONTANE	22.005f	316127	2.886 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042121\
Data File : FG007875.D
Signal(s) : FID1A.ch
Acq On : 21 Apr 2021 18:35
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Apr 22 01:55:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

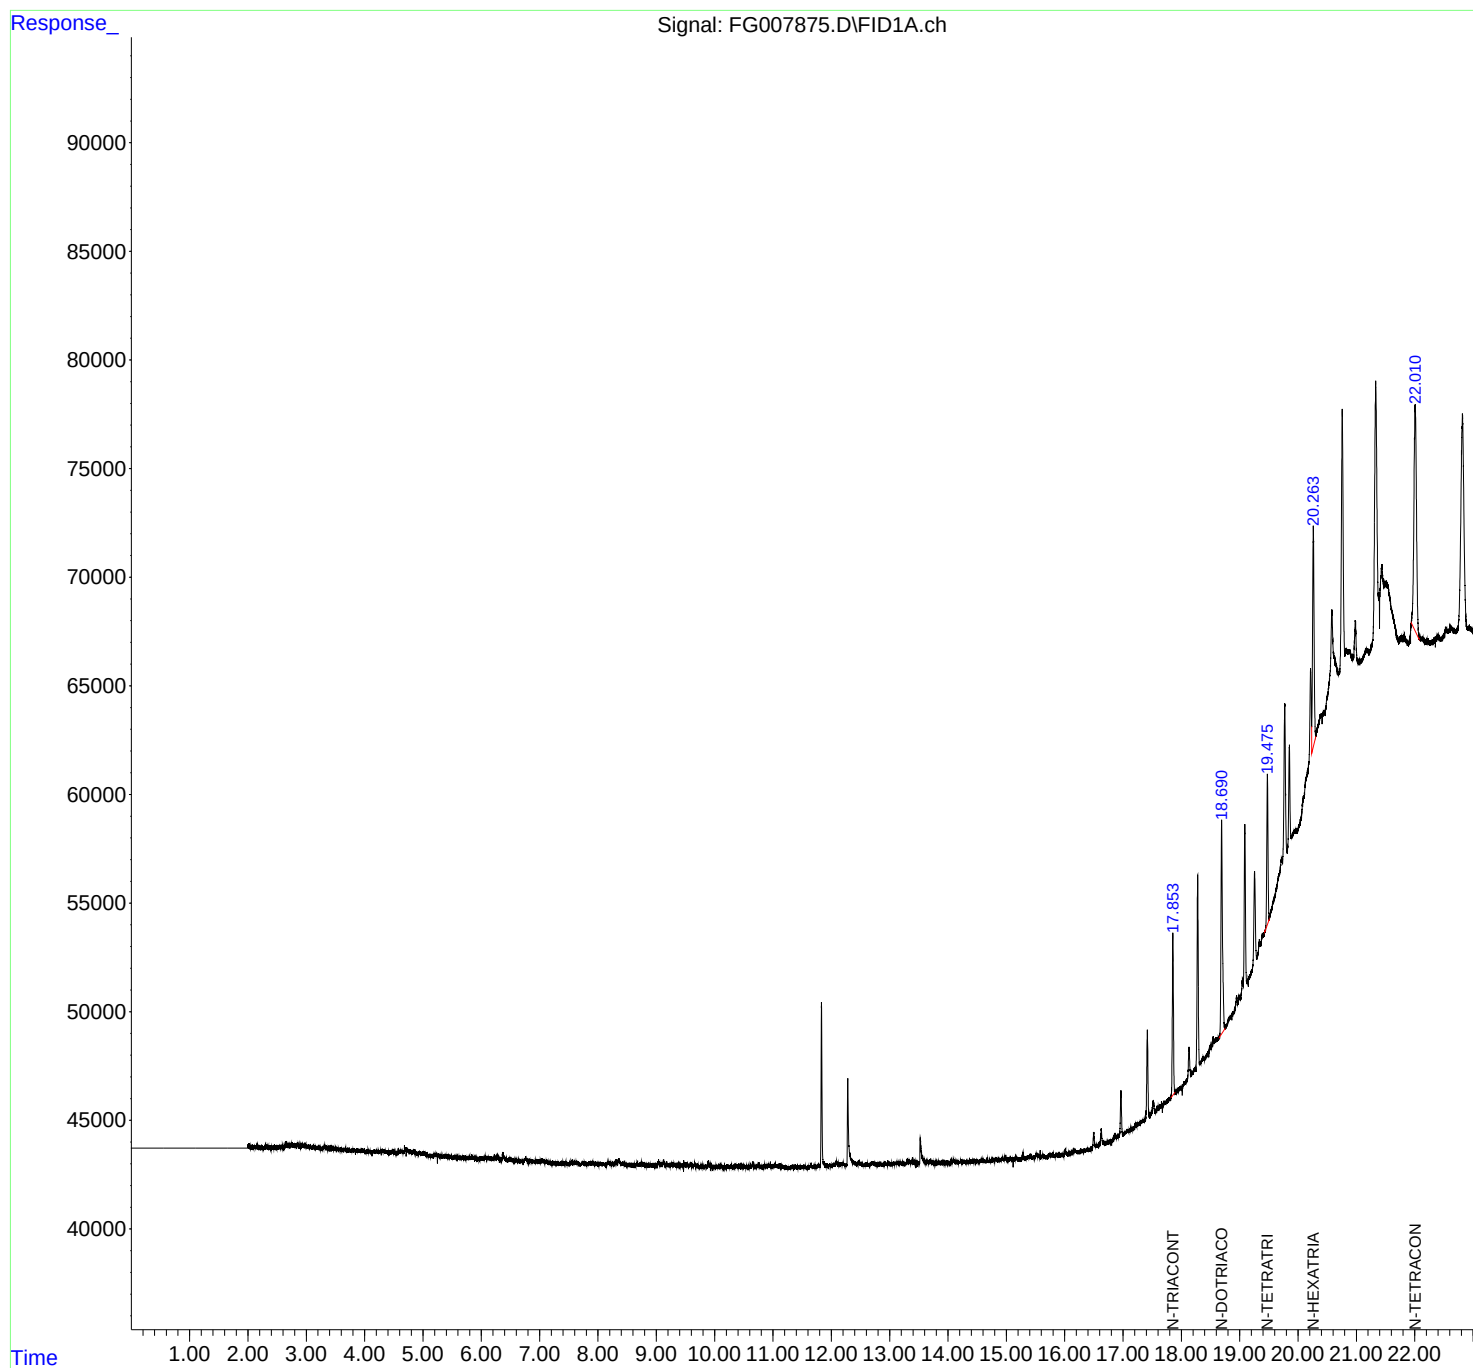


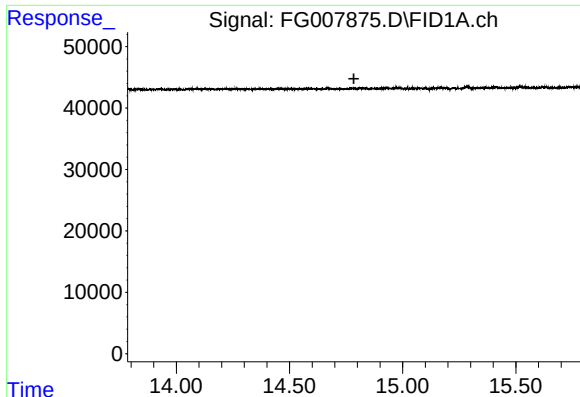

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.784 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

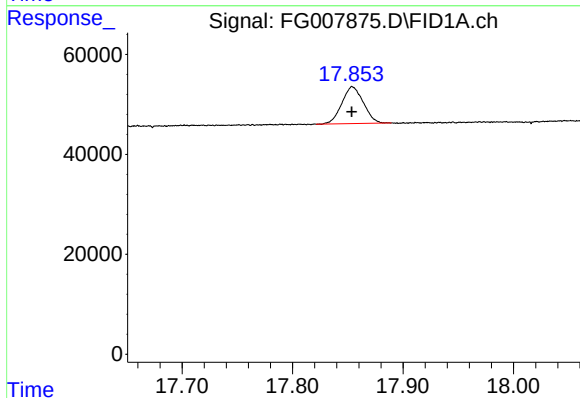


#13 N-TRIACONTANE

R.T.: 17.854 min
Delta R.T.: 0.000 min
Response: 100172
Conc: 0.70 ug/ml

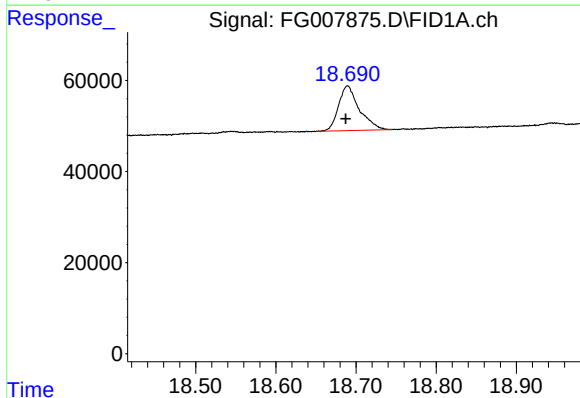


#14 N-DOTRIACONTANE

R.T.: 18.690 min
Delta R.T.: 0.002 min
Response: 176794
Conc: 1.30 ug/ml

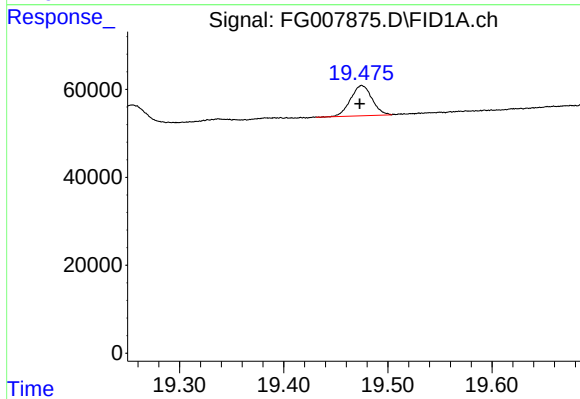

#15 N-TETRATRIACONTANE


R.T.: 19.475 min
Delta R.T.: 0.002 min
Response: 98028
Conc: 0.76 ug/ml

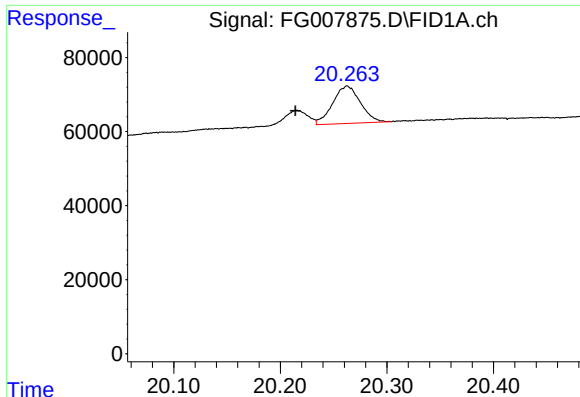

#16 N-HEXATRIACONTANE

R.T.: 20.263 min
Delta R.T.: 0.049 min
Response: 182431
Conc: 1.56 ug/ml

Instrument :
FID_G
ClientSampleId :

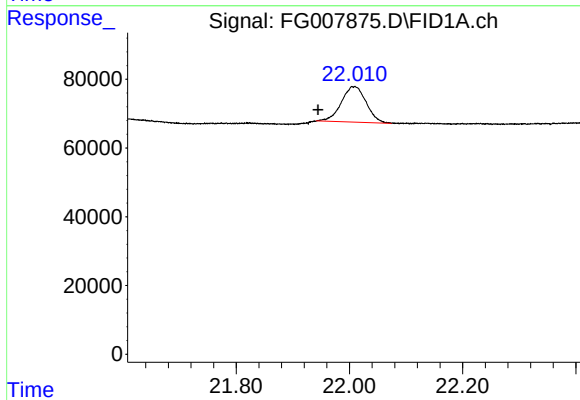

#18 N-TETRACONTANE

R.T.: 22.005 min
Delta R.T.: 0.060 min
Response: 316127
Conc: 2.89 ug/ml