

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042219\
 Data File : FG004767.D
 Signal(s) : FID1A.ch
 Acq On : 22 Apr 2019 13:20
 Operator : AJ\SJ
 Sample : PB119086BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 22 22:17:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.402	1580461	15.322 ug/ml
Target Compounds			
2) N-DECANE	4.134	1986048	18.815 ug/ml
3) N-DODECANE	6.155	2032505	19.291 ug/ml
4) N-TETRADECANE	7.948	2049063	18.912 ug/ml
5) N-HEXADECANE	9.549	2048877	18.313 ug/ml
6) N-OCTADECANE	10.991	2011306	17.732 ug/ml
7) N-EICOSANE	12.302	1973984	17.268 ug/ml
8) N-DOCOSANE	13.501	1942664	16.994 ug/ml
10) N-TETRACOSANE	14.607	1968494	17.041 ug/ml
11) N-HEXACOSANE	15.628	1929922	16.836 ug/ml
12) N-OCTACOSANE	16.581	1954270	16.893 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042219\
Data File : FG004767.D
Signal(s) : FID1A.ch
Acq On : 22 Apr 2019 13:20
Operator : AJ\SJ
Sample : PB119086BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 22 22:17:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

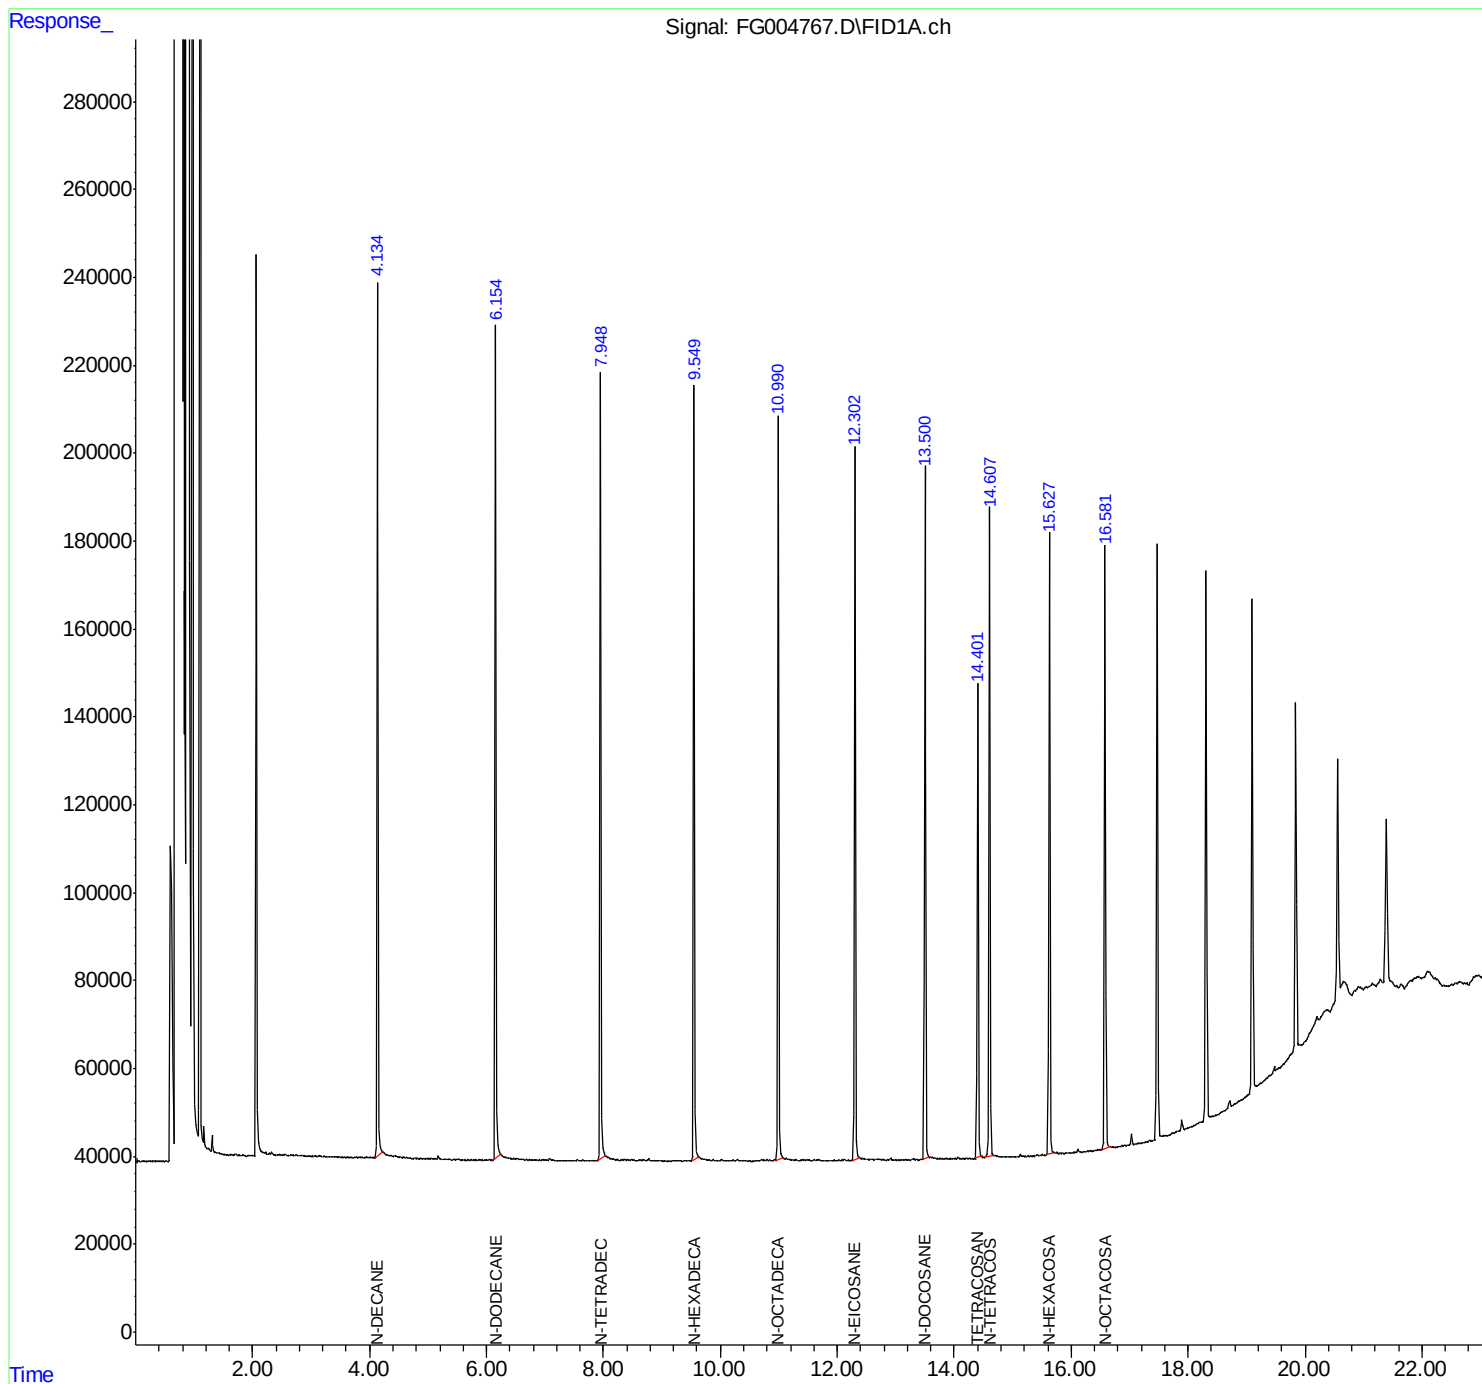

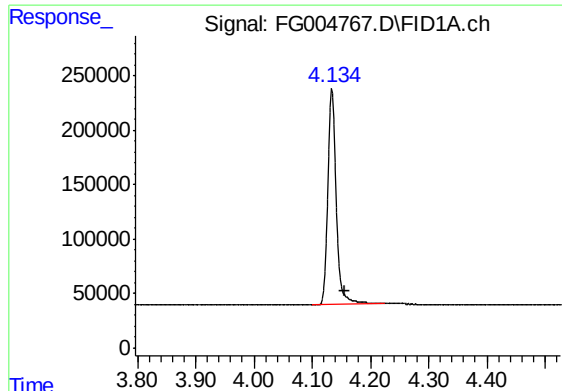


#2 N-DECANE

R.T.: 4.134 min
Delta R.T.: -0.023 min
Response: 1986048
Conc: 18.82 ug/ml

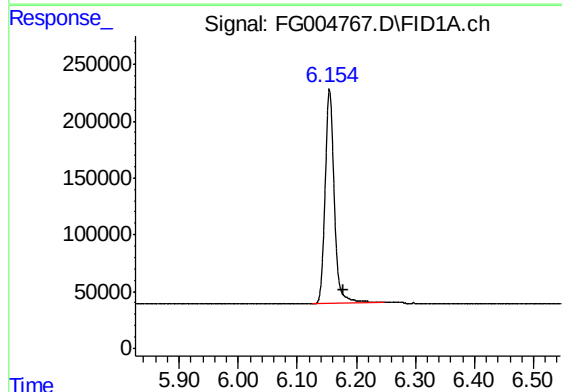


#3 N-DODECANE

R.T.: 6.155 min
Delta R.T.: -0.023 min
Response: 2032505
Conc: 19.29 ug/ml

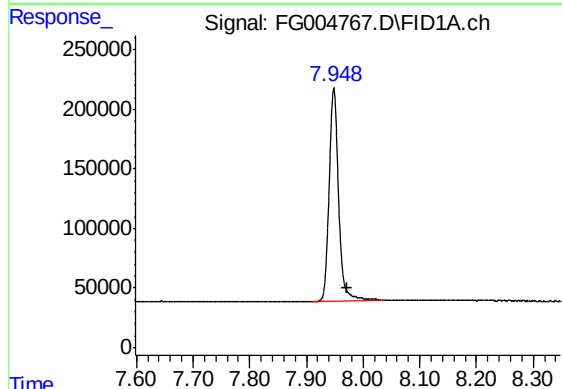


#4 N-TETRADECANE

R.T.: 7.948 min
Delta R.T.: -0.023 min
Response: 2049063
Conc: 18.91 ug/ml

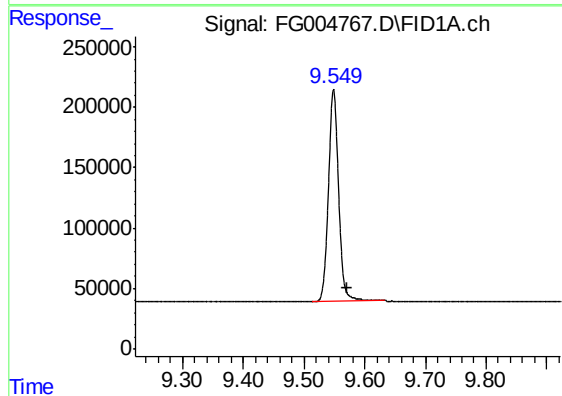


#5 N-HEXADECANE

R.T.: 9.549 min
Delta R.T.: -0.023 min
Response: 2048877
Conc: 18.31 ug/ml

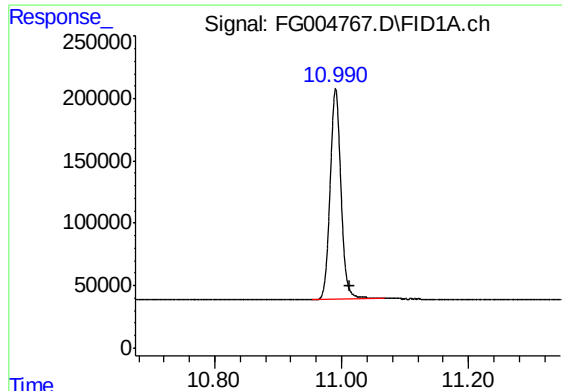


#6 N-OCTADECANE

R.T.: 10.991 min
Delta R.T.: -0.022 min
Response: 2011306
Conc: 17.73 ug/ml

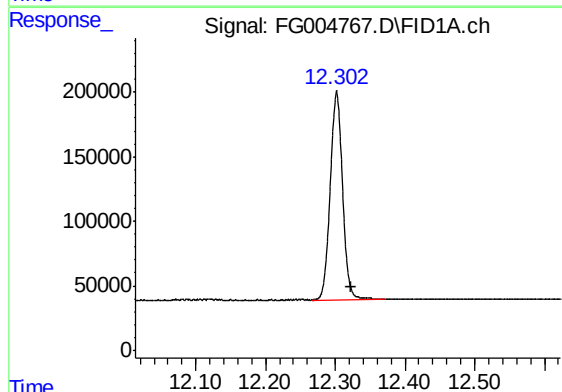


#7 N-EICOSANE

R.T.: 12.302 min
Delta R.T.: -0.021 min
Response: 1973984
Conc: 17.27 ug/ml

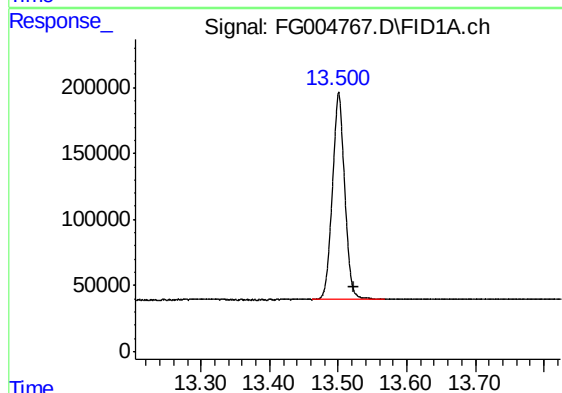


#8 N-DOCOSANE

R.T.: 13.501 min
Delta R.T.: -0.022 min
Response: 1942664
Conc: 16.99 ug/ml

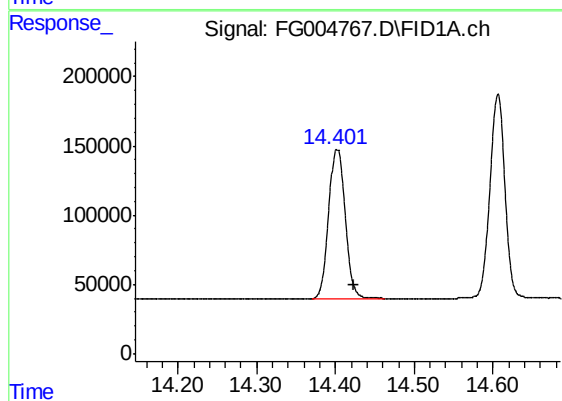


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.402 min
Delta R.T.: -0.020 min
Response: 1580461
Conc: 15.32 ug/ml

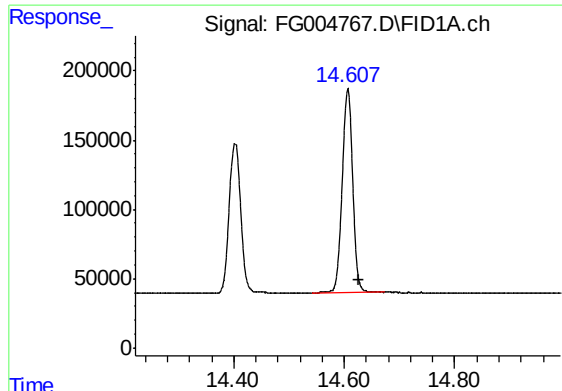


#10 N-TETRACOSANE

R.T.: 14.607 min
Delta R.T.: -0.018 min
Response: 1968494
Conc: 17.04 ug/ml

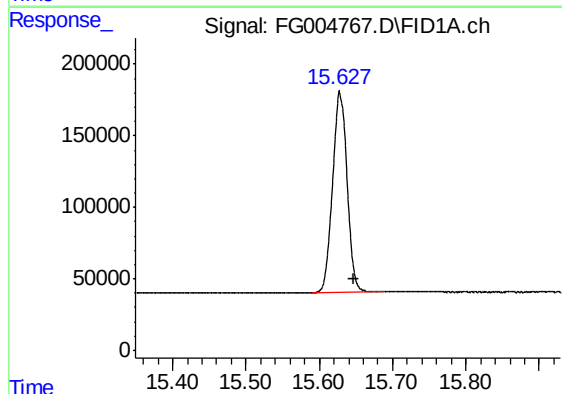

#11 N-HEXACOSANE

R.T.: 15.628 min
Delta R.T.: -0.019 min
Response: 1929922
Conc: 16.84 ug/ml

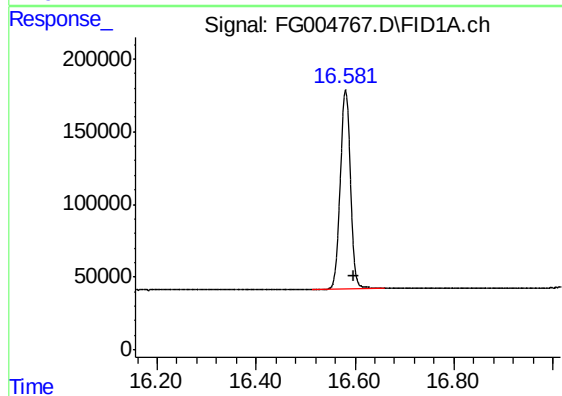

#12 N-OCTACOSANE

R.T.: 16.581 min
Delta R.T.: -0.016 min
Response: 1954270
Conc: 16.89 ug/ml