

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042321\
Data File : FG007892.D
Signal(s) : FID1A.ch
Acq On : 23 Apr 2021 16:41
Operator : DD\AJ
Sample : M2131-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 23 23:42:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.781	2768178	20.793 ug/ml
Target Compounds			
4) N-TETRADECANE	8.368f	210633	1.349 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042321\
Data File : FG007892.D
Signal(s) : FID1A.ch
Acq On : 23 Apr 2021 16:41
Operator : DD\AJ
Sample : M2131-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 23 23:42:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

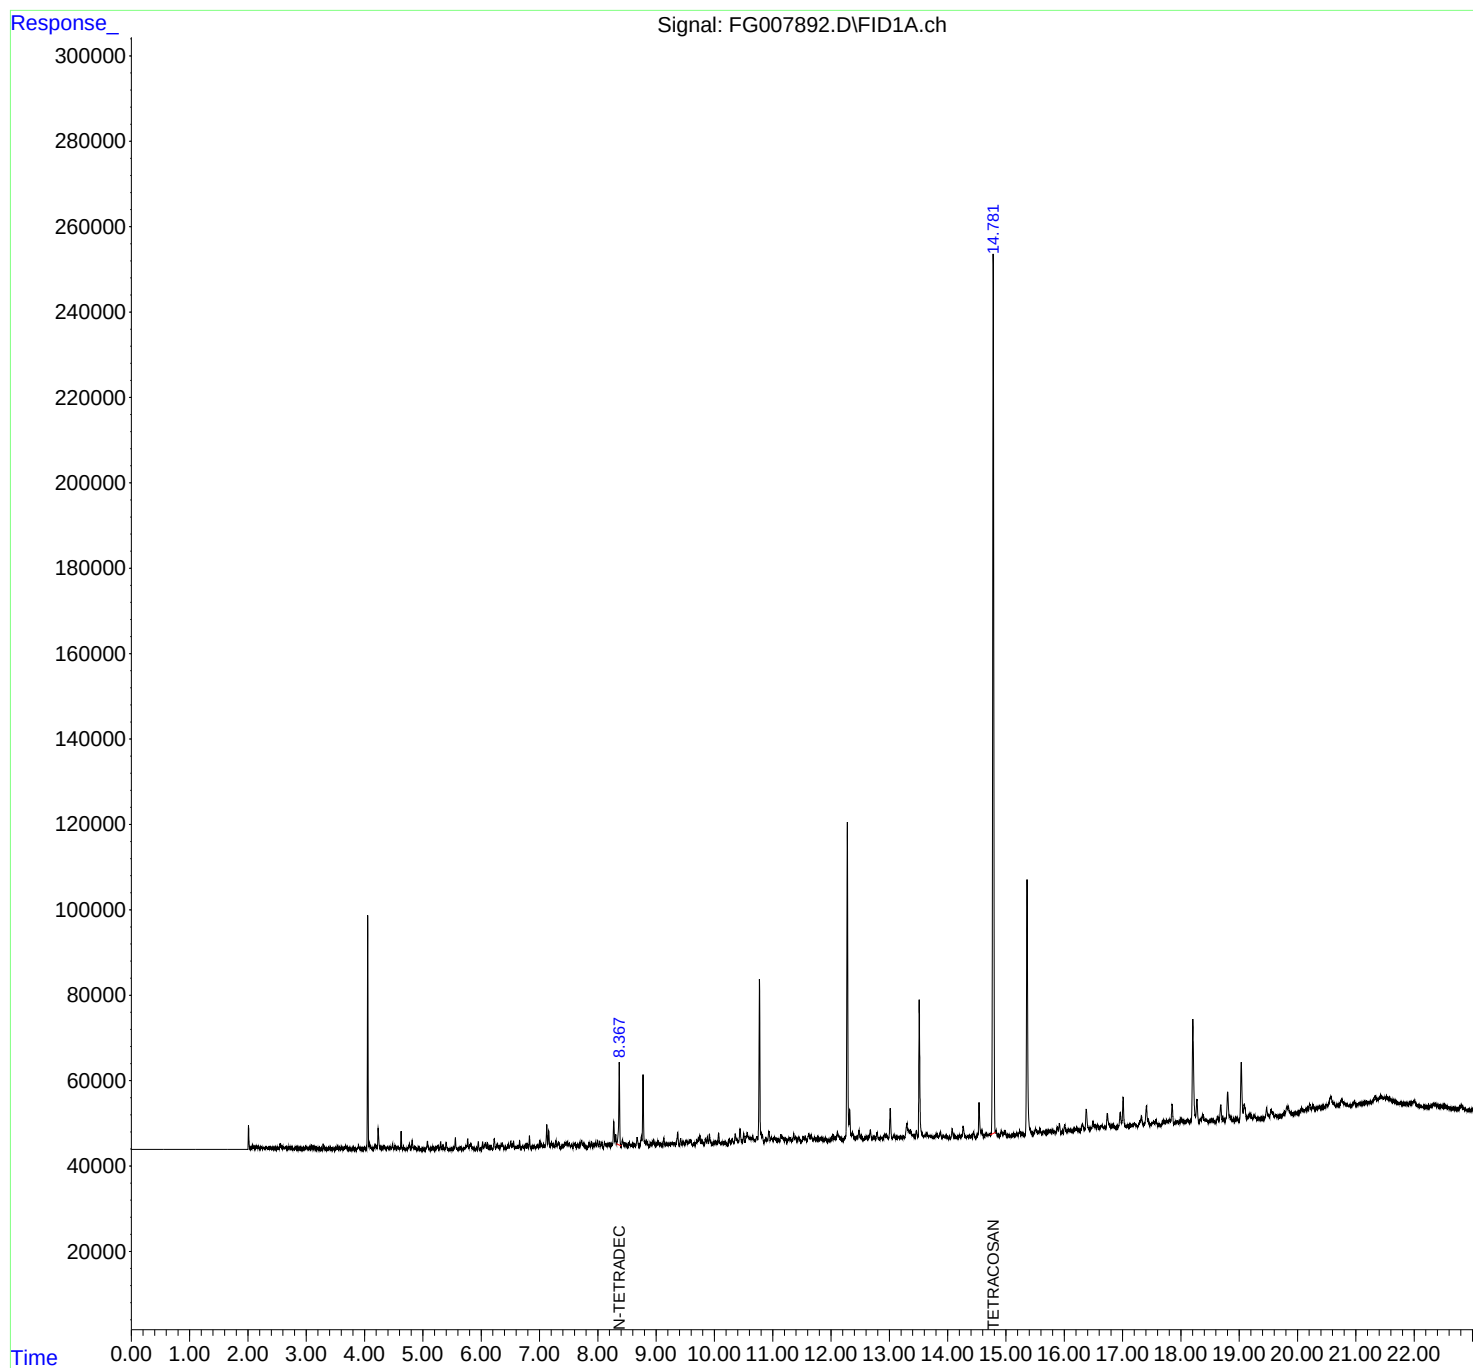


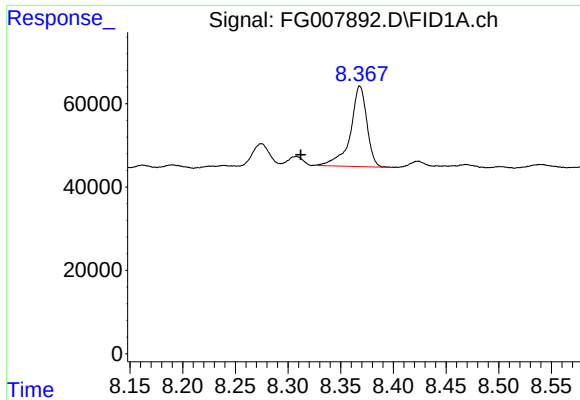

#4 N-TETRADECANE

R.T.: 8.368 min
Delta R.T.: 0.056 min
Response: 210633
Conc: 1.35 ug/ml

Instrument :
FID_G
ClientSampleId :

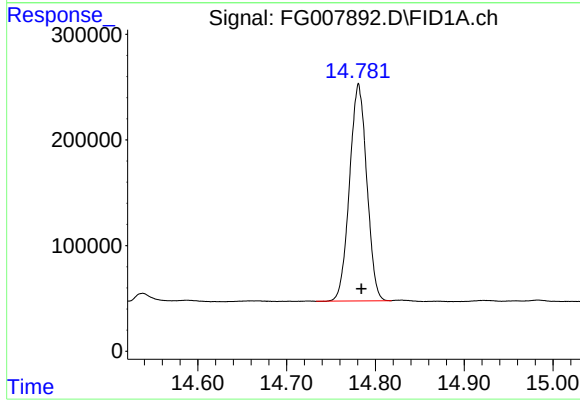

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.781 min
Delta R.T.: -0.003 min
Response: 2768178
Conc: 20.79 ug/ml