

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042423\
 Data File : FG011853.D
 Signal(s) : FID1A.ch
 Acq On : 24 Apr 2023 13:57
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Apr 24 18:03:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041323.M
 Quant Title :
 QLast Update : Wed Apr 12 18:20:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.033	5176485	50.663 ug/ml
Target Compounds			
2) N-DECANE	4.559	6567158	52.597 ug/ml
3) N-DODECANE	6.731	6539191	52.503 ug/ml
4) N-TETRADECANE	8.561	6406862	52.933 ug/ml
5) N-HEXADECANE	10.173	6395551	51.674 ug/ml
6) N-OCTADECANE	11.618	6282893	51.227 ug/ml
7) N-EICOSANE	12.931	6137752	50.876 ug/ml
8) N-DOCOSANE	14.132	5889988	50.917 ug/ml
10) N-TETRACOSANE	15.237	5895854	50.756 ug/ml
11) N-HEXACOSANE	16.261	5730075	50.920 ug/ml
12) N-OCTACOSANE	17.214	5637528	51.388 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042423\
Data File : FG011853.D
Signal(s) : FID1A.ch
Acq On : 24 Apr 2023 13:57
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Apr 24 18:03:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041323.M
Quant Title :
QLast Update : Wed Apr 12 18:20:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

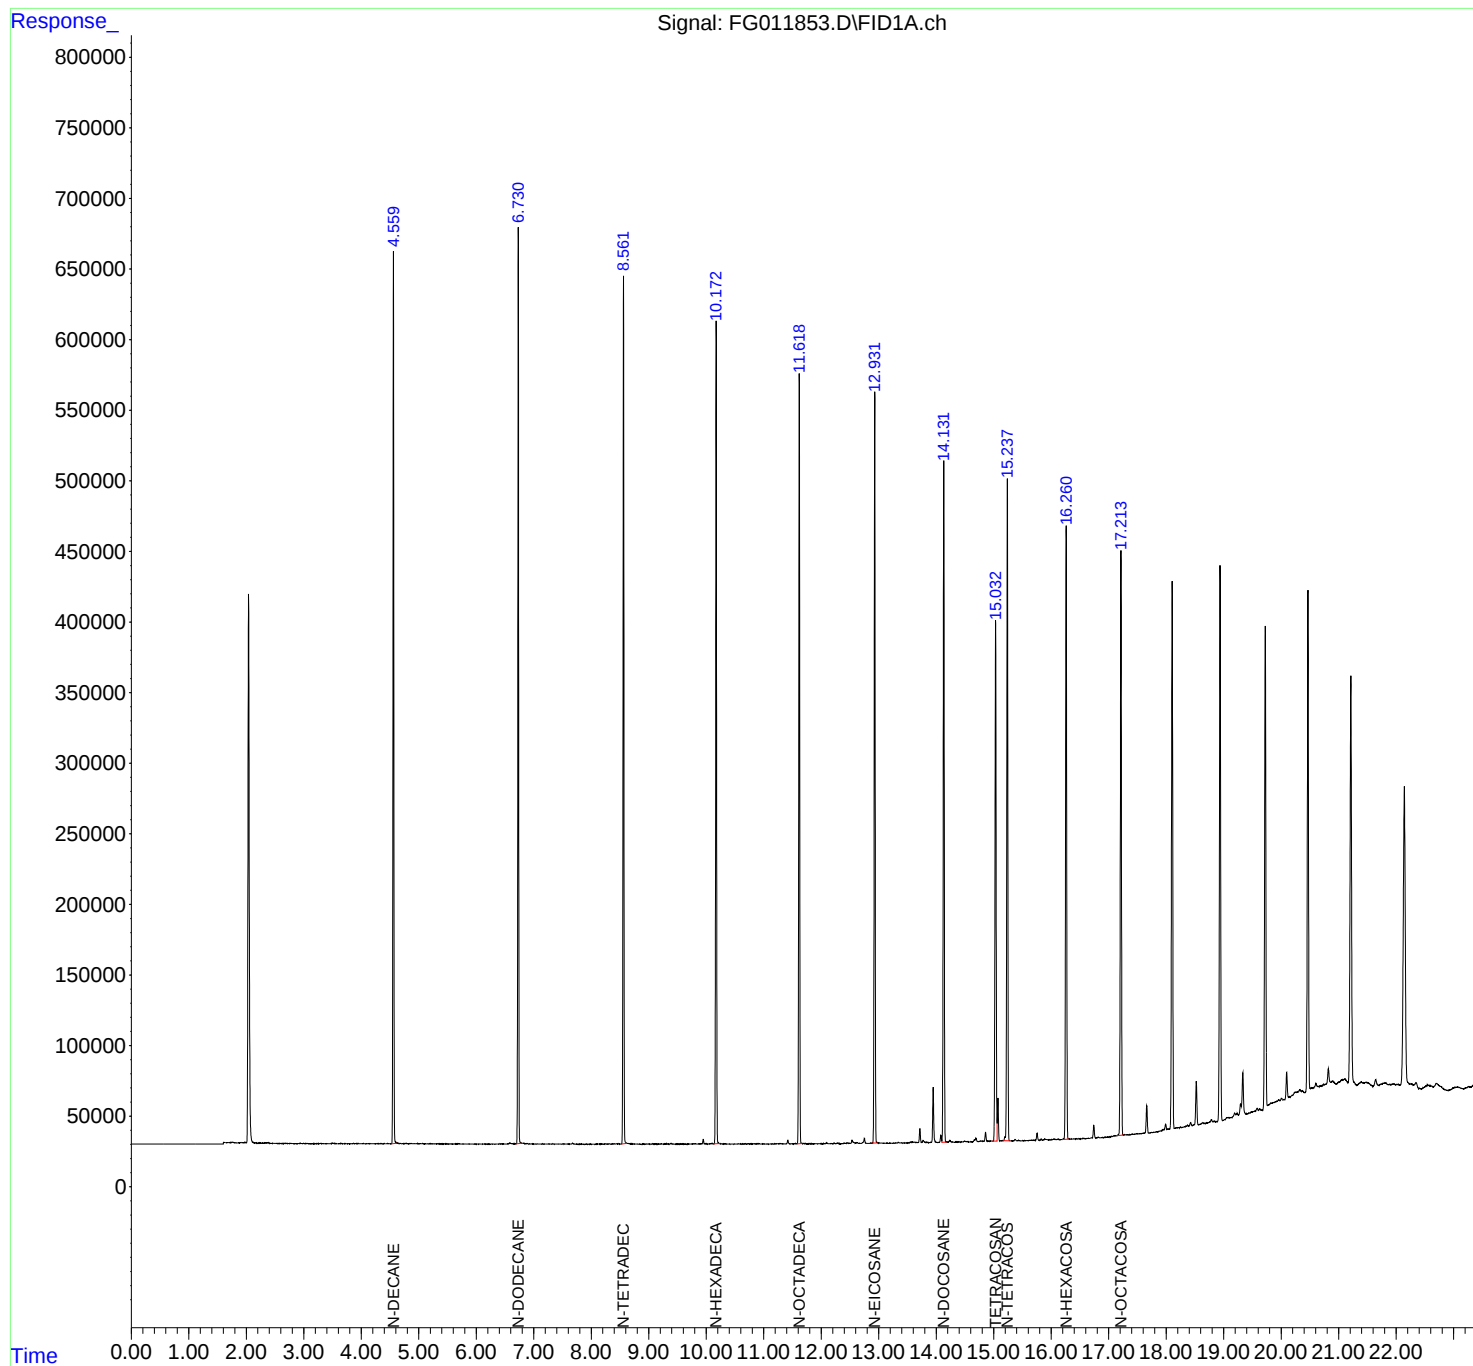


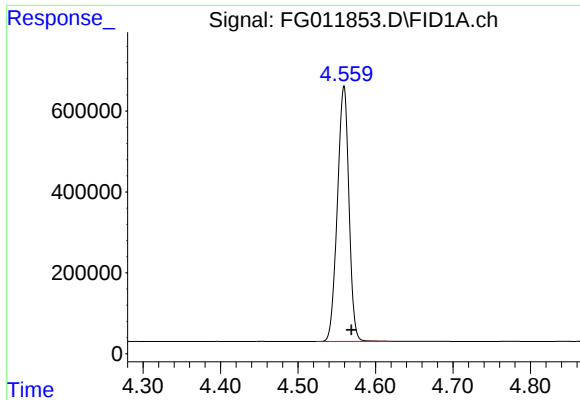

#2 N-DECANE


R.T.: 4.559 min
Delta R.T.: -0.009 min
Response: 6567158
Conc: 52.60 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

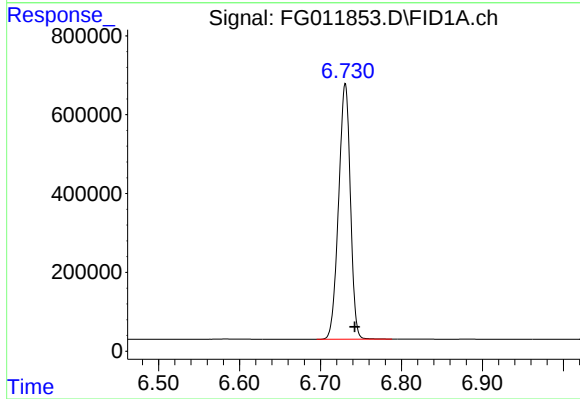


#3 N-DODECANE

R.T.: 6.731 min
Delta R.T.: -0.012 min
Response: 6539191
Conc: 52.50 ug/ml

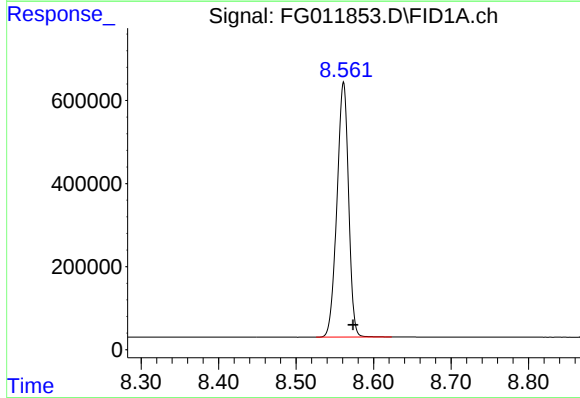


#4 N-TETRADECANE

R.T.: 8.561 min
Delta R.T.: -0.012 min
Response: 6406862
Conc: 52.93 ug/ml

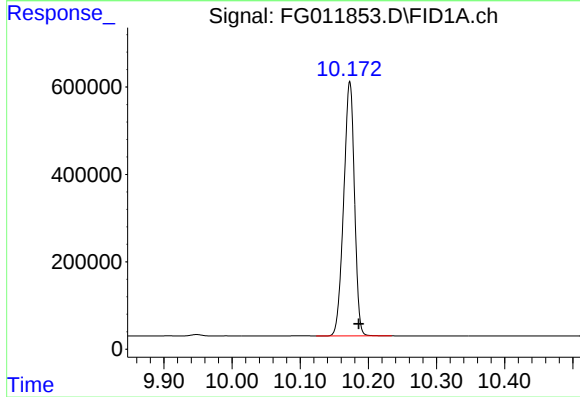

#5 N-HEXADECANE


R.T.: 10.173 min
Delta R.T.: -0.013 min
Response: 6395551
Conc: 51.67 ug/ml

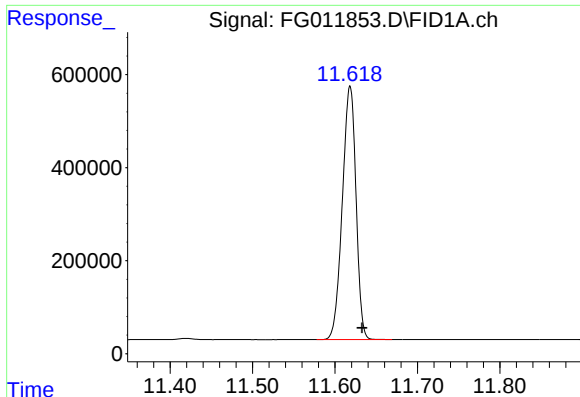

#6 N-OCTADECANE


R.T.: 11.618 min
Delta R.T.: -0.015 min
Response: 6282893
Conc: 51.23 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

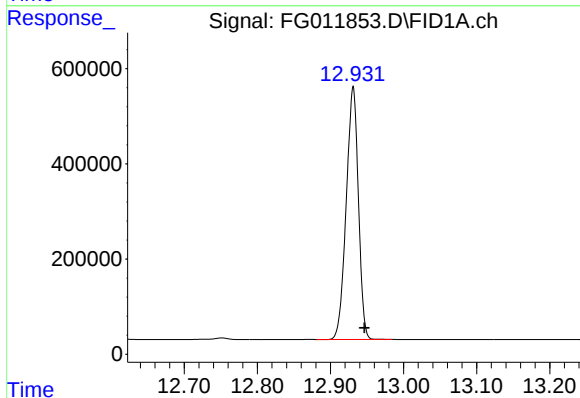


#7 N-EICOSANE

R.T.: 12.931 min
Delta R.T.: -0.015 min
Response: 6137752
Conc: 50.88 ug/ml

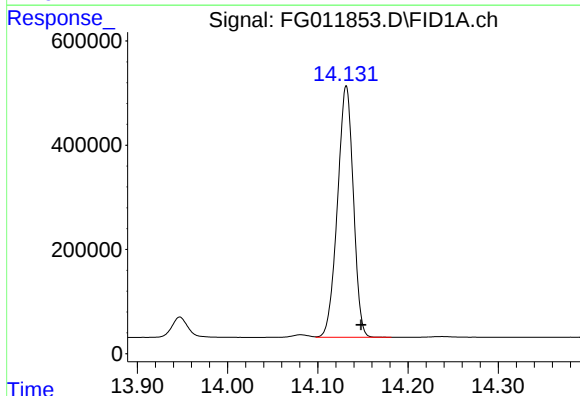


#8 N-DOCOSANE

R.T.: 14.132 min
Delta R.T.: -0.016 min
Response: 5889988
Conc: 50.92 ug/ml

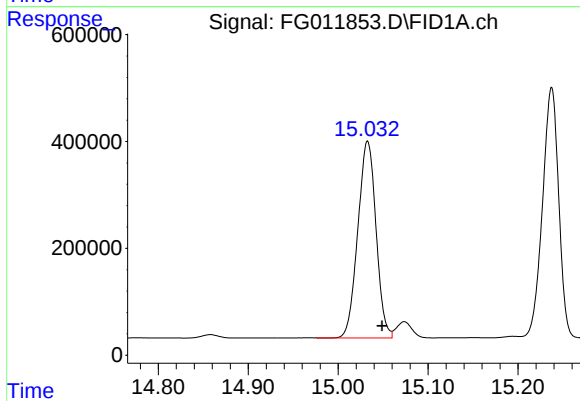

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.033 min
Delta R.T.: -0.016 min
Response: 5176485
Conc: 50.66 ug/ml

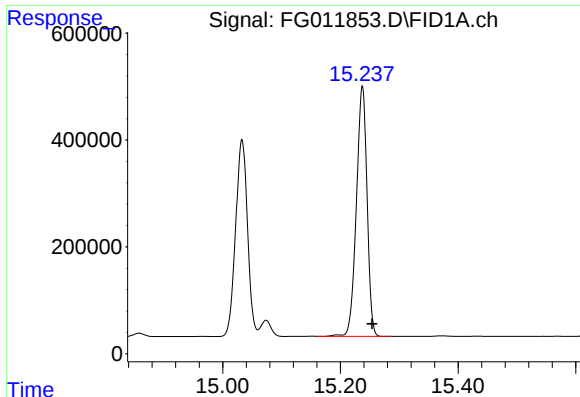

#10 N-TETRACOSANE


R.T.: 15.237 min
Delta R.T.: -0.016 min
Response: 5895854
Conc: 50.76 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

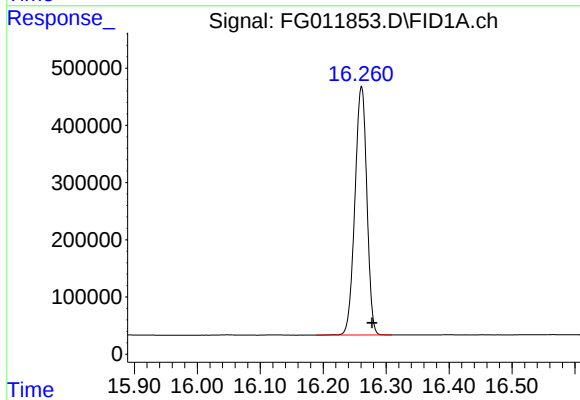

#11 N-HEXACOSANE

R.T.: 16.261 min
Delta R.T.: -0.017 min
Response: 5730075
Conc: 50.92 ug/ml

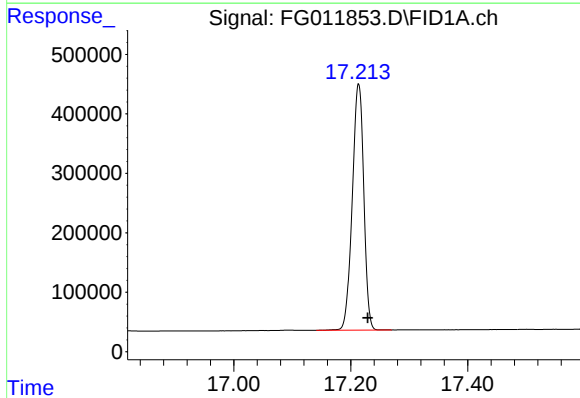

#12 N-OCTACOSANE

R.T.: 17.214 min
Delta R.T.: -0.016 min
Response: 5637528
Conc: 51.39 ug/ml