

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042524\
Data File : FG013688.D
Signal(s) : FID1A.ch
Acq On : 25 Apr 2024 11:52
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 26 05:11:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041124.M
Quant Title :
QLast Update : Thu Apr 11 13:37:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.753	3055192	24.047 ug/ml
12)	N-OCTACOSANE	17.250	3127113	24.259 ug/ml
13)	N-TRIACONTANE	18.137	56103	0.432 ug/ml
14)	N-DOTRIACONTANE	18.972	68877	0.538 ug/ml
15)	N-TETRATRIACONTANE	19.758	49281	0.412 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042524\
Data File : FG013688.D
Signal(s) : FID1A.ch
Acq On : 25 Apr 2024 11:52
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 26 05:11:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041124.M
Quant Title :
QLast Update : Thu Apr 11 13:37:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

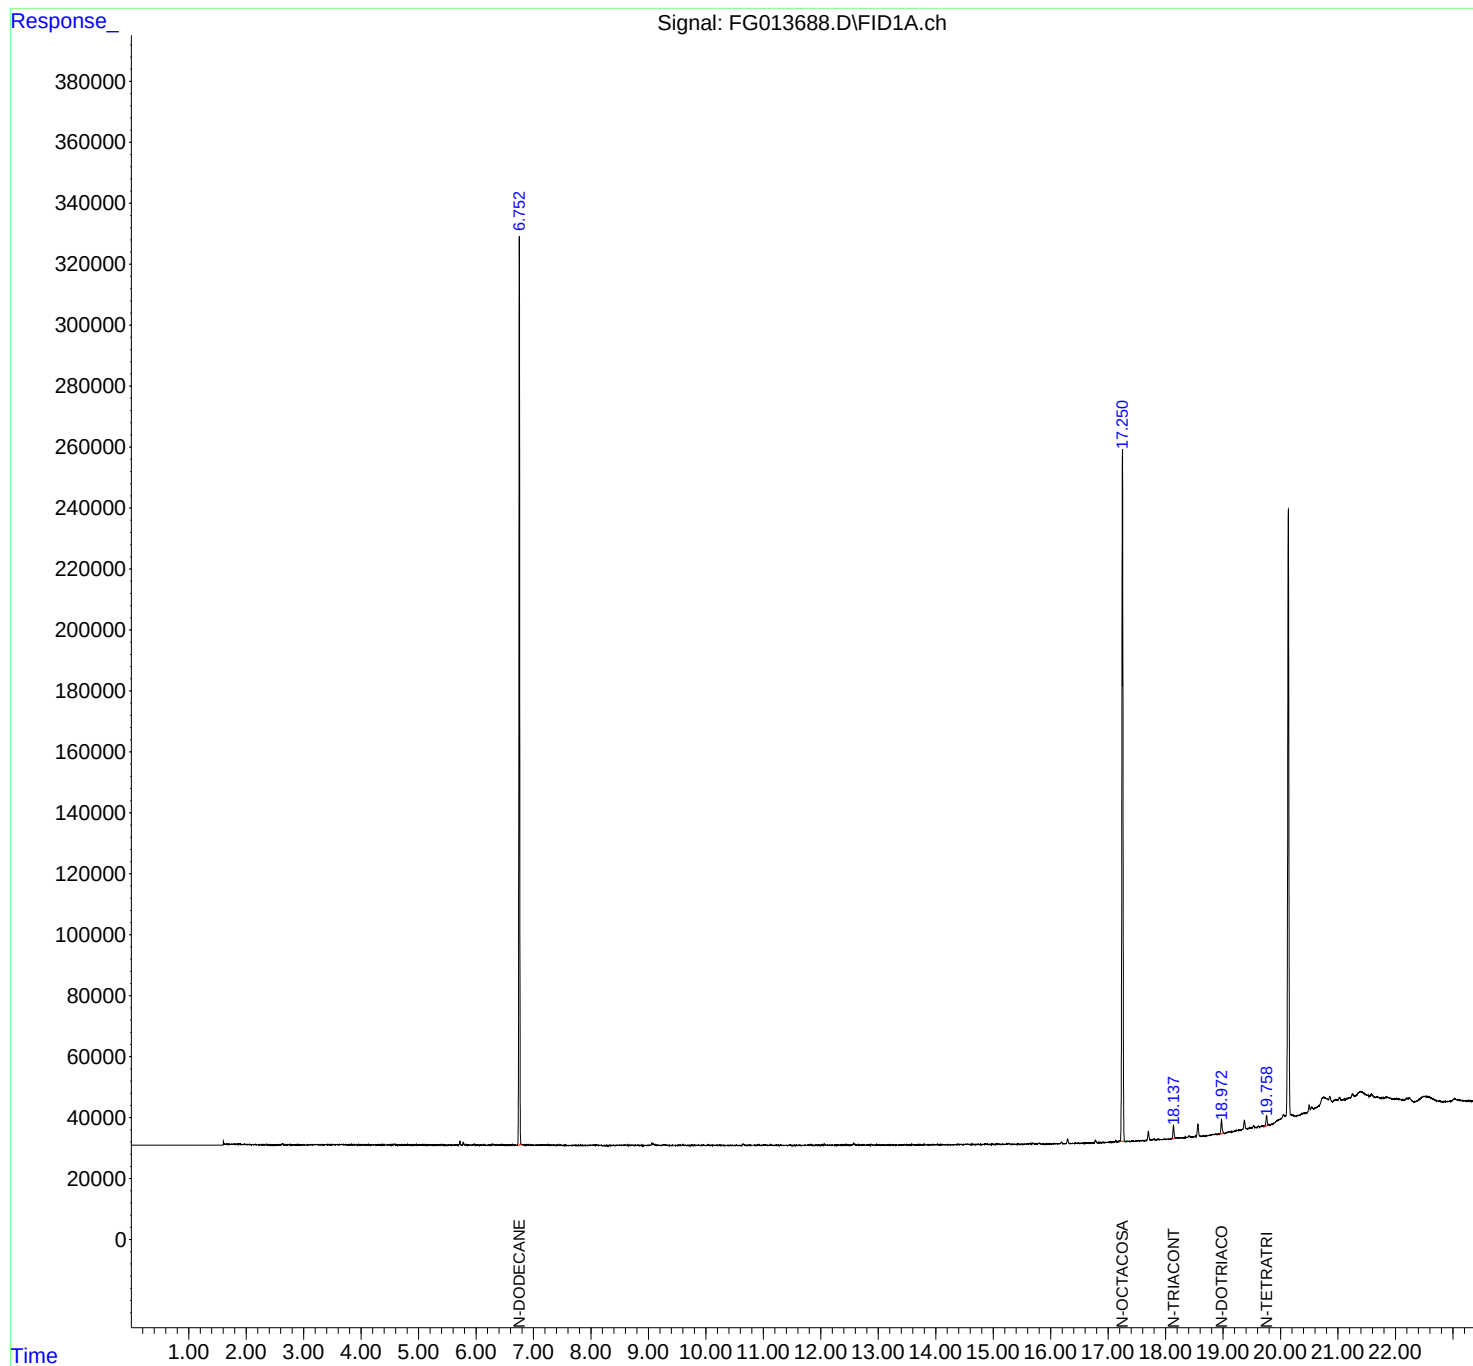


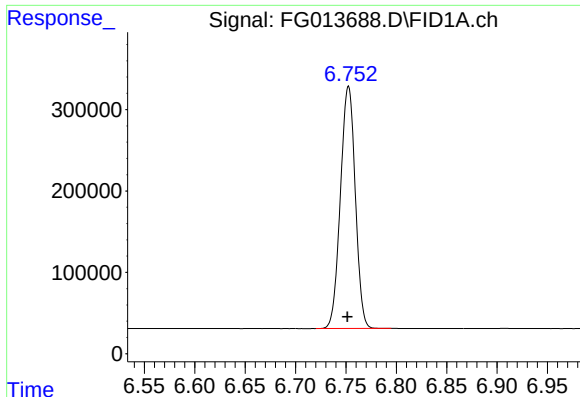

#3 N-DODECANE


R.T.: 6.753 min
Delta R.T.: 0.001 min
Response: 3055192
Conc: 24.05 ug/ml

Instrument :
FID_G
ClientSampleId :

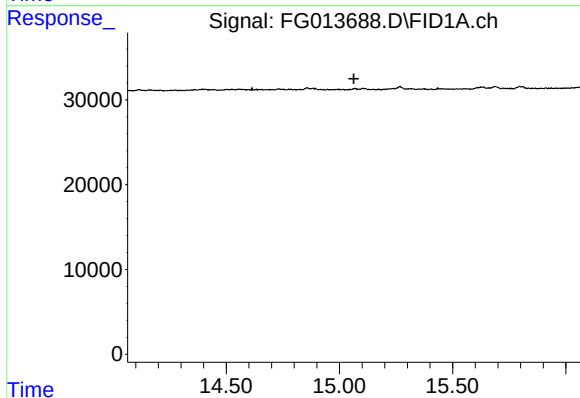


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.064 min
Response: 0
Conc: N.D.

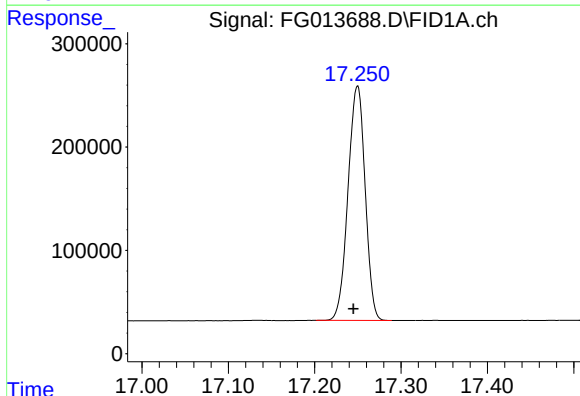


#12 N-OCTACOSANE

R.T.: 17.250 min
Delta R.T.: 0.005 min
Response: 3127113
Conc: 24.26 ug/ml

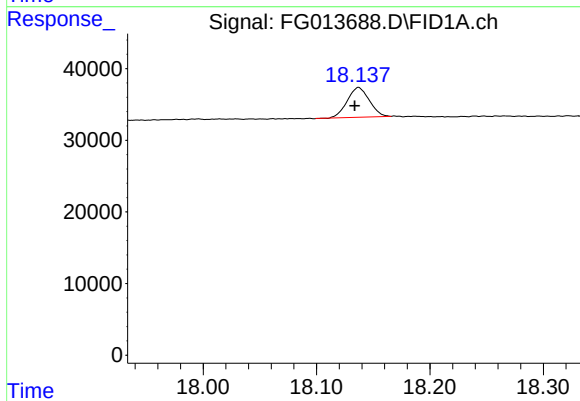

#13 N-TRIACONTANE


R.T.: 18.137 min
Delta R.T.: 0.003 min
Response: 56103
Conc: 0.43 ug/ml

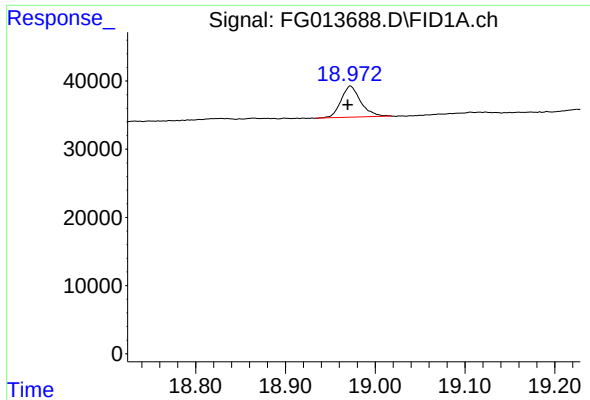

#14 N-DOTRIACONTANE

R.T.: 18.972 min
Delta R.T.: 0.003 min
Response: 68877
Conc: 0.54 ug/ml

Instrument :
FID_G
ClientSampleId :

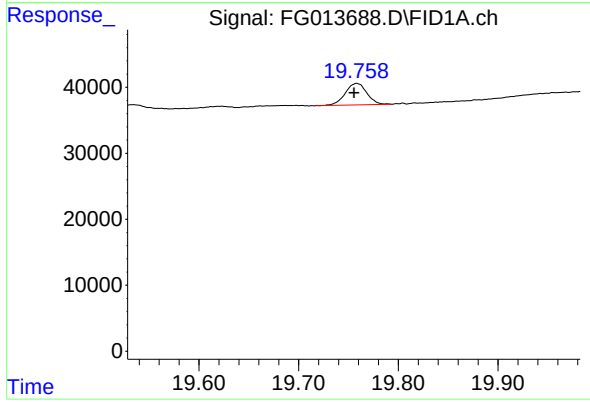

#15 N-TETRATRIACONTANE

R.T.: 19.758 min
Delta R.T.: 0.003 min
Response: 49281
Conc: 0.41 ug/ml