

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042619\
Data File : FG004832.D
Signal(s) : FID1A.ch
Acq On : 26 Apr 2019 21:20
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 03:53:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042619.M
Quant Title :
QLast Update : Sat Apr 27 03:52:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
12)	N-OCTACOSANE	16.579	35870	0.255 ug/ml
13)	N-TRIACONTANE	17.467	51067	0.377 ug/ml
14)	N-DOTRIACONTANE	18.306	46234	0.372 ug/ml
16)	N-HEXATRIACONTANE	19.876	20390	0.193 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042619\
Data File : FG004832.D
Signal(s) : FID1A.ch
Acq On : 26 Apr 2019 21:20
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 03:53:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042619.M
Quant Title :
QLast Update : Sat Apr 27 03:52:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

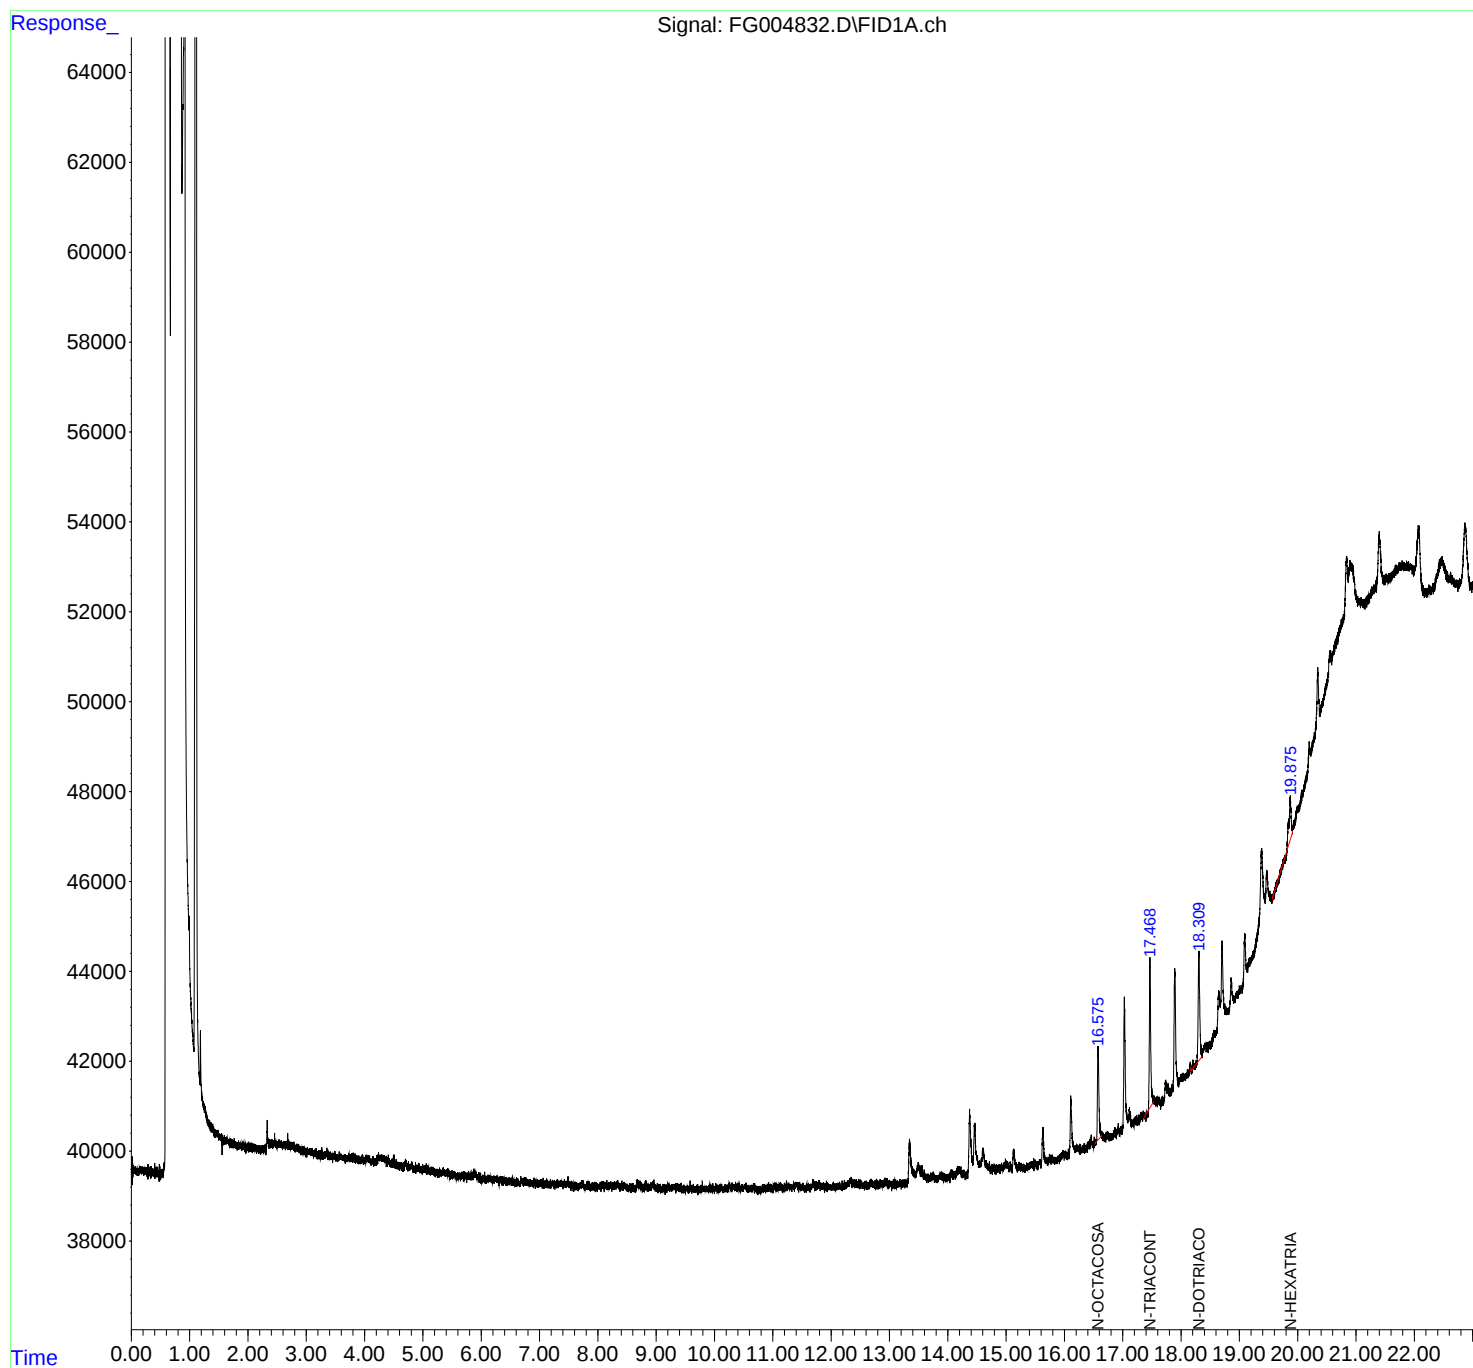


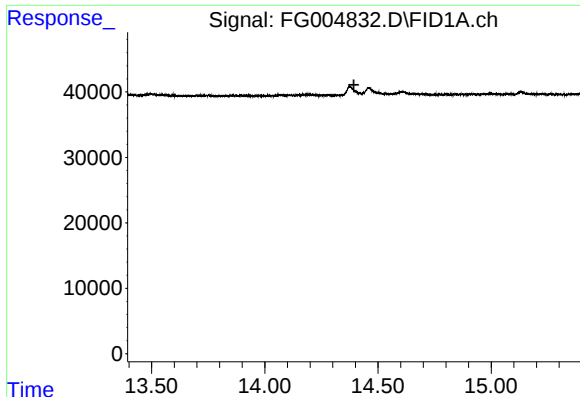

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.394 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

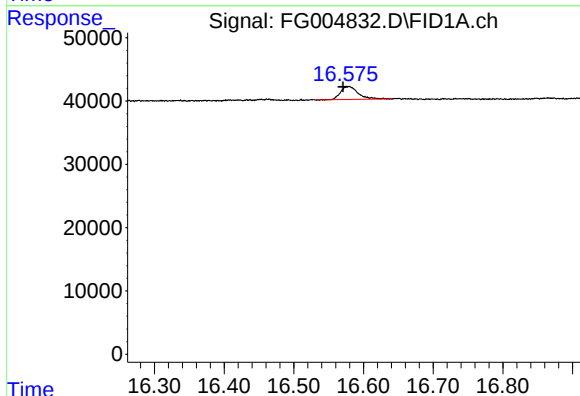


#12 N-OCTACOSANE

R.T.: 16.579 min
Delta R.T.: 0.008 min
Response: 35870
Conc: 0.26 ug/ml

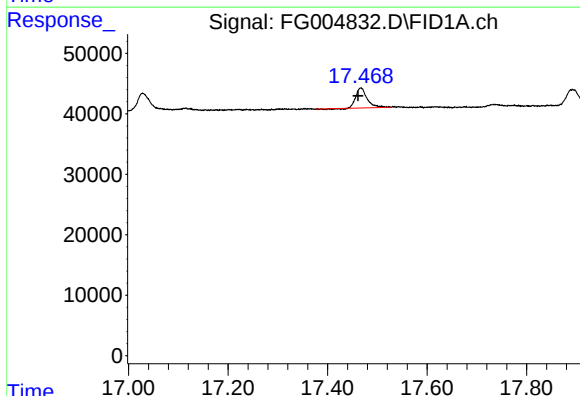


#13 N-TRIACONTANE

R.T.: 17.467 min
Delta R.T.: 0.006 min
Response: 51067
Conc: 0.38 ug/ml

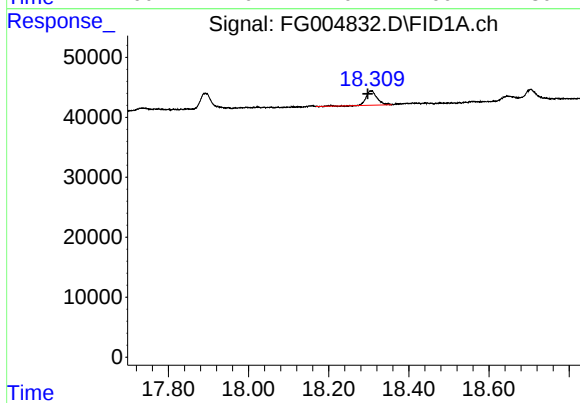

#14 N-DOTRIACONTANE

R.T.: 18.306 min
Delta R.T.: 0.009 min
Response: 46234
Conc: 0.37 ug/ml

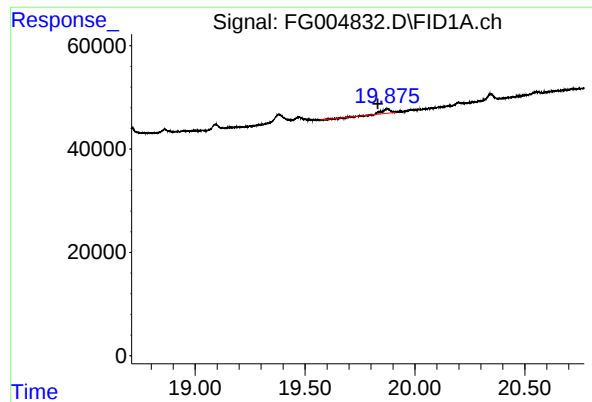

#16 N-HEXATRIACONTANE

R.T.: 19.876 min
Delta R.T.: 0.045 min
Response: 20390
Conc: 0.19 ug/ml

Instrument :
FID_G
ClientSampleId :