

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042622\
Data File : FG009671.D
Signal(s) : FID1A.ch
Acq On : 26 Apr 2022 11:46
Operator : AJ\MA
Sample : N2549-08 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RW-M-20220422

Integration File: Sample.e
Quant Time: Apr 27 01:12:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.620	450925	3.500 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042622\
Data File : FG009671.D
Signal(s) : FID1A.ch
Acq On : 26 Apr 2022 11:46
Operator : AJ\MA
Sample : N2549-08 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RW-M-20220422

Integration File: Sample.e
Quant Time: Apr 27 01:12:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

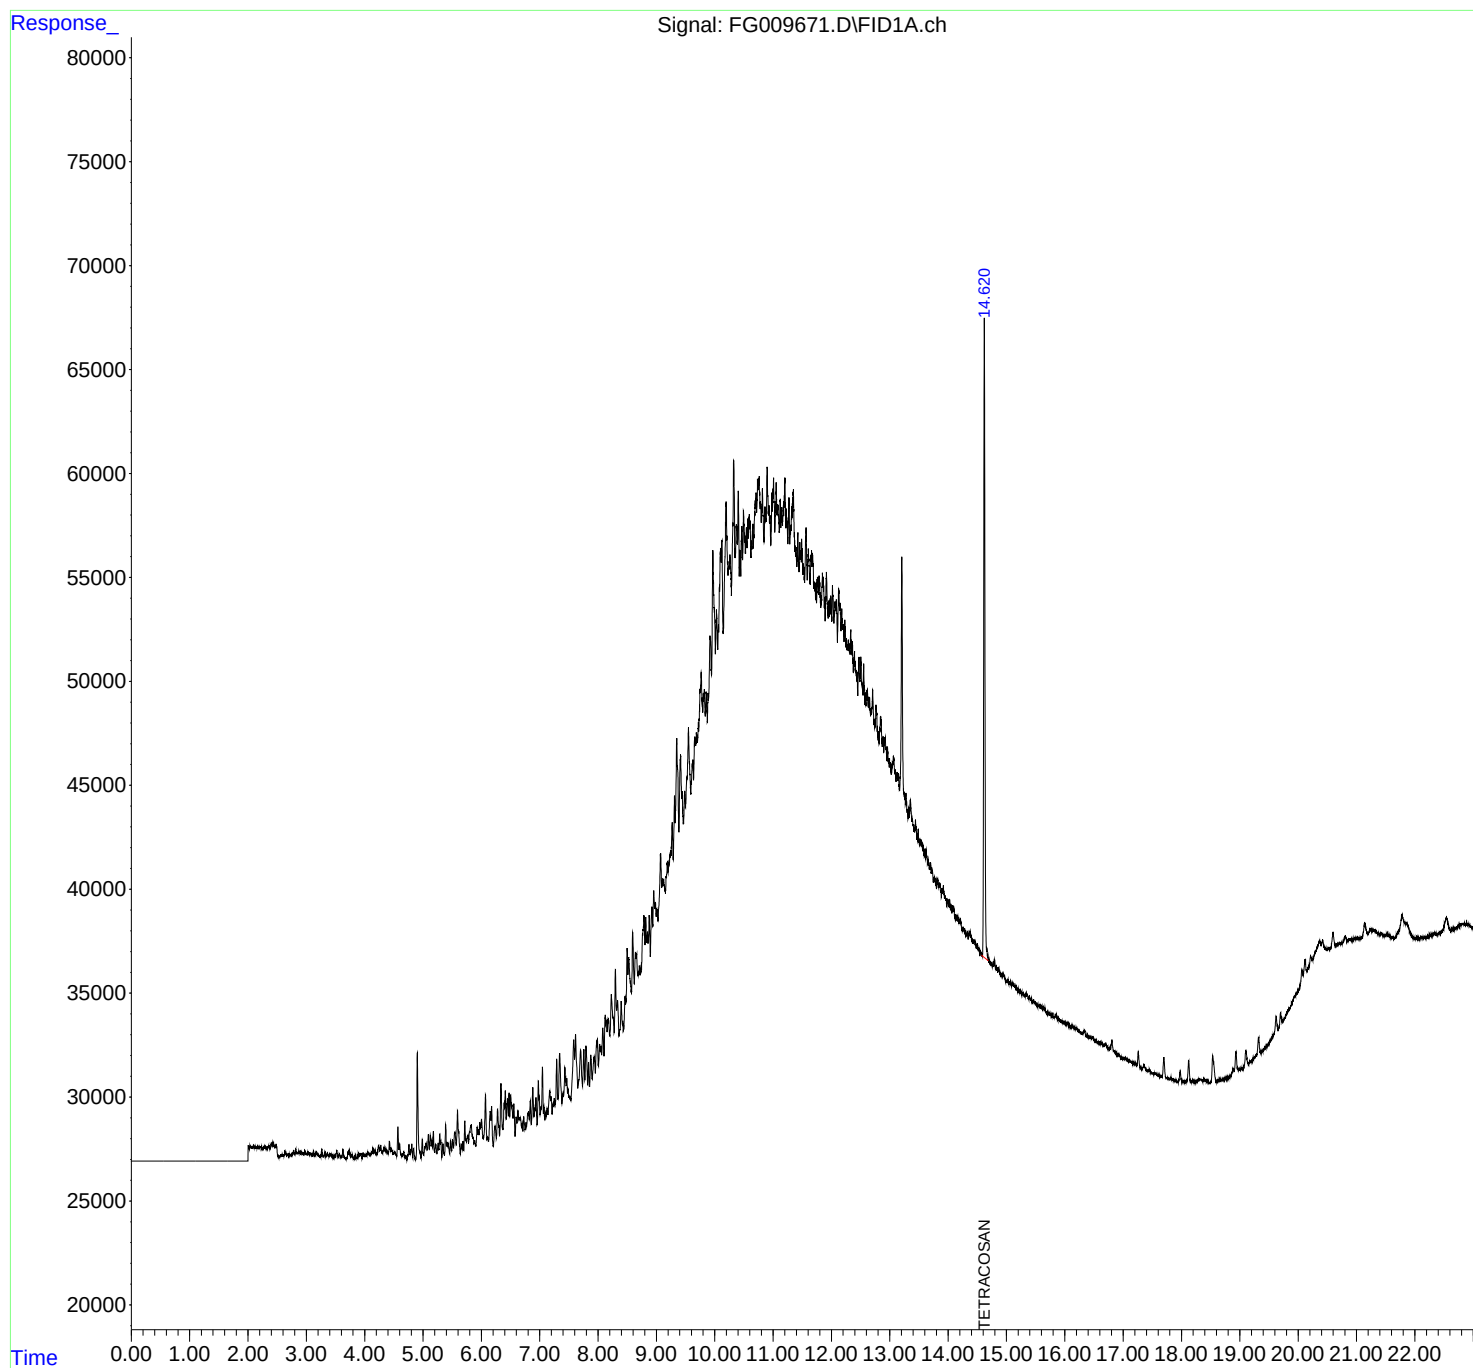

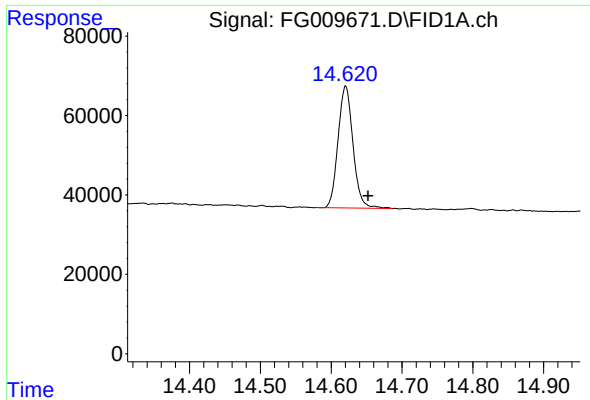

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.620 min
Delta R.T.: -0.032 min
Response: 450925
Conc: 3.50 ug/ml

Instrument :
FID_G
ClientSampleId :
RW-M-20220422