

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042624\
 Data File : FG013707.D
 Signal(s) : FID1A.ch
 Acq On : 26 Apr 2024 12:34
 Operator : YP\AJ
 Sample : P2252-14 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 27 05:54:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041124.M
 Quant Title :
 QLast Update : Thu Apr 11 13:37:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.069	164266	1.413 ug/ml
Target Compounds			
2) N-DECANE	4.582	737597	5.888 ug/ml
3) N-DODECANE	6.754	1050378	8.267 ug/ml
4) N-TETRADECANE	8.588	1356924	10.566 ug/ml
5) N-HEXADECANE	10.201	1260505	9.738 ug/ml
6) N-OCTADECANE	11.649	930177	7.022 ug/ml
7) N-EICOSANE	12.965	474658	3.523 ug/ml
8) N-DOCOSANE	14.167	208292	1.589 ug/ml
10) N-TETRACOSANE	15.274	67399	0.513 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042624\
Data File : FG013707.D
Signal(s) : FID1A.ch
Acq On : 26 Apr 2024 12:34
Operator : YP\AJ
Sample : P2252-14 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 05:54:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041124.M
Quant Title :
QLast Update : Thu Apr 11 13:37:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

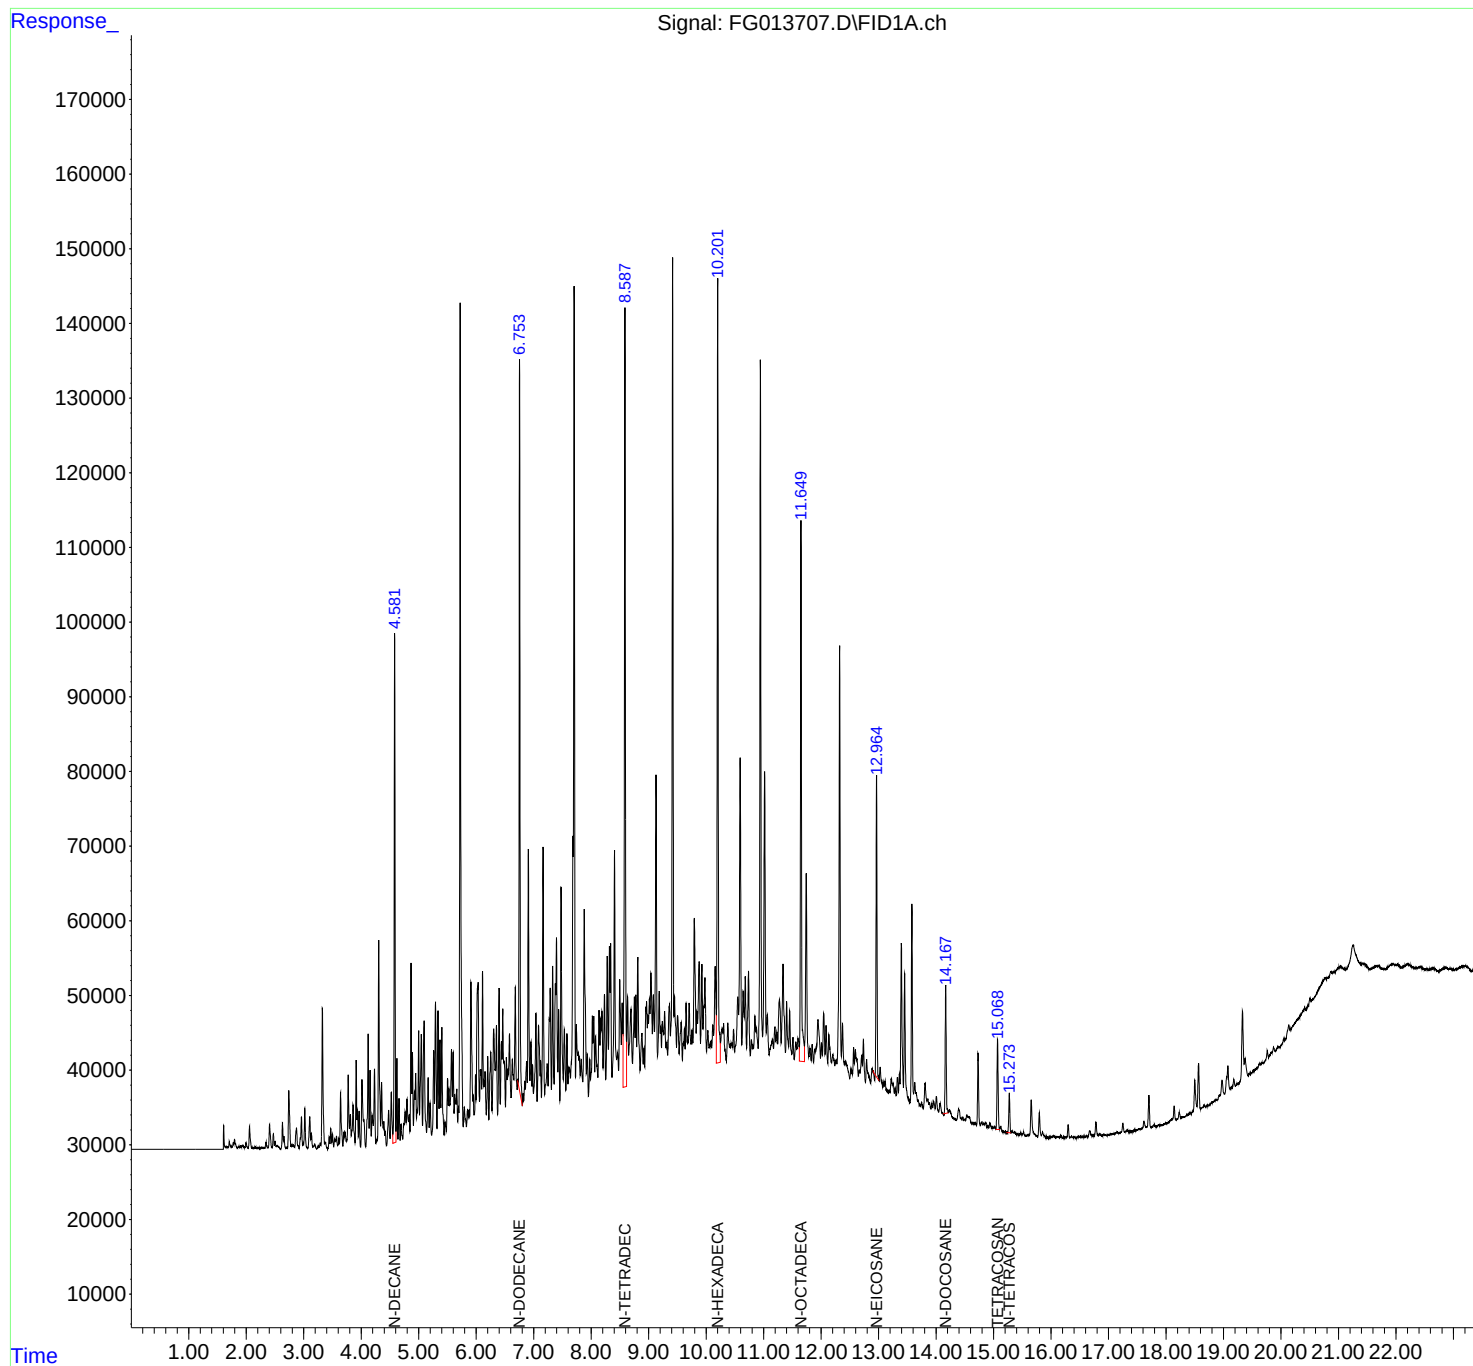


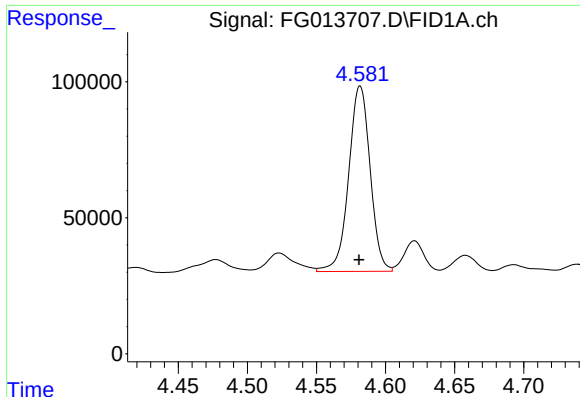

#2 N-DECANE


R.T.: 4.582 min
Delta R.T.: 0.000 min
Response: 737597
Conc: 5.89 ug/ml

Instrument :
FID_G
ClientSampleId :

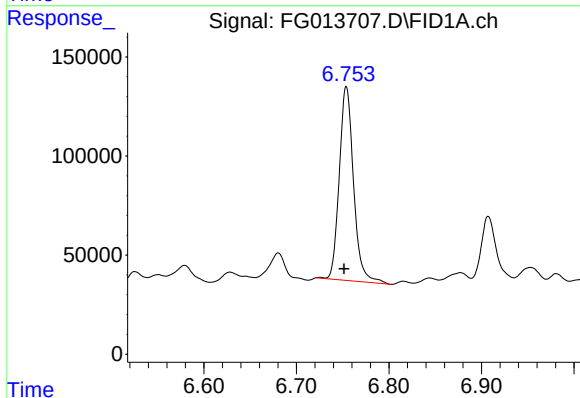


#3 N-DODECANE

R.T.: 6.754 min
Delta R.T.: 0.002 min
Response: 1050378
Conc: 8.27 ug/ml

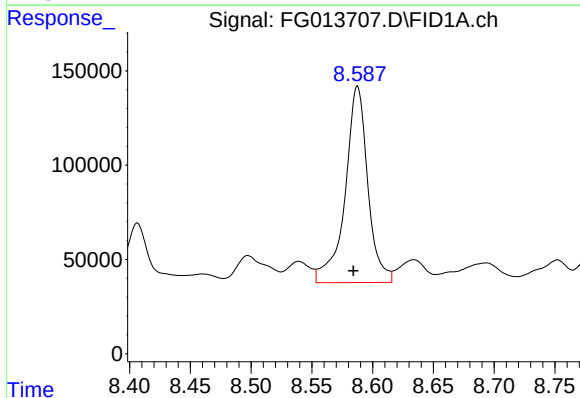


#4 N-TETRADECANE

R.T.: 8.588 min
Delta R.T.: 0.004 min
Response: 1356924
Conc: 10.57 ug/ml

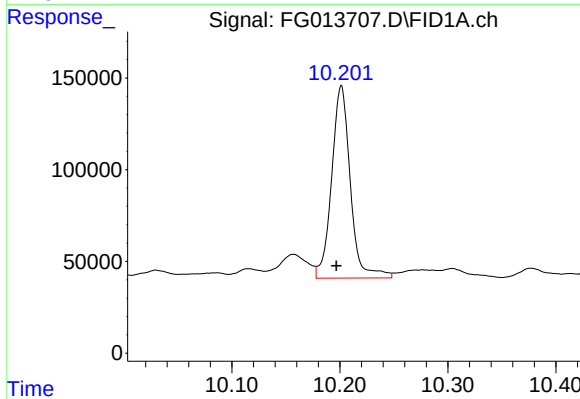

#5 N-HEXADECANE


R.T.: 10.201 min
Delta R.T.: 0.005 min
Response: 1260505
Conc: 9.74 ug/ml

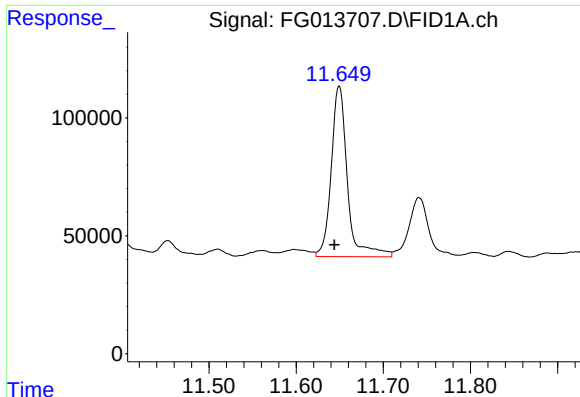

#6 N-OCTADECANE


R.T.: 11.649 min
Delta R.T.: 0.005 min
Response: 930177
Conc: 7.02 ug/ml

Instrument :
FID_G
ClientSampleId :

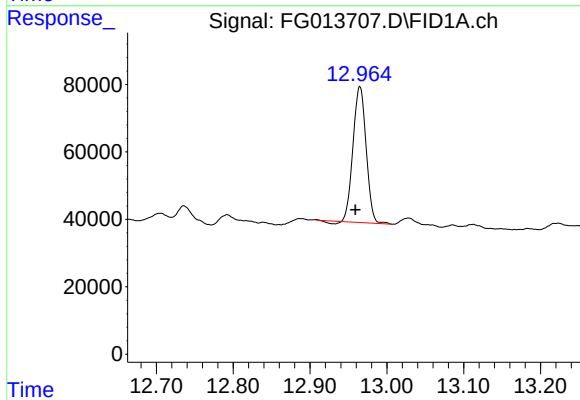


#7 N-EICOSANE

R.T.: 12.965 min
Delta R.T.: 0.006 min
Response: 474658
Conc: 3.52 ug/ml

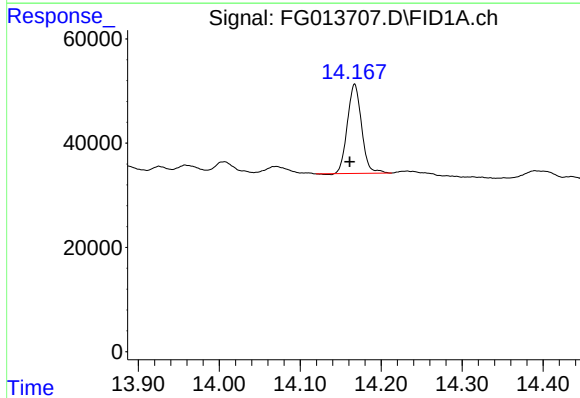


#8 N-DOCOSANE

R.T.: 14.167 min
Delta R.T.: 0.006 min
Response: 208292
Conc: 1.59 ug/ml

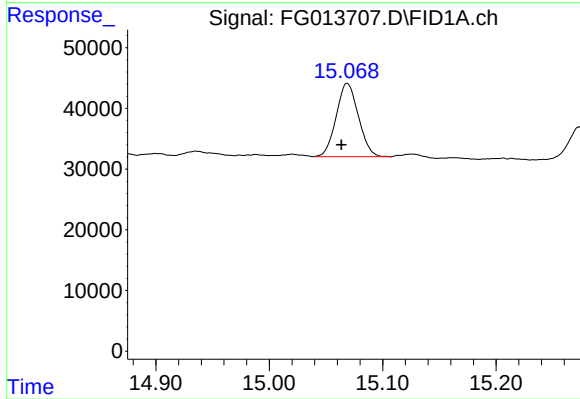

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.069 min
Delta R.T.: 0.005 min
Response: 164266
Conc: 1.41 ug/ml

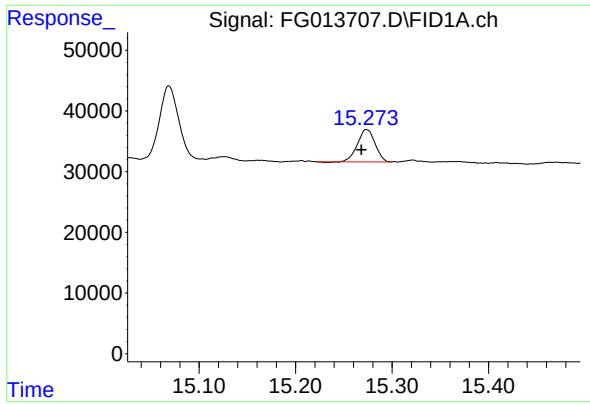

#10 N-TETRACOSANE

R.T.: 15.274 min
Delta R.T.: 0.005 min
Response: 67399
Conc: 0.51 ug/ml

Instrument :

FID_G

ClientSampleId :