

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042624\
 Data File : FG013705.D
 Signal(s) : FID1A.ch
 Acq On : 26 Apr 2024 10:44
 Operator : YP\AJ
 Sample : PB160527BS
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 PB160527BS

Integration File: autoint1.e
 Quant Time: Apr 27 05:54:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041124.M
 Quant Title :
 QLast Update : Thu Apr 11 13:37:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.070	1953899	16.801 ug/ml
Target Compounds			
2) N-DECANE	4.582	2082607	16.626 ug/ml
3) N-DODECANE	6.754	2168704	17.070 ug/ml
4) N-TETRADECANE	8.588	2222613	17.307 ug/ml
5) N-HEXADECANE	10.201	2254949	17.420 ug/ml
6) N-OCTADECANE	11.649	2296522	17.336 ug/ml
7) N-EICOSANE	12.964	2314646	17.180 ug/ml
8) N-DOCOSANE	14.168	2227740	16.994 ug/ml
10) N-TETRACOSANE	15.275	2203137	16.783 ug/ml
11) N-HEXACOSANE	16.299	2166093	16.577 ug/ml
12) N-OCTACOSANE	17.253	2106474	16.341 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042624\
Data File : FG013705.D
Signal(s) : FID1A.ch
Acq On : 26 Apr 2024 10:44
Operator : YP\AJ
Sample : PB160527BS
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB160527BS

Integration File: autoint1.e
Quant Time: Apr 27 05:54:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041124.M
Quant Title :
QLast Update : Thu Apr 11 13:37:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

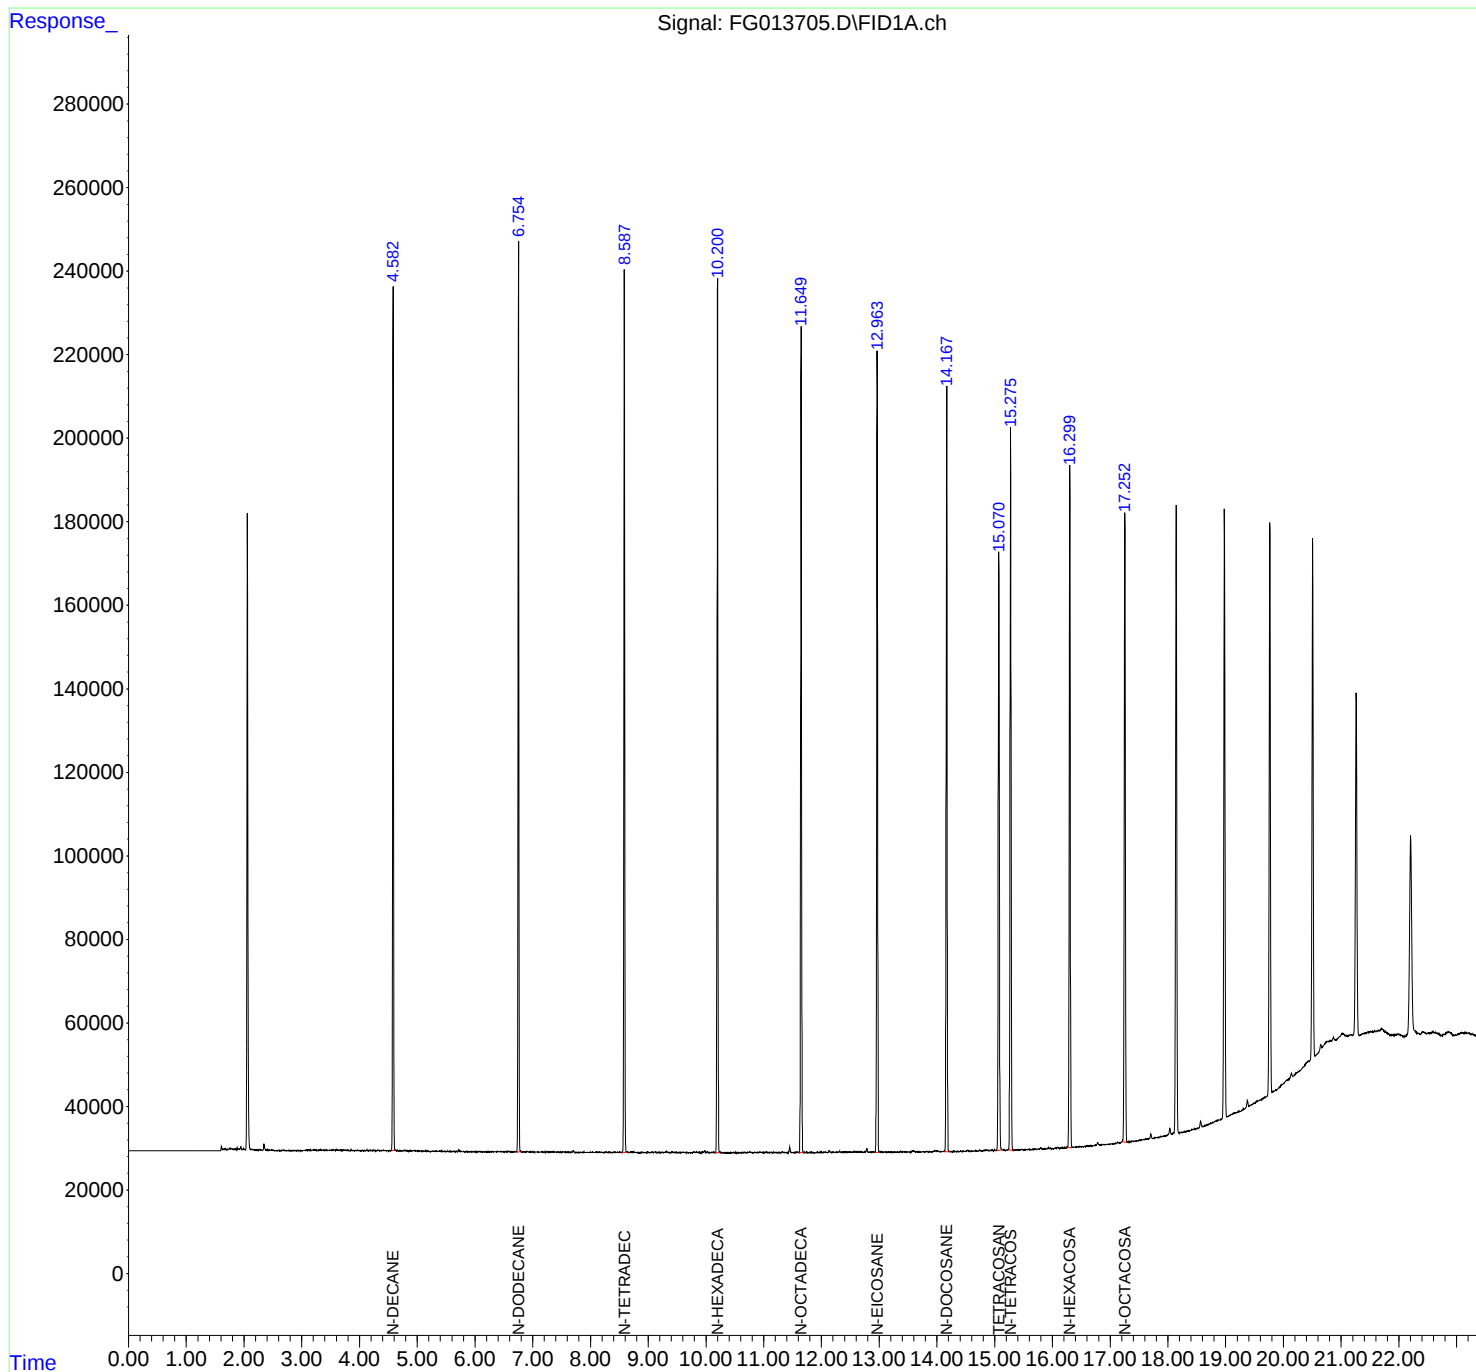


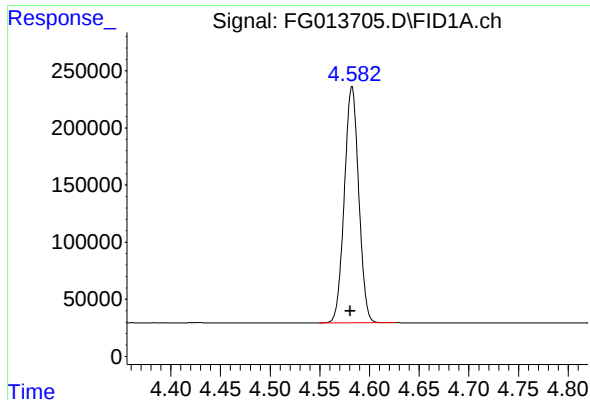

#2 N-DECANE


R.T.: 4.582 min
Delta R.T.: 0.002 min
Response: 2082607
Conc: 16.63 ug/ml

Instrument :
FID_G
ClientSampleId :
PB160527BS

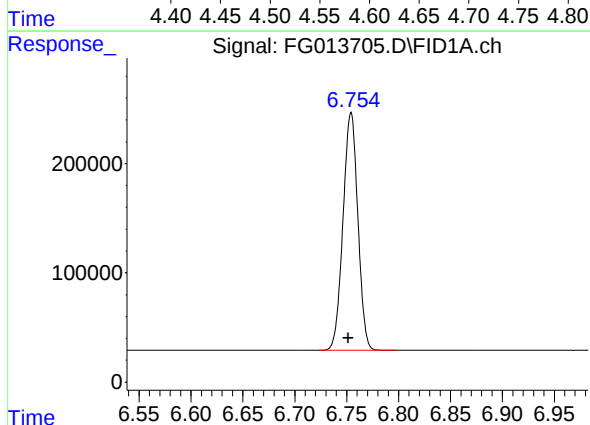


#3 N-DODECANE

R.T.: 6.754 min
Delta R.T.: 0.003 min
Response: 2168704
Conc: 17.07 ug/ml

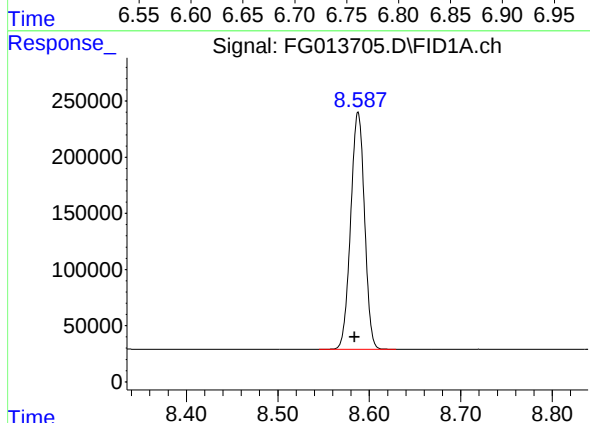


#4 N-TETRADECANE

R.T.: 8.588 min
Delta R.T.: 0.004 min
Response: 2222613
Conc: 17.31 ug/ml

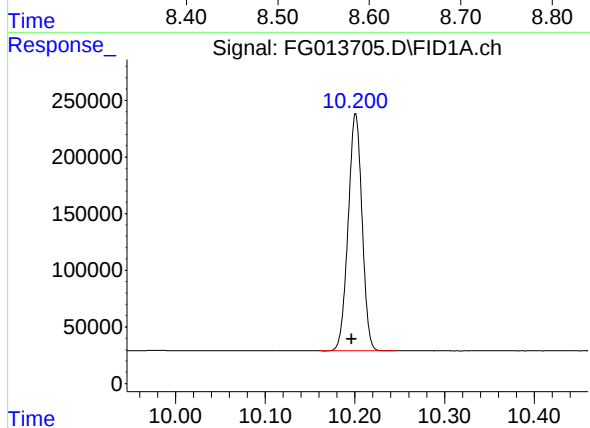

#5 N-HEXADECANE


R.T.: 10.201 min
Delta R.T.: 0.004 min
Response: 2254949
Conc: 17.42 ug/ml

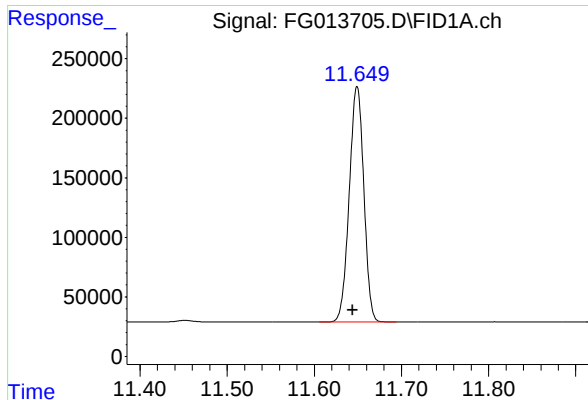

#6 N-OCTADECANE


R.T.: 11.649 min
Delta R.T.: 0.005 min
Response: 2296522
Conc: 17.34 ug/ml

Instrument :
FID_G
ClientSampleId :
PB160527BS

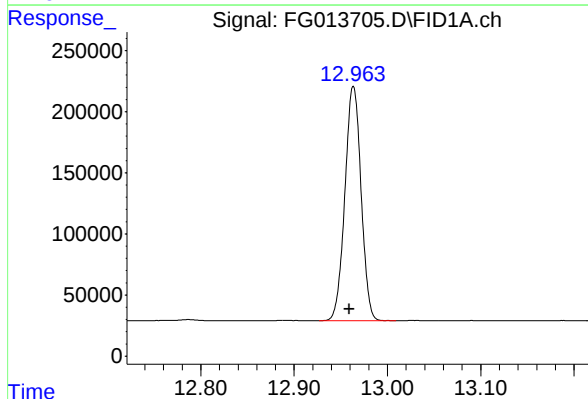


#7 N-EICOSANE

R.T.: 12.964 min
Delta R.T.: 0.004 min
Response: 2314646
Conc: 17.18 ug/ml

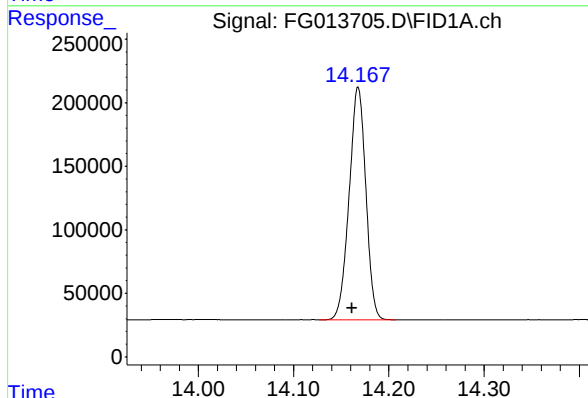


#8 N-DOCOSANE

R.T.: 14.168 min
Delta R.T.: 0.006 min
Response: 2227740
Conc: 16.99 ug/ml

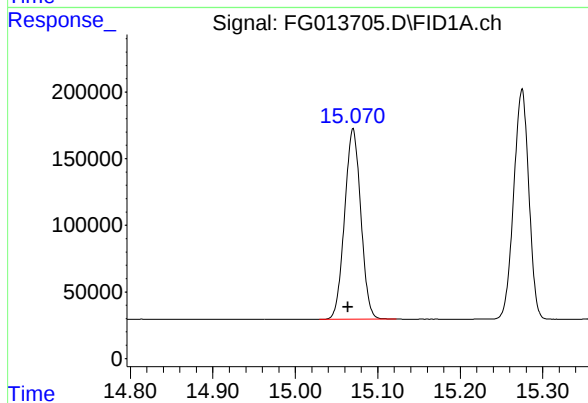

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.070 min
Delta R.T.: 0.006 min
Response: 1953899
Conc: 16.80 ug/ml

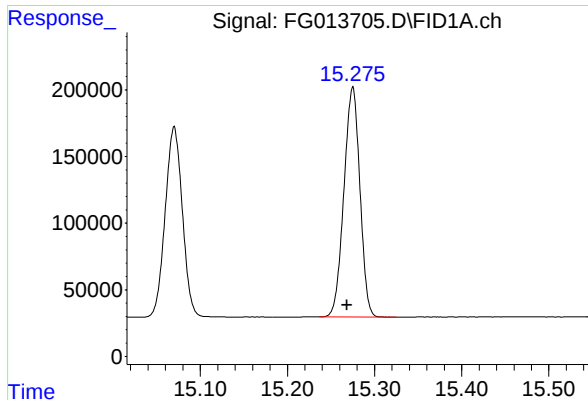

#10 N-TETRACOSANE


R.T.: 15.275 min
Delta R.T.: 0.007 min
Response: 2203137
Conc: 16.78 ug/ml

Instrument :
FID_G
ClientSampleId :
PB160527BS

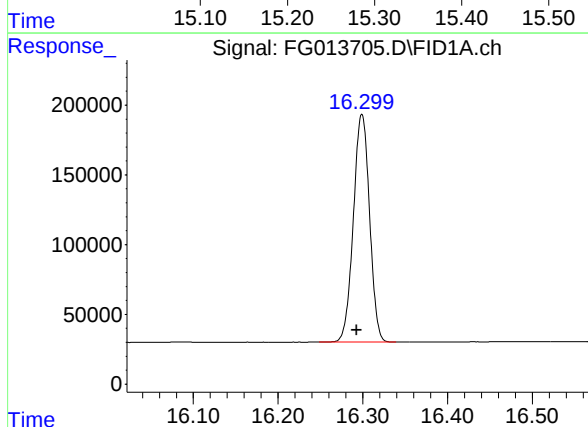

#11 N-HEXACOSANE

R.T.: 16.299 min
Delta R.T.: 0.007 min
Response: 2166093
Conc: 16.58 ug/ml

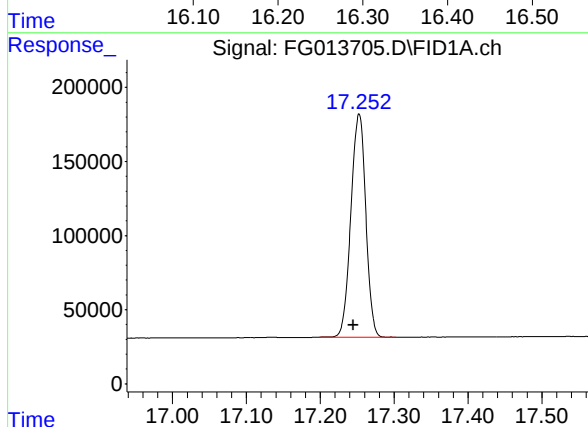

#12 N-OCTACOSANE

R.T.: 17.253 min
Delta R.T.: 0.008 min
Response: 2106474
Conc: 16.34 ug/ml