

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042722\
Data File : FG009674.D
Signal(s) : FID1A.ch
Acq On : 27 Apr 2022 10:33
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 28 03:05:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.796f	121499	0.848 ug/ml
14)	N-DOTRIACONTANE	18.560	162555	1.400 ug/ml
16)	N-HEXATRIACONTANE	20.120	175787	1.856 ug/ml
18)	N-TETRACONTANE	21.784f	116184	1.346 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042722\
Data File : FG009674.D
Signal(s) : FID1A.ch
Acq On : 27 Apr 2022 10:33
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 28 03:05:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

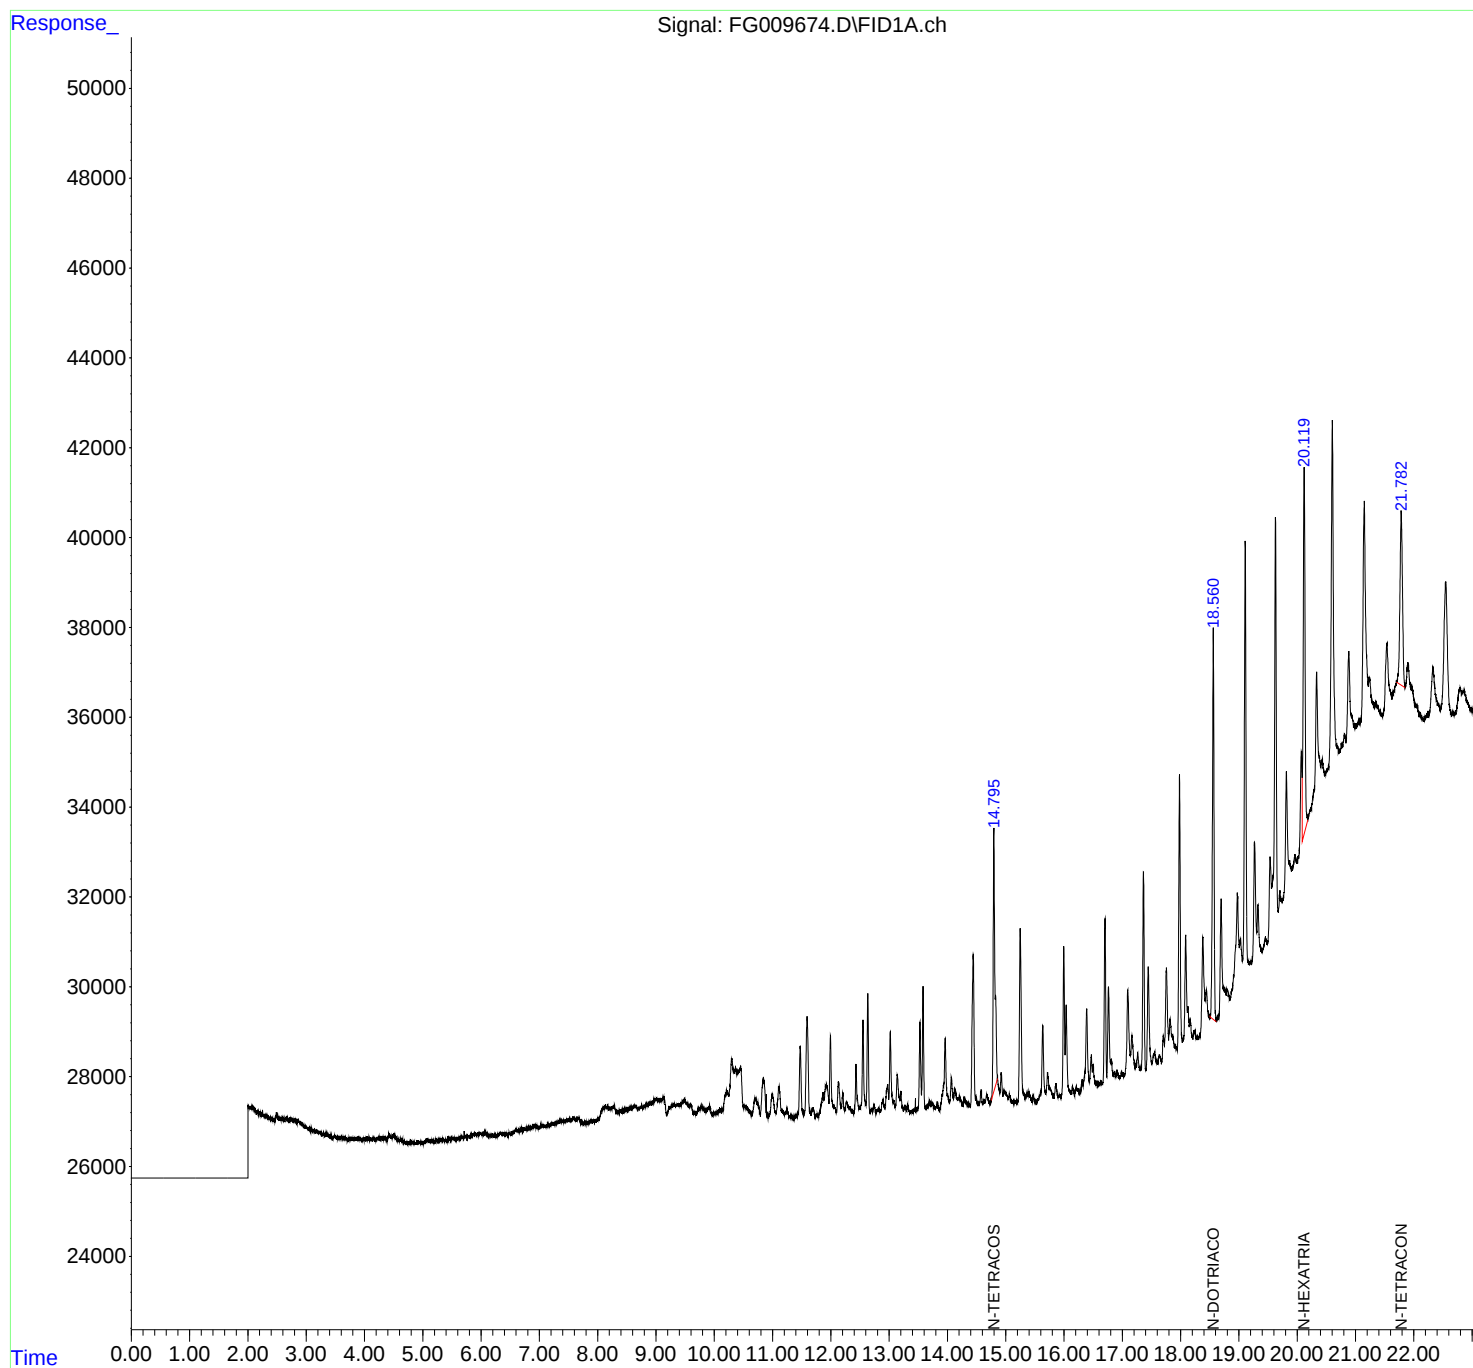


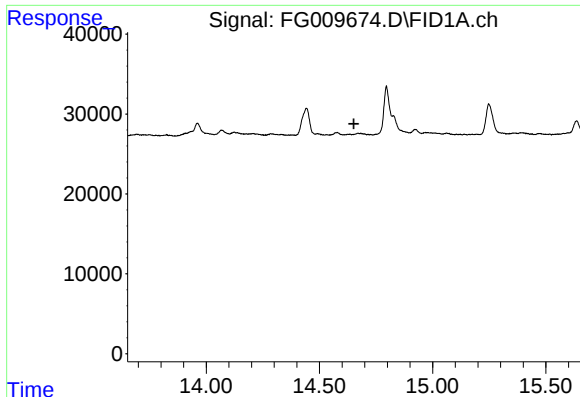

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.652 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

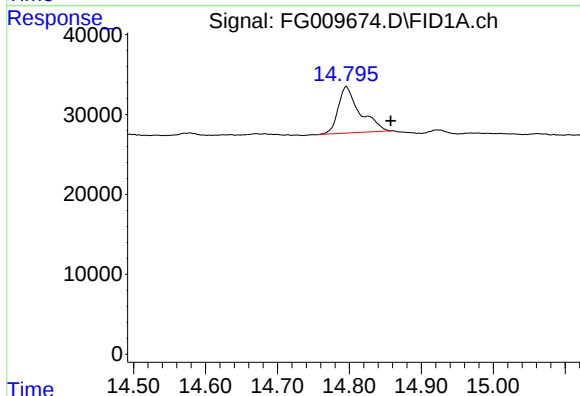


#10 N-TETRACOSANE

R.T.: 14.796 min
Delta R.T.: -0.062 min
Response: 121499
Conc: 0.85 ug/ml

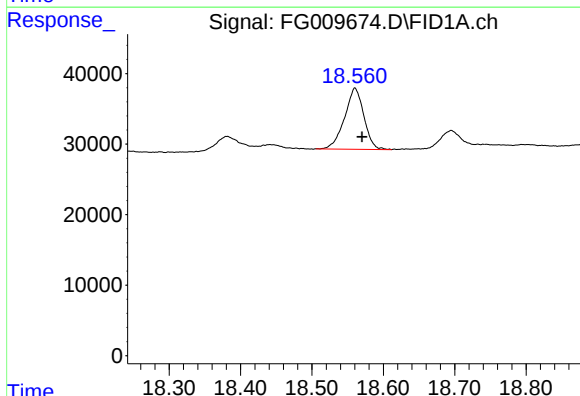


#14 N-DOTRIACONTANE

R.T.: 18.560 min
Delta R.T.: -0.010 min
Response: 162555
Conc: 1.40 ug/ml

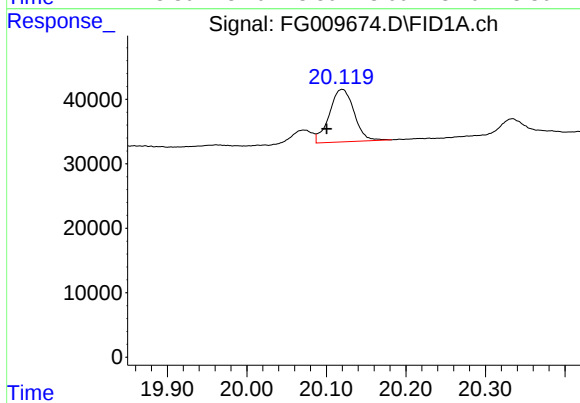

#16 N-HEXATRIACONTANE

R.T.: 20.120 min
Delta R.T.: 0.020 min
Response: 175787
Conc: 1.86 ug/ml

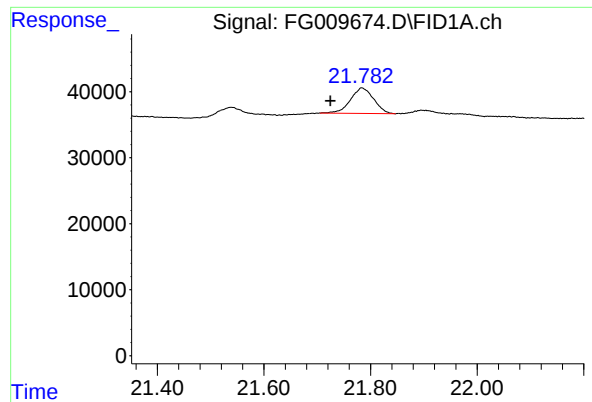

#18 N-TETRACONTANE

R.T.: 21.784 min
Delta R.T.: 0.059 min
Response: 116184
Conc: 1.35 ug/ml

Instrument :

FID_G

ClientSampleId :