

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042722\
Data File : FG009677.D
Signal(s) : FID1A.ch
Acq On : 27 Apr 2022 12:36
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Apr 28 03:06:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.345	2449648	16.254 ug/ml
12)	N-OCTACOSANE	16.807	2736360	20.967 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042722\
Data File : FG009677.D
Signal(s) : FID1A.ch
Acq On : 27 Apr 2022 12:36
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Apr 28 03:06:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

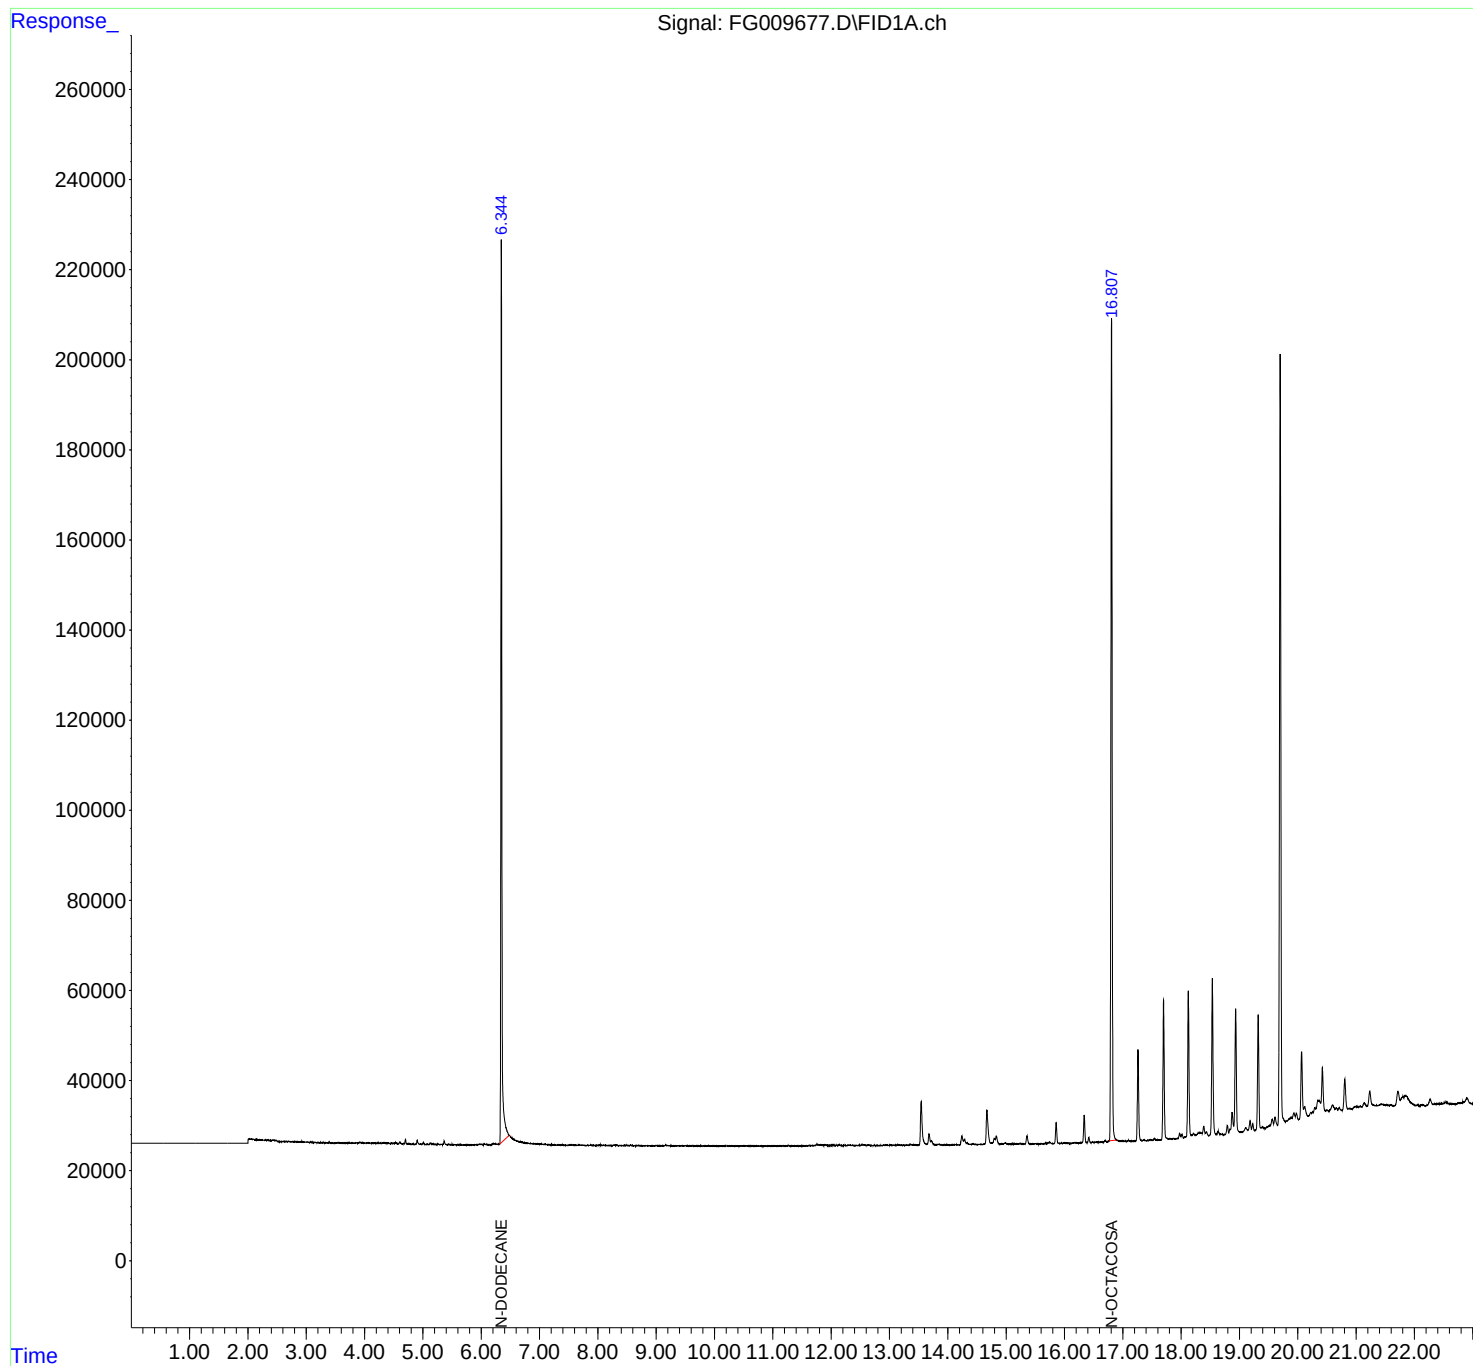


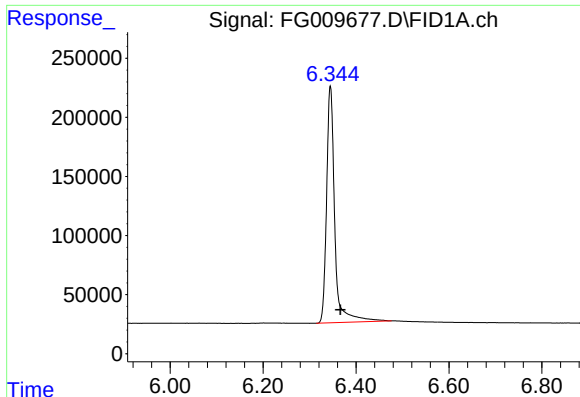

#3 N-DODECANE


R.T.: 6.345 min
Delta R.T.: -0.022 min
Response: 2449648
Conc: 16.25 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

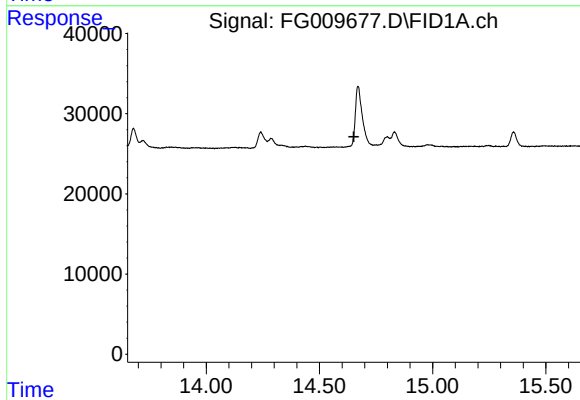

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.652 min
Response: 0
Conc: N.D.

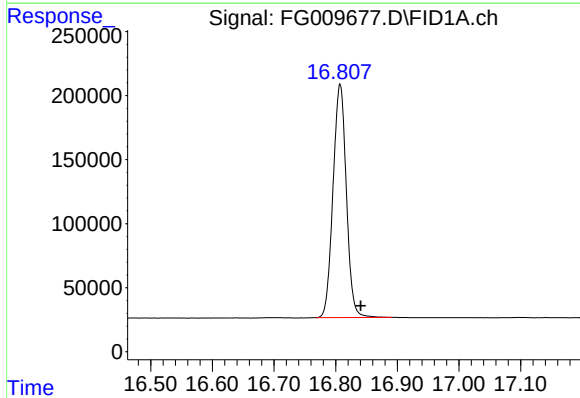

#12 N-OCTACOSANE

R.T.: 16.807 min
Delta R.T.: -0.033 min
Response: 2736360
Conc: 20.97 ug/ml