

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042821\
Data File : FG007947.D
Signal(s) : FID1A.ch
Acq On : 29 Apr 2021 00:45
Operator : DD\AJ
Sample :
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 29 01:24:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) N-HEXATRIACONTANE	20.263	118583	1.013 ug/ml
18) N-TETRACONTANE	22.002f	239766	2.189 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042821\
Data File : FG007947.D
Signal(s) : FID1A.ch
Acq On : 29 Apr 2021 00:45
Operator : DD\AJ
Sample :
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 29 01:24:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

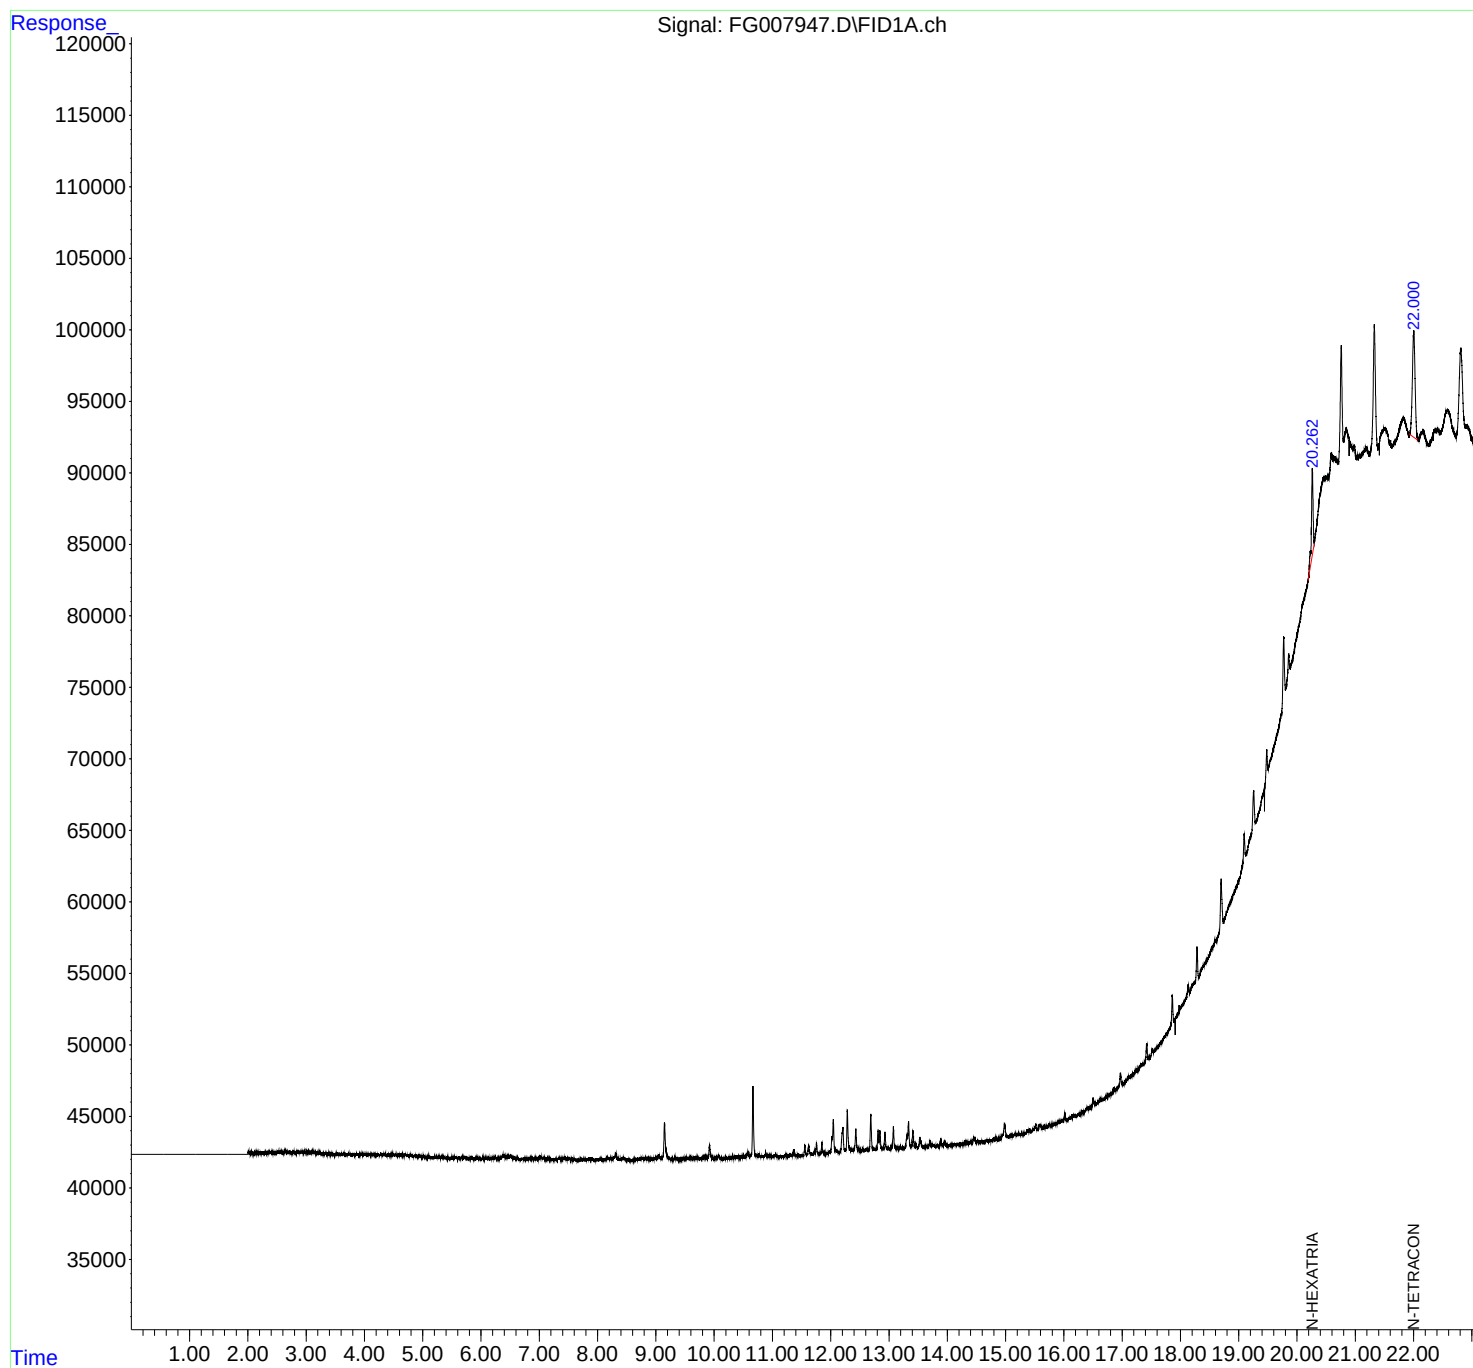


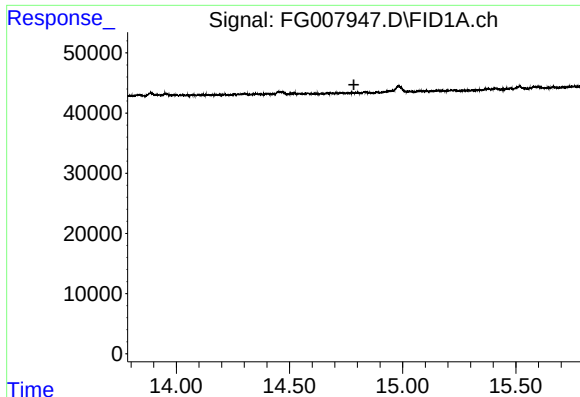

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.784 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

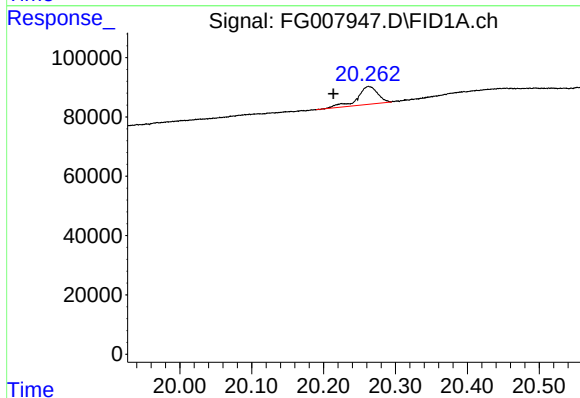

#16 N-HEXATRIACONTANE

R.T.: 20.263 min
Delta R.T.: 0.049 min
Response: 118583
Conc: 1.01 ug/ml

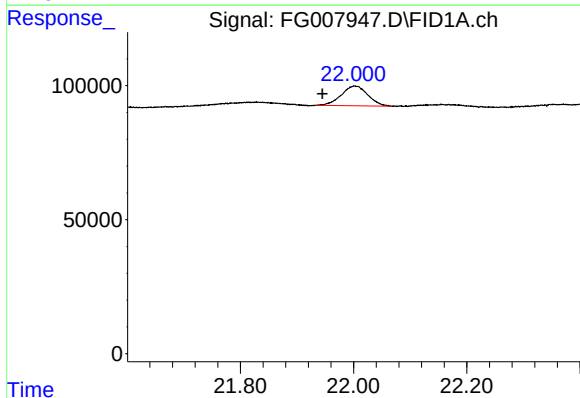

#18 N-TETRACONTANE

R.T.: 22.002 min
Delta R.T.: 0.057 min
Response: 239766
Conc: 2.19 ug/ml