

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042822\
Data File : FG009686.D
Signal(s) : FID1A.ch
Acq On : 28 Apr 2022 09:16
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 29 01:40:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) N-HEXATRIACONTANE	20.120	276092	2.916 ug/ml
18) N-TETRACONTANE	21.786f	172769	2.002 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042822\
Data File : FG009686.D
Signal(s) : FID1A.ch
Acq On : 28 Apr 2022 09:16
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 29 01:40:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 08 10:19:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

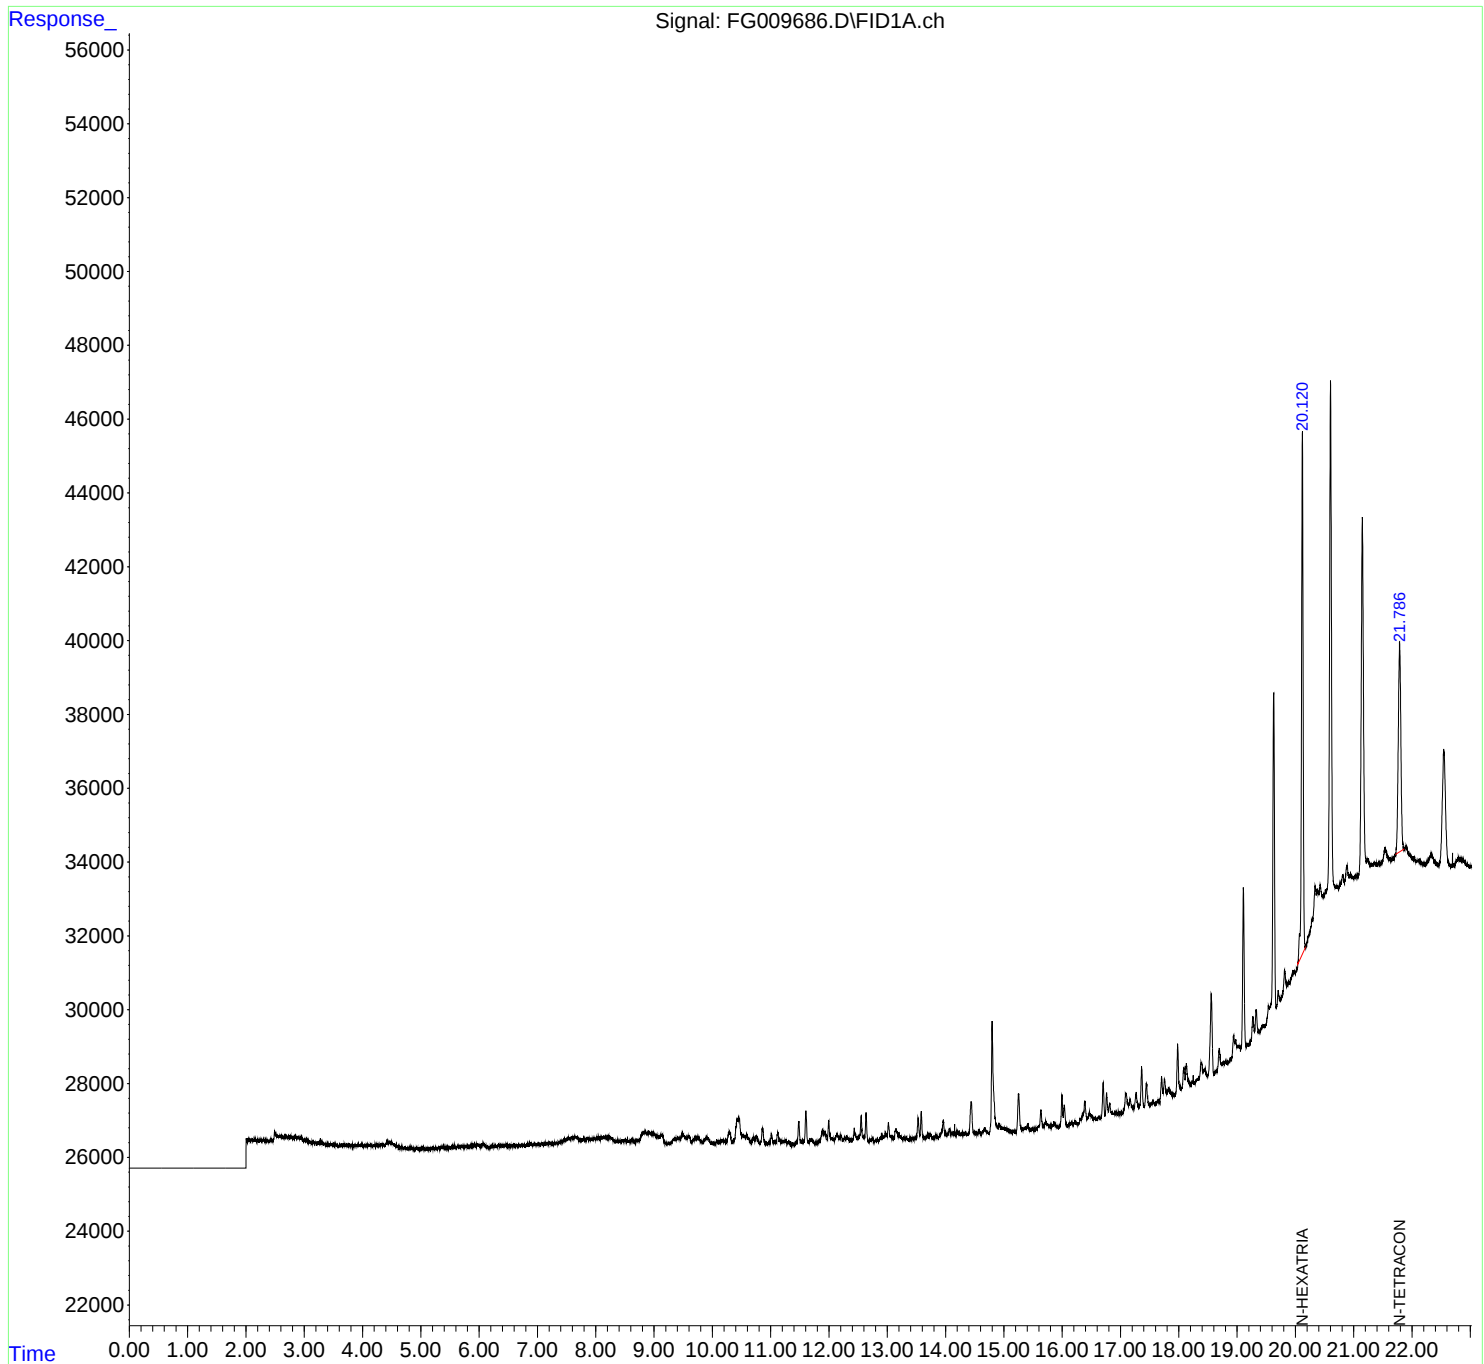


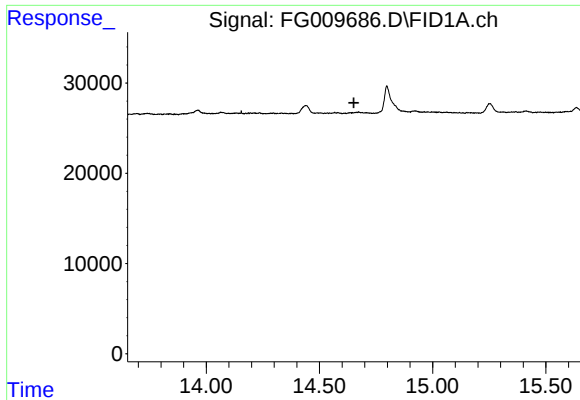

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.652 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

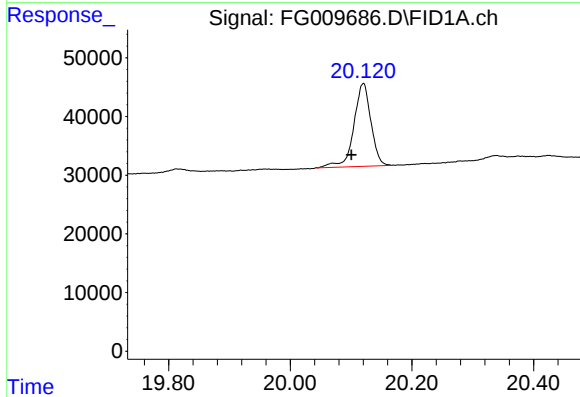

#16 N-HEXATRIACONTANE

R.T.: 20.120 min
Delta R.T.: 0.020 min
Response: 276092
Conc: 2.92 ug/ml

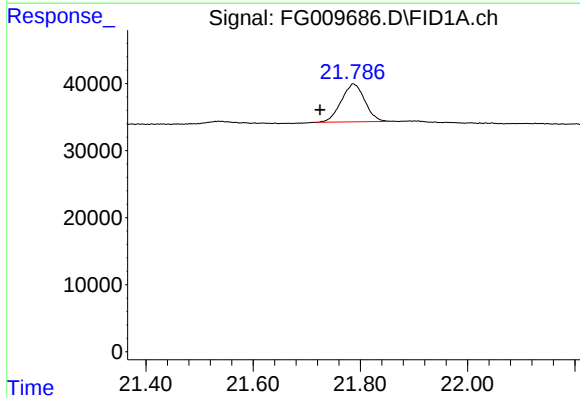

#18 N-TETRACONTANE

R.T.: 21.786 min
Delta R.T.: 0.061 min
Response: 172769
Conc: 2.00 ug/ml