

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042919\
Data File : FG004843.D
Signal(s) : FID1A.ch
Acq On : 29 Apr 2019 12:00
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 30 01:03:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042619.M
Quant Title :
QLast Update : Sat Apr 27 03:52:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.147	2366491	16.911 ug/ml
12)	N-OCTACOSANE	16.567	2773569	19.741 ug/ml
13)	N-TRIACONTANE	17.462	71119	0.525 ug/ml
14)	N-DOTRIACONTANE	18.298	76351	0.614 ug/ml
15)	N-TETRATRIACONTANE	19.083	49947	0.434 ug/ml
16)	N-HEXATRIACONTANE	19.837	16112	0.153 ug/ml
18)	N-TETRACONTANE	21.395	54724	0.527 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042919\
Data File : FG004843.D
Signal(s) : FID1A.ch
Acq On : 29 Apr 2019 12:00
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 30 01:03:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042619.M
Quant Title :
QLast Update : Sat Apr 27 03:52:23 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

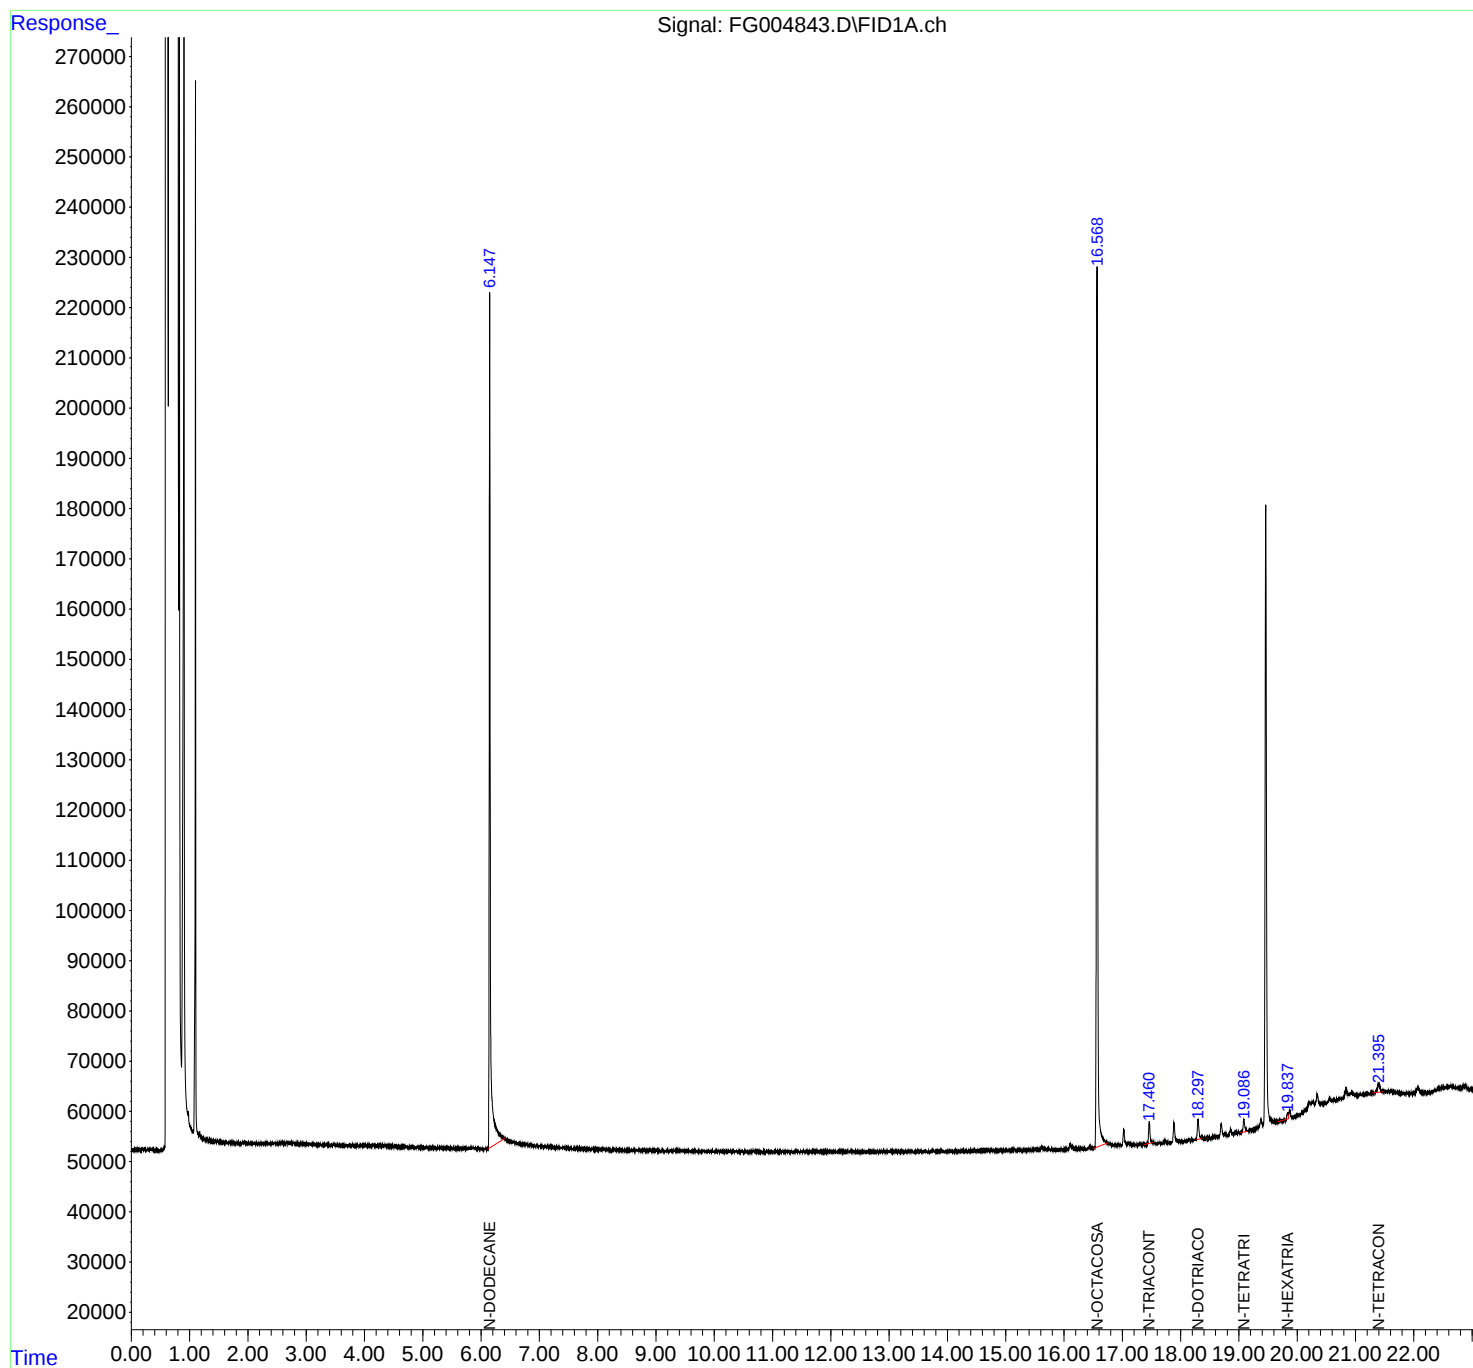

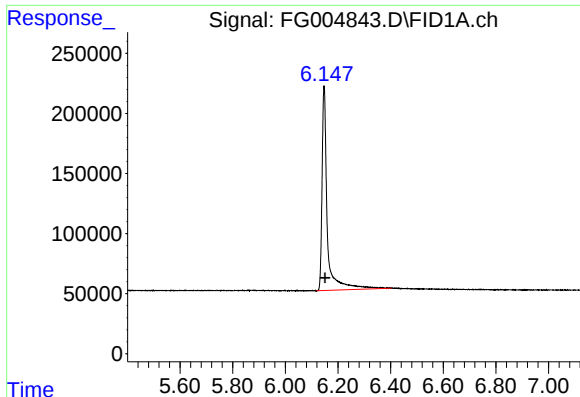


#3 N-DODECANE

R.T.: 6.147 min
Delta R.T.: -0.003 min
Response: 2366491
Conc: 16.91 ug/ml

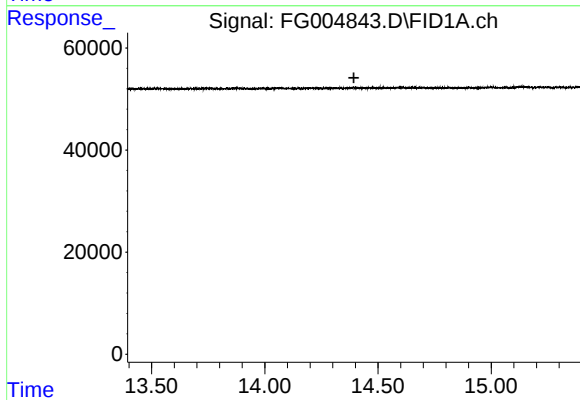


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.394 min
Response: 0
Conc: N.D.

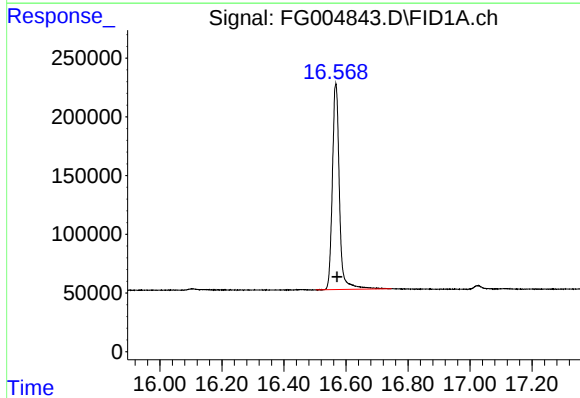


#12 N-OCTACOSANE

R.T.: 16.567 min
Delta R.T.: -0.004 min
Response: 2773569
Conc: 19.74 ug/ml

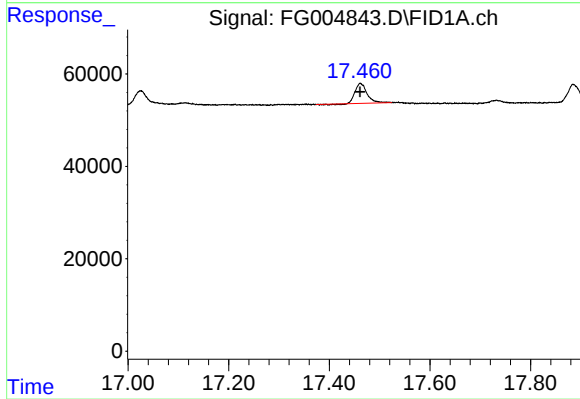


#13 N-TRIACONTANE

R.T.: 17.462 min
Delta R.T.: 0.000 min
Response: 71119
Conc: 0.52 ug/ml

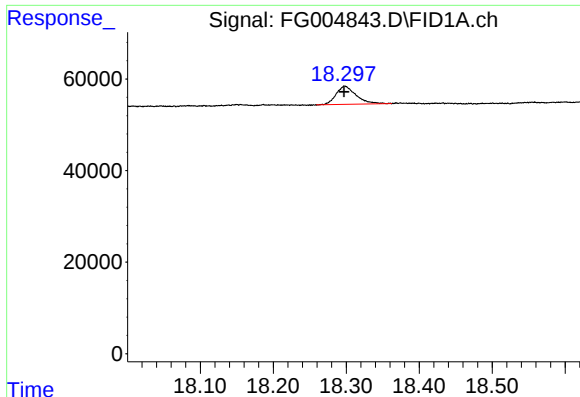


#14 N-DOTRIACONTANE

R.T.: 18.298 min
Delta R.T.: 0.000 min
Response: 76351
Conc: 0.61 ug/ml

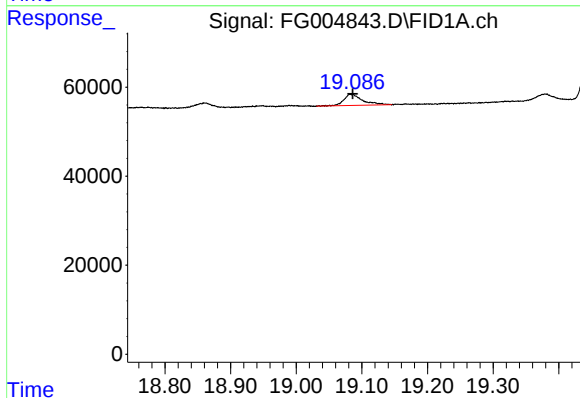


#15 N-TETRATRIACONTANE

R.T.: 19.083 min
Delta R.T.: -0.003 min
Response: 49947
Conc: 0.43 ug/ml

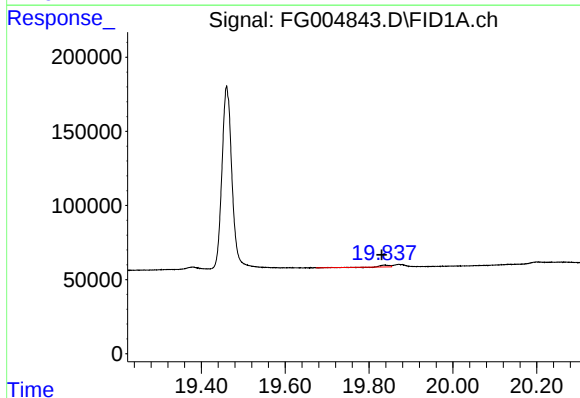

#16 N-HEXATRIACONTANE

R.T.: 19.837 min
Delta R.T.: 0.006 min
Response: 16112
Conc: 0.15 ug/ml

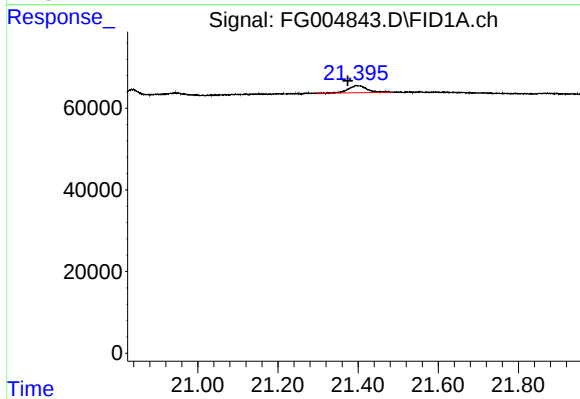

#18 N-TETRACONTANE

R.T.: 21.395 min
Delta R.T.: 0.021 min
Response: 54724
Conc: 0.53 ug/ml