

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042921\
 Data File : FG007953.D
 Signal(s) : FID1A.ch
 Acq On : 29 Apr 2021 13:50
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 30 02:00:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
 Quant Title :
 QLast Update : Thu Apr 22 01:54:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.794	6759344	50.773 ug/ml
Target Compounds			
2) N-DECANE	4.486	9027388	59.718 ug/ml
3) N-DODECANE	6.516	9021347	58.965 ug/ml
4) N-TETRADECANE	8.320	9022235	57.802 ug/ml
5) N-HEXADECANE	9.927	8766225	56.579 ug/ml
6) N-OCTADECANE	11.374	8676676	55.183 ug/ml
7) N-EICOSANE	12.690	8293938	53.523 ug/ml
8) N-DOCOSANE	13.893	7959488	51.797 ug/ml
10) N-TETRACOSANE	15.000	7620428	50.082 ug/ml
11) N-HEXACOSANE	16.023	7317188	49.125 ug/ml
12) N-OCTACOSANE	16.976	7187617	49.081 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042921\
Data File : FG007953.D
Signal(s) : FID1A.ch
Acq On : 29 Apr 2021 13:50
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 30 02:00:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

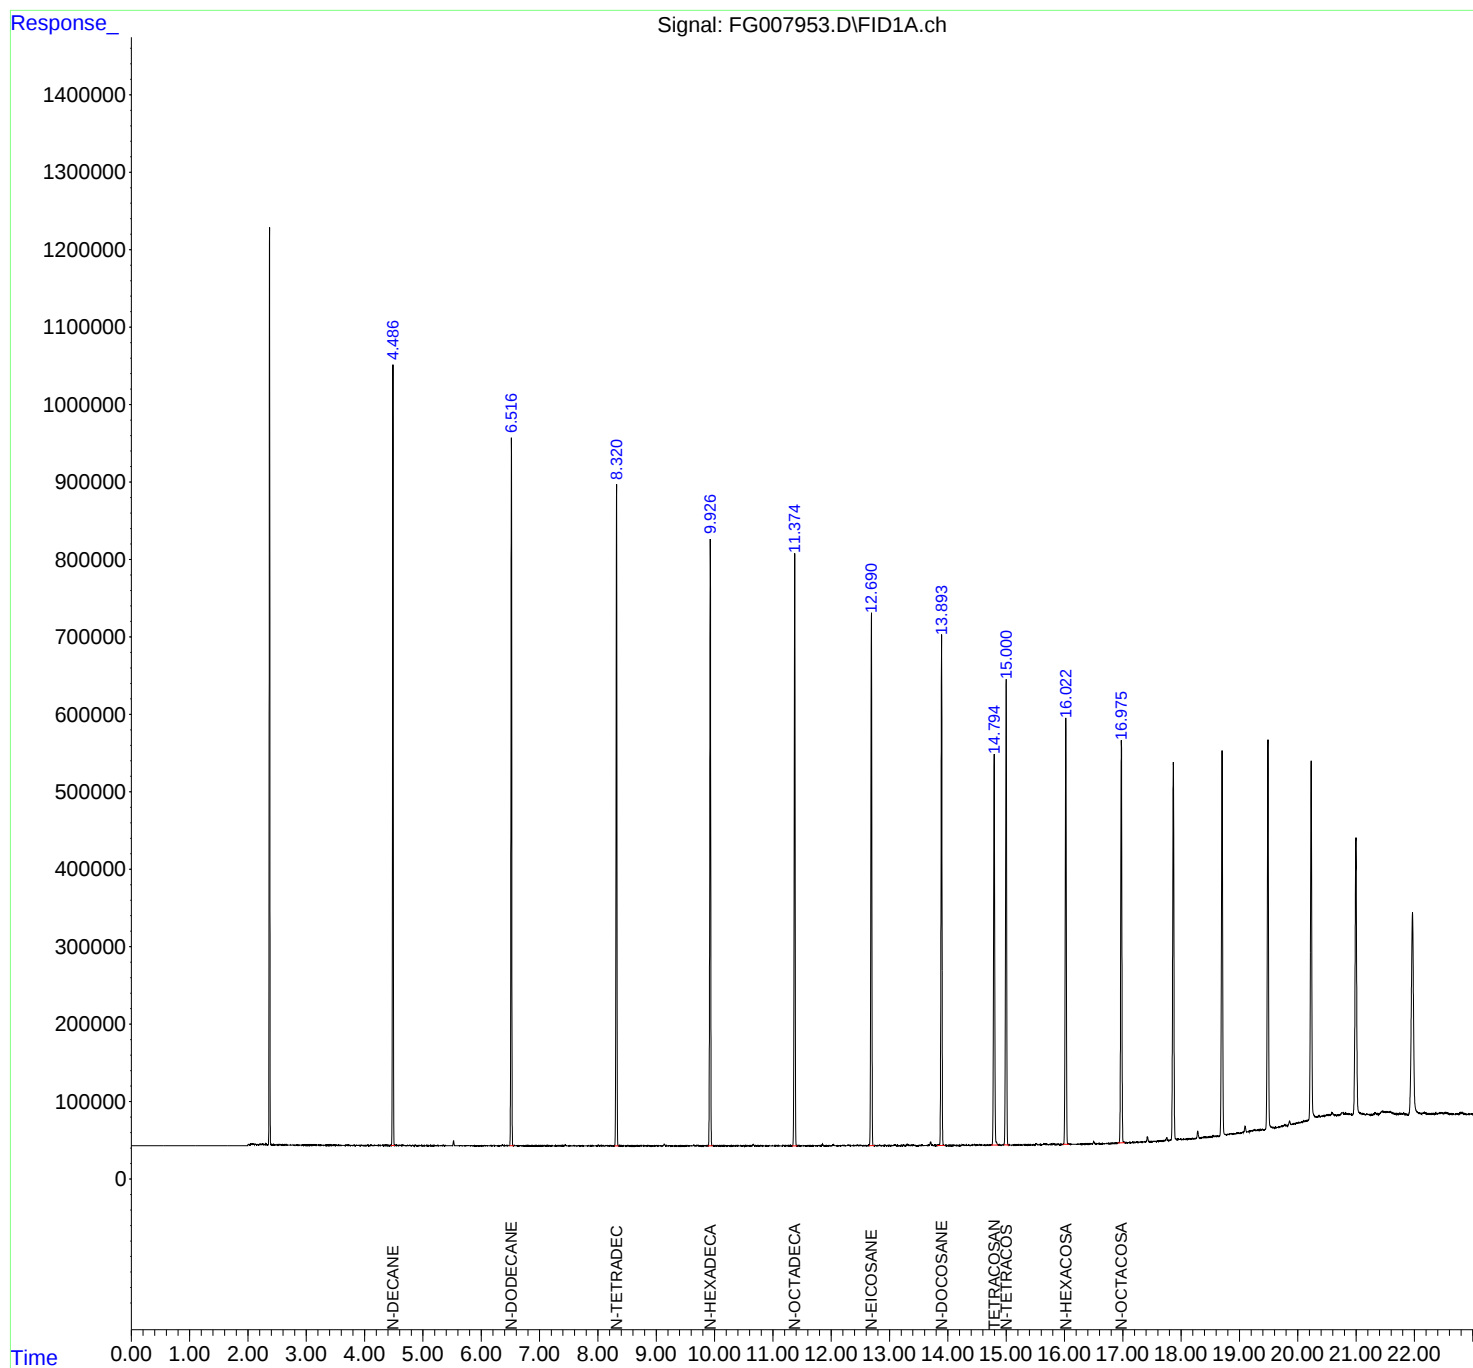

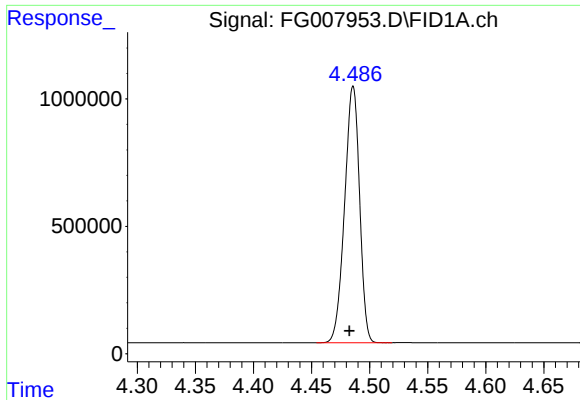


#2 N-DECANE

R.T.: 4.486 min
Delta R.T.: 0.003 min
Response: 9027388
Conc: 59.72 ug/ml

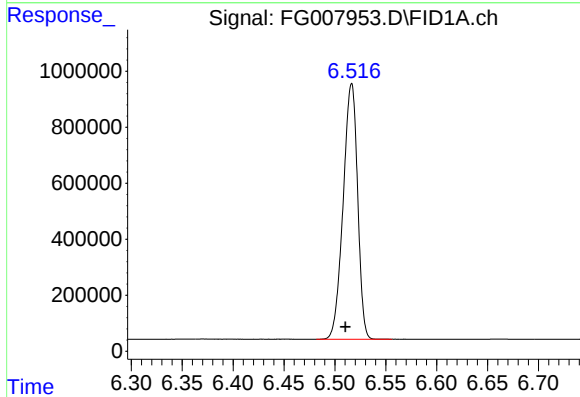


#3 N-DODECANE

R.T.: 6.516 min
Delta R.T.: 0.006 min
Response: 9021347
Conc: 58.97 ug/ml

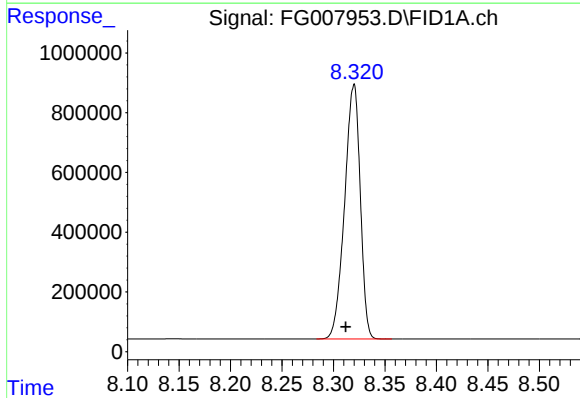


#4 N-TETRADECANE

R.T.: 8.320 min
Delta R.T.: 0.008 min
Response: 9022235
Conc: 57.80 ug/ml

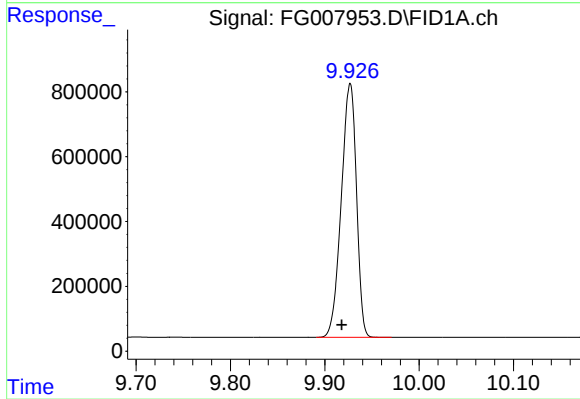


#5 N-HEXADECANE

R.T.: 9.927 min
Delta R.T.: 0.009 min
Response: 8766225
Conc: 56.58 ug/ml

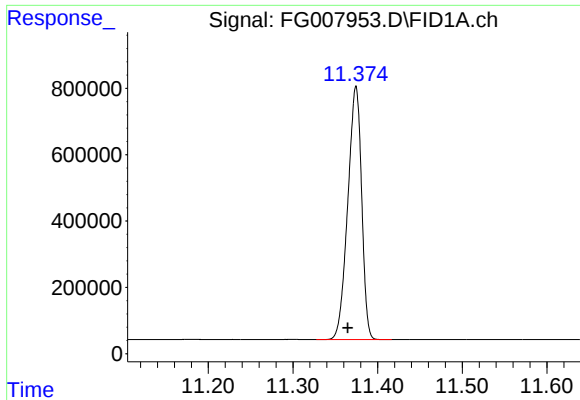


#6 N-OCTADECANE

R.T.: 11.374 min
Delta R.T.: 0.010 min
Response: 8676676
Conc: 55.18 ug/ml

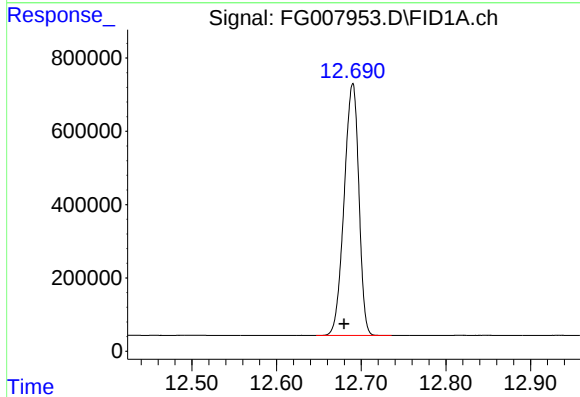


#7 N-EICOSANE

R.T.: 12.690 min
Delta R.T.: 0.010 min
Response: 8293938
Conc: 53.52 ug/ml

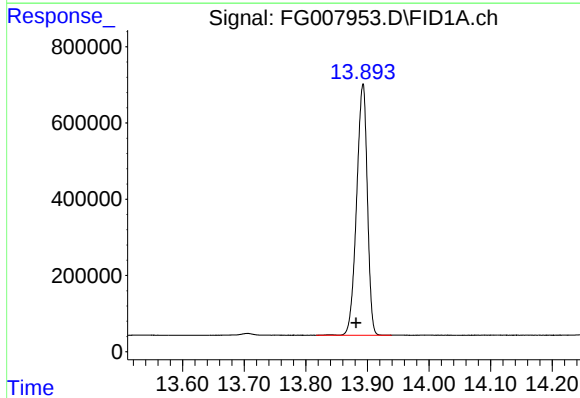


#8 N-DOCOSANE

R.T.: 13.893 min
Delta R.T.: 0.011 min
Response: 7959488
Conc: 51.80 ug/ml

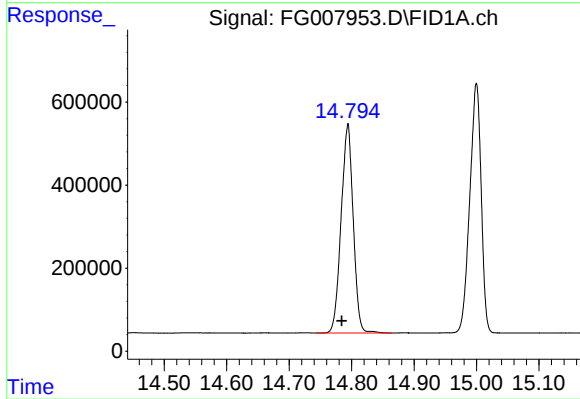


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.794 min
Delta R.T.: 0.010 min
Response: 6759344
Conc: 50.77 ug/ml

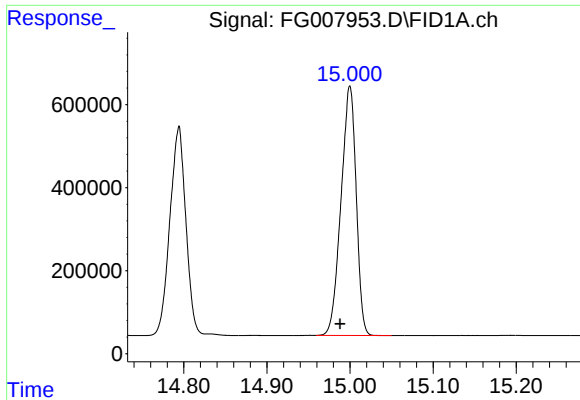


#10 N-TETRACOSANE

R.T.: 15.000 min
Delta R.T.: 0.012 min
Response: 7620428
Conc: 50.08 ug/ml

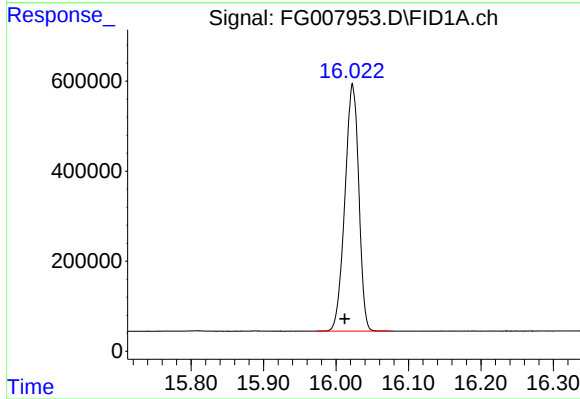

#11 N-HEXACOSANE

R.T.: 16.023 min
Delta R.T.: 0.011 min
Response: 7317188
Conc: 49.12 ug/ml

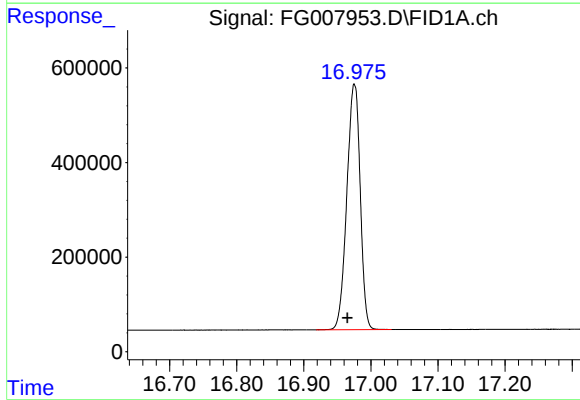

#12 N-OCTACOSANE

R.T.: 16.976 min
Delta R.T.: 0.011 min
Response: 7187617
Conc: 49.08 ug/ml