

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG043024\
 Data File : FG013728.D
 Signal(s) : FID1A.ch
 Acq On : 30 Apr 2024 23:30
 Operator : YP\AJ
 Sample : P2294-03 10X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 01 05:01:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041124.M
 Quant Title :
 QLast Update : Thu Apr 11 13:37:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.071	135042	1.161 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.258	52240	0.398 ug/ml
13) N-TRIACONTANE	18.146	55532	0.428 ug/ml
14) N-DOTRIACONTANE	18.978	45499	0.355 ug/ml
17) N-OCTATRIACONTANE	21.259	344162	3.401 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG043024\
Data File : FG013728.D
Signal(s) : FID1A.ch
Acq On : 30 Apr 2024 23:30
Operator : YP\AJ
Sample : P2294-03 10X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 01 05:01:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041124.M
Quant Title :
QLast Update : Thu Apr 11 13:37:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

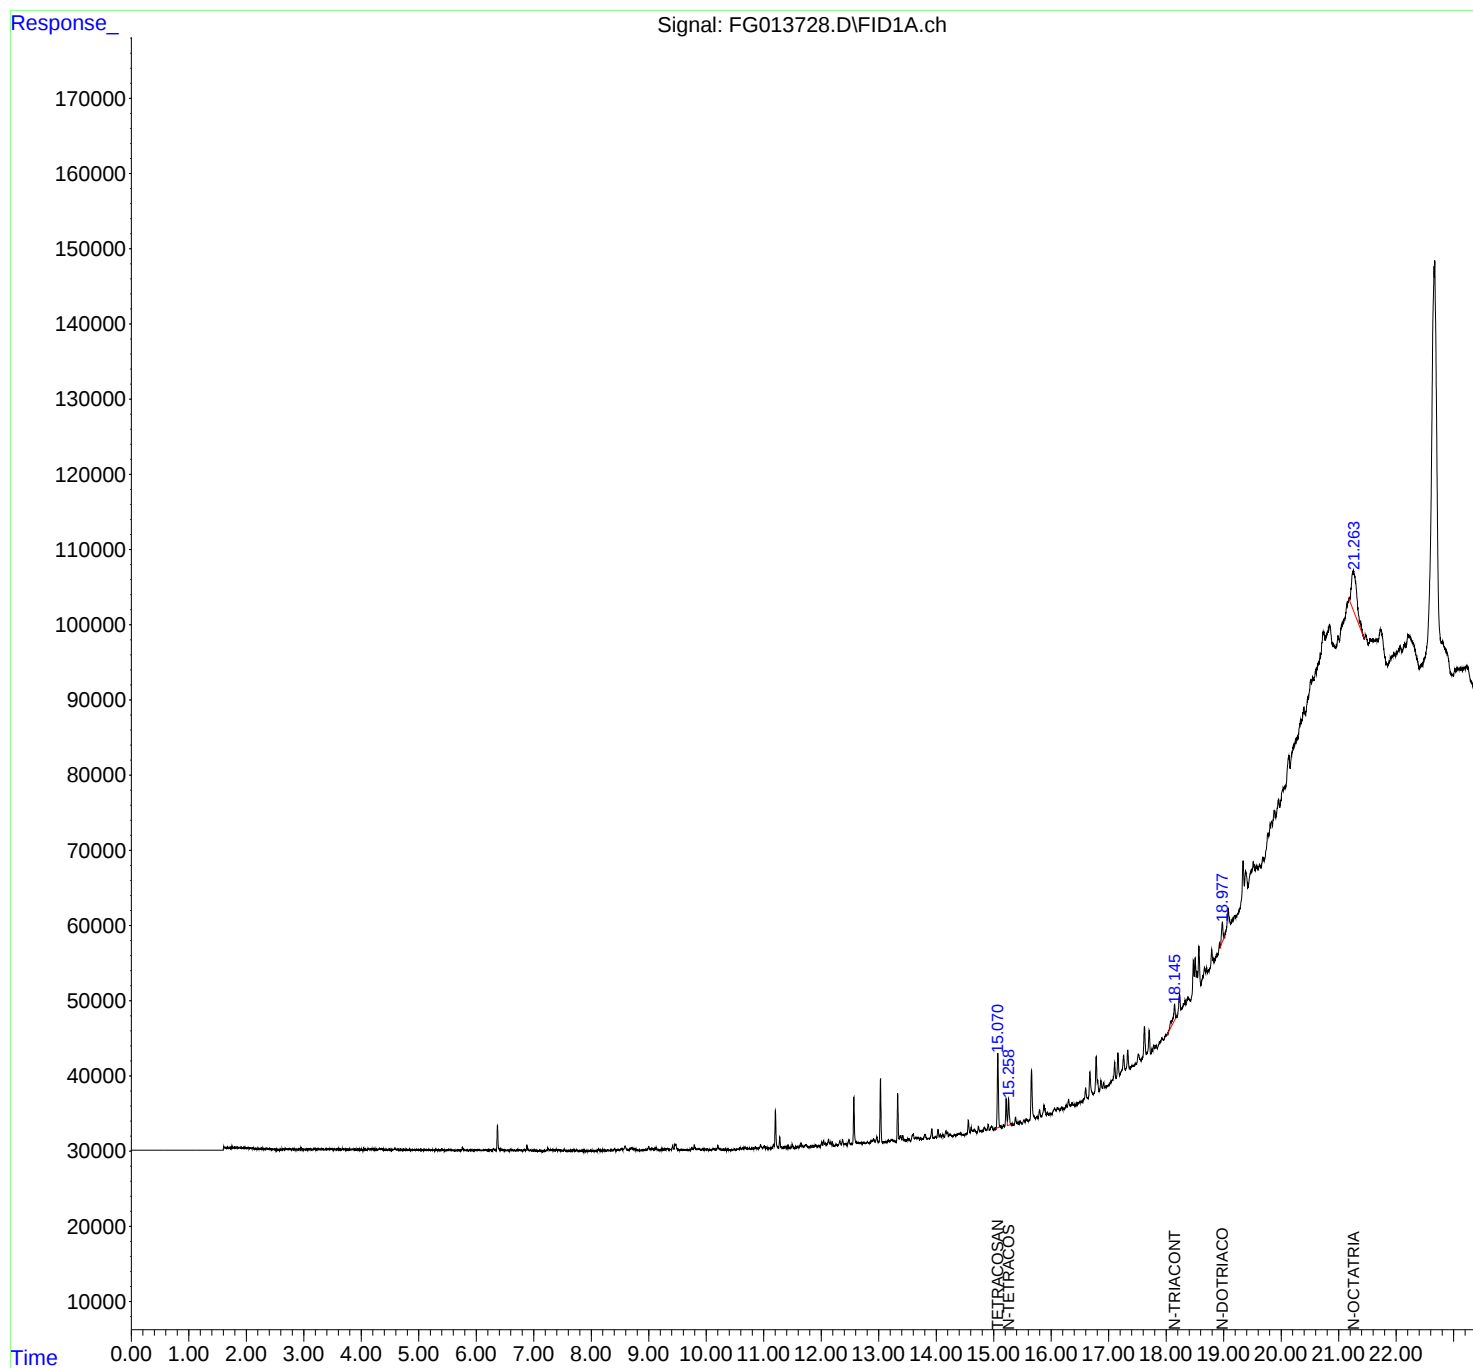


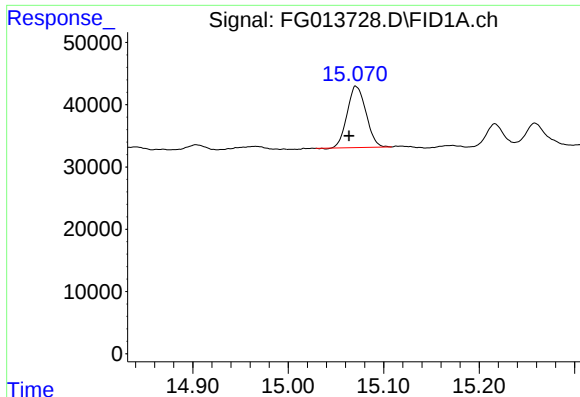

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.071 min
Delta R.T.: 0.007 min
Response: 135042
Conc: 1.16 ug/ml

Instrument :
FID_G
ClientSampleId :

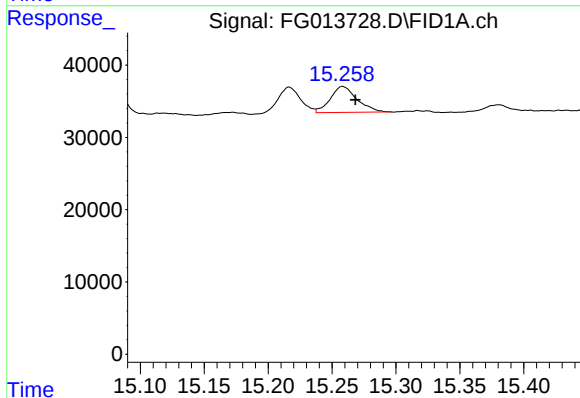


#10 N-TETRACOSANE

R.T.: 15.258 min
Delta R.T.: -0.010 min
Response: 52240
Conc: 0.40 ug/ml

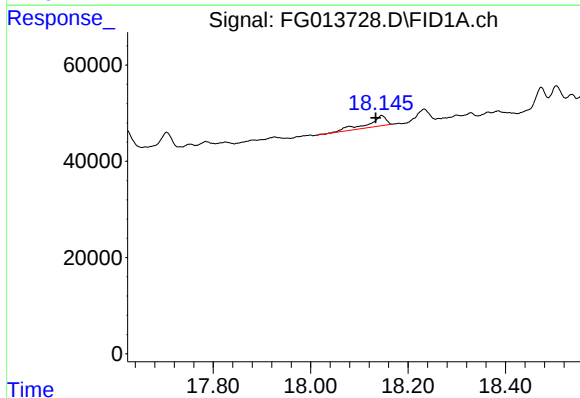


#13 N-TRIACONTANE

R.T.: 18.146 min
Delta R.T.: 0.012 min
Response: 55532
Conc: 0.43 ug/ml

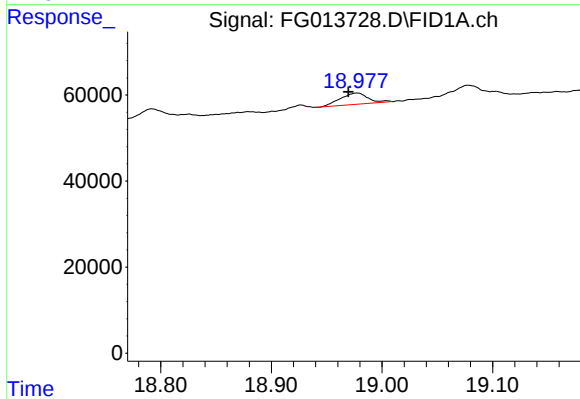

#14 N-DOTRIACONTANE

R.T.: 18.978 min
Delta R.T.: 0.008 min
Response: 45499
Conc: 0.36 ug/ml

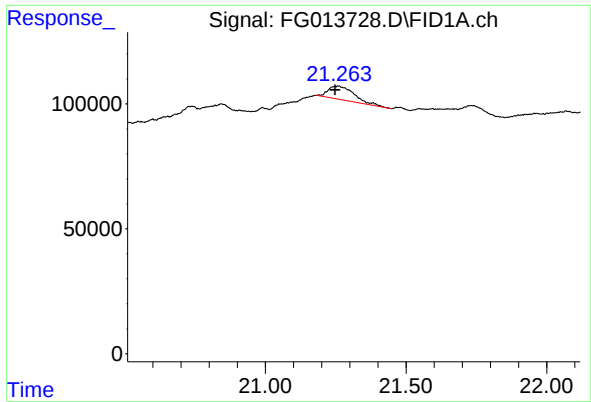

#17 N-OCTATRIACONTANE

R.T.: 21.259 min
Delta R.T.: 0.011 min
Response: 344162
Conc: 3.40 ug/ml

Instrument :
FID_G
ClientSampleId :