

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG050421\  
Data File : FG007958.D  
Signal(s) : FID1A.ch  
Acq On : 04 May 2021 09:58  
Operator : DD\AJ  
Sample : M2260-01  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: May 05 01:34:45 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG042121.M  
Quant Title :  
QLast Update : Thu Apr 22 01:54:01 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

|                             | Compound                 | R.T.   | Response | Conc Units   |
|-----------------------------|--------------------------|--------|----------|--------------|
| -----                       |                          |        |          |              |
| System Monitoring Compounds |                          |        |          |              |
| 9) S                        | TETRACOSANE-d50 (SURR... | 14.789 | 1915015  | 14.385 ug/ml |
|                             |                          |        |          |              |
| Target Compounds            |                          |        |          |              |
| 4)                          | N-TETRADECANE            | 8.375f | 123865   | 0.794 ug/ml  |
| -----                       |                          |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG050421\  
Data File : FG007958.D  
Signal(s) : FID1A.ch  
Acq On : 04 May 2021 09:58  
Operator : DD\AJ  
Sample : M2260-01  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: May 05 01:34:45 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG042121.M  
Quant Title :  
QLast Update : Thu Apr 22 01:54:01 2021  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

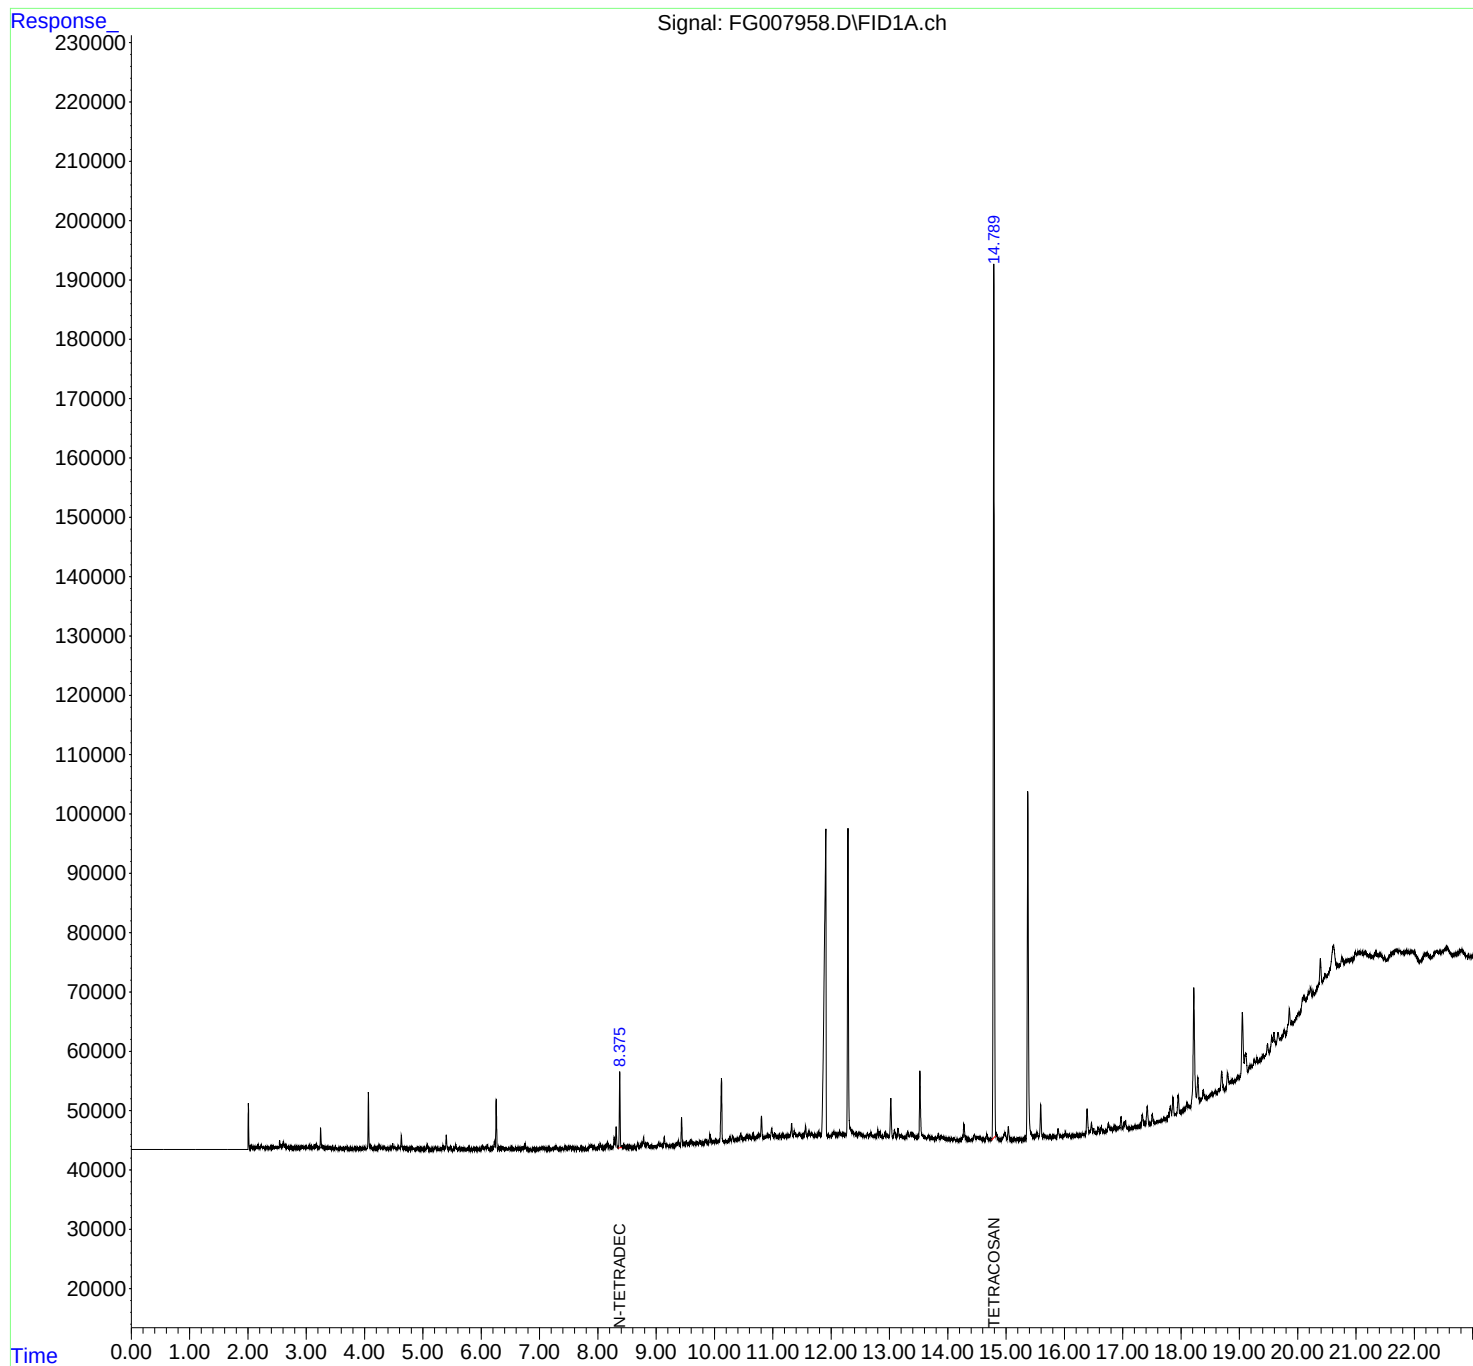

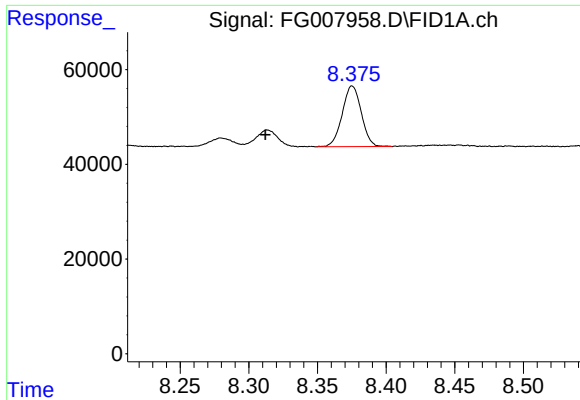

#4 N-TETRADECANE

R.T.: 8.375 min  
Delta R.T.: 0.063 min  
Response: 123865  
Conc: 0.79 ug/ml

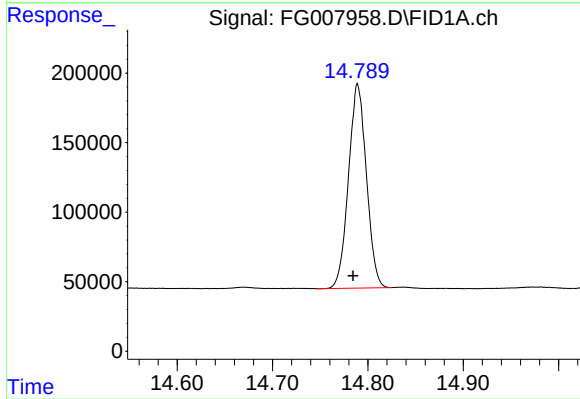

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.789 min  
Delta R.T.: 0.005 min  
Response: 1915015  
Conc: 14.38 ug/ml