

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050422AL\
 Data File : FG009750.D
 Signal(s) : FID1A.ch
 Acq On : 04 May 2022 19:40
 Operator : AJ\MA
 Sample : N2667-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 05 01:41:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH FG050322.M
 Quant Title : GC Extractables
 QLast Update : Tue May 03 14:00:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.837	4669826	30.466 ug/ml
Spiked Amount 50.000		Recovery =	60.93%
12) S 1-chlorooctadecane (S...	12.288	3706046	30.455 ug/ml
Spiked Amount 50.000		Recovery =	60.91%
Target Compounds			
10) T n-Eicosane (C20)	11.886	179677	1.290 ug/ml
14) T n-Tetracosane (C24)	14.115	69750	0.489 ug/ml
16) T n-Octacosane (C28)	16.136	62097	0.437 ug/ml
18) T n-Dotriacontane (C32)	17.850	71308	0.541 ug/ml
19) T n-Tetratriacontane (C34)	18.656	46686	0.398 ug/ml
20) T n-Hexatriacontane (C36)	19.399	26440	0.264 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050422AL\
Data File : FG009750.D
Signal(s) : FID1A.ch
Acq On : 04 May 2022 19:40
Operator : AJ\MA
Sample : N2667-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 05 01:41:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH FG050322.M
Quant Title : GC Extractables
QLast Update : Tue May 03 14:00:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

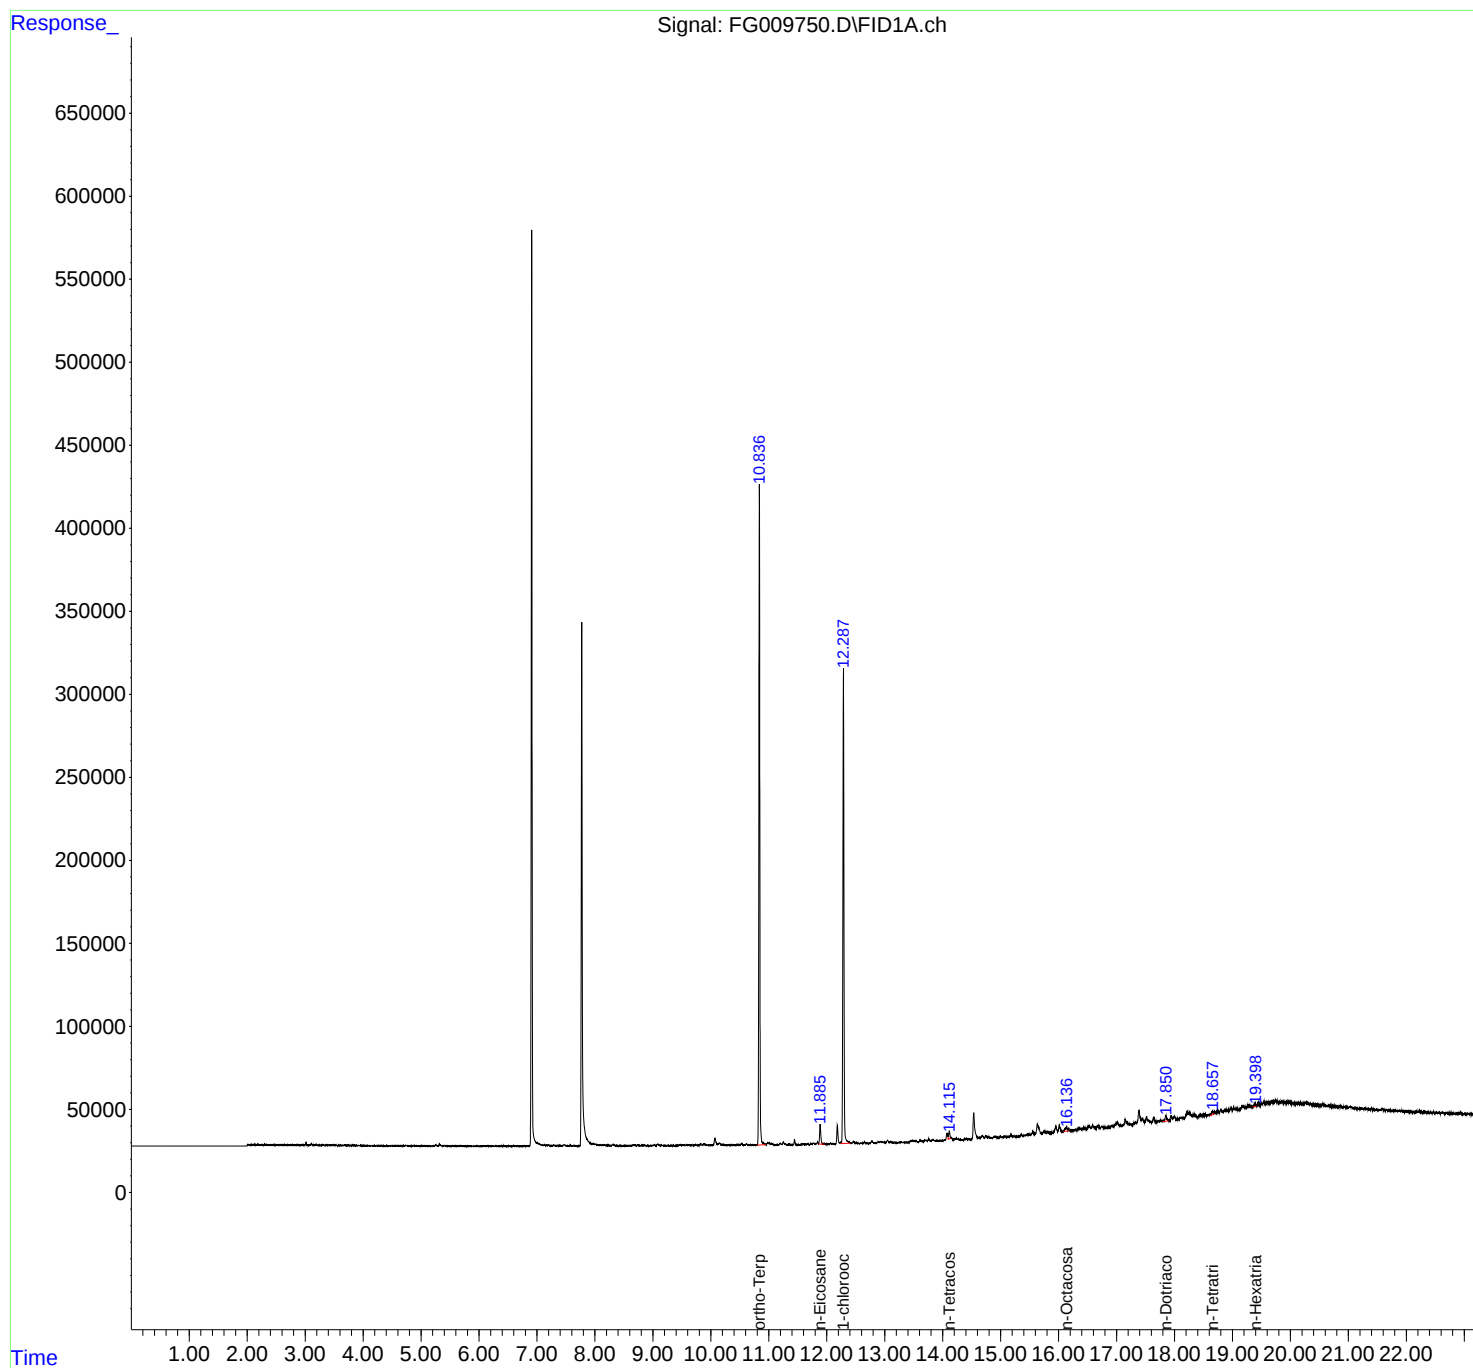


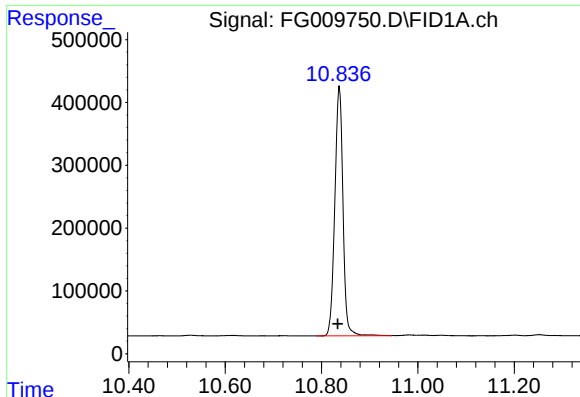

#9 ortho-Terphenyl (SURR)


R.T.: 10.837 min
Delta R.T.: 0.003 min
Response: 4669826
Conc: 30.47 ug/ml

Instrument :
FID_G
ClientSampleId :

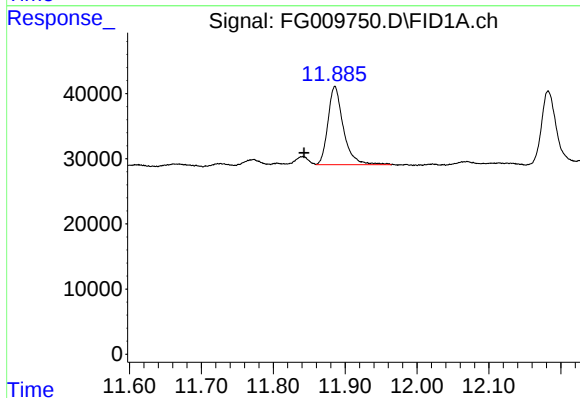


#10 n-Eicosane (C20)

R.T.: 11.886 min
Delta R.T.: 0.043 min
Response: 179677
Conc: 1.29 ug/ml

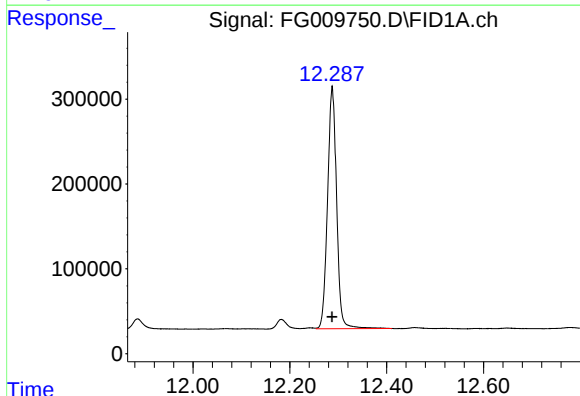


#12 1-chlorooctadecane (SURR)

R.T.: 12.288 min
Delta R.T.: 0.000 min
Response: 3706046
Conc: 30.45 ug/ml

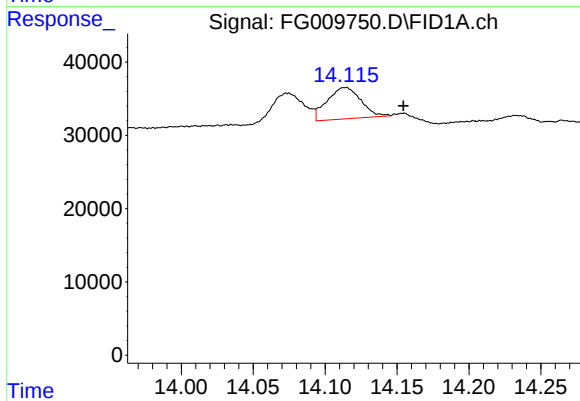

#14 n-Tetracosane (C24)


R.T.: 14.115 min
Delta R.T.: -0.039 min
Response: 69750
Conc: 0.49 ug/ml

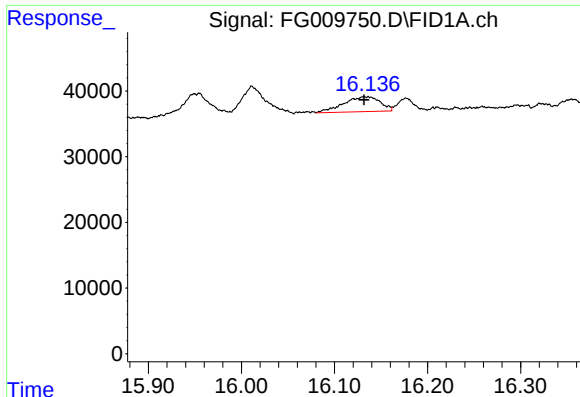

#16 n-Octacosane (C28)


R.T.: 16.136 min
Delta R.T.: 0.005 min
Response: 62097
Conc: 0.44 ug/ml

Instrument :
FID_G
ClientSampleId :

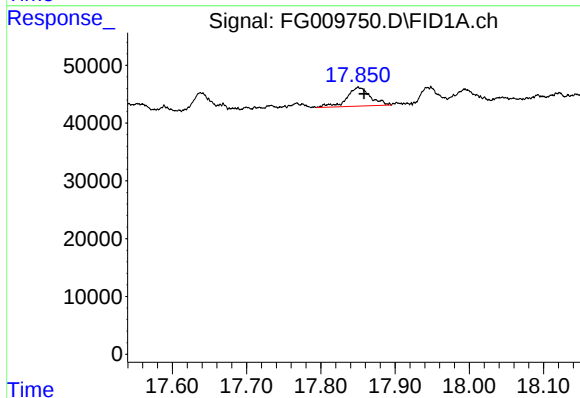


#18 n-Dotriacontane (C32)

R.T.: 17.850 min
Delta R.T.: -0.008 min
Response: 71308
Conc: 0.54 ug/ml

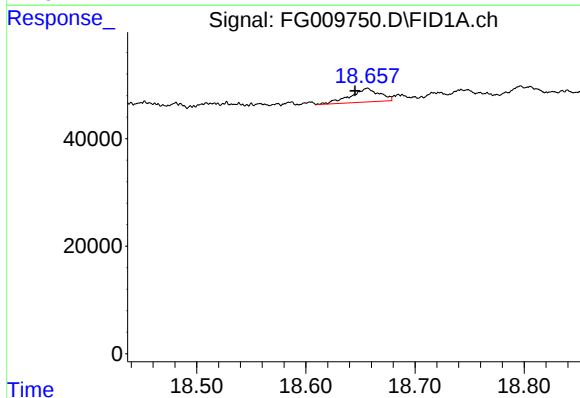

#19 n-Tetratriacontane (C34)

R.T.: 18.656 min
Delta R.T.: 0.011 min
Response: 46686
Conc: 0.40 ug/ml

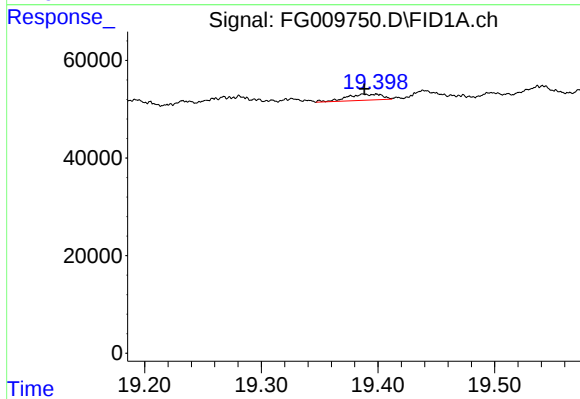

#20 n-Hexatriacontane (C36)

R.T.: 19.399 min
Delta R.T.: 0.010 min
Response: 26440
Conc: 0.26 ug/ml