

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050621\
 Data File : FG007992.D
 Signal(s) : FID1A.ch
 Acq On : 06 May 2021 16:55
 Operator : DD\AJ
 Sample : M2303-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 07 02:16:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
 Quant Title :
 QLast Update : Thu Apr 22 01:54:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.786	2115666	15.892 ug/ml
Target Compounds			
3) N-DODECANE	6.531	277052	1.811 ug/ml
4) N-TETRADECANE	8.288	749108	4.799 ug/ml
5) N-HEXADECANE	9.896	125071	0.807 ug/ml
6) N-OCTADECANE	11.386	103315	0.657 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG050621\
Data File : FG007992.D
Signal(s) : FID1A.ch
Acq On : 06 May 2021 16:55
Operator : DD\AJ
Sample : M2303-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 07 02:16:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042121.M
Quant Title :
QLast Update : Thu Apr 22 01:54:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

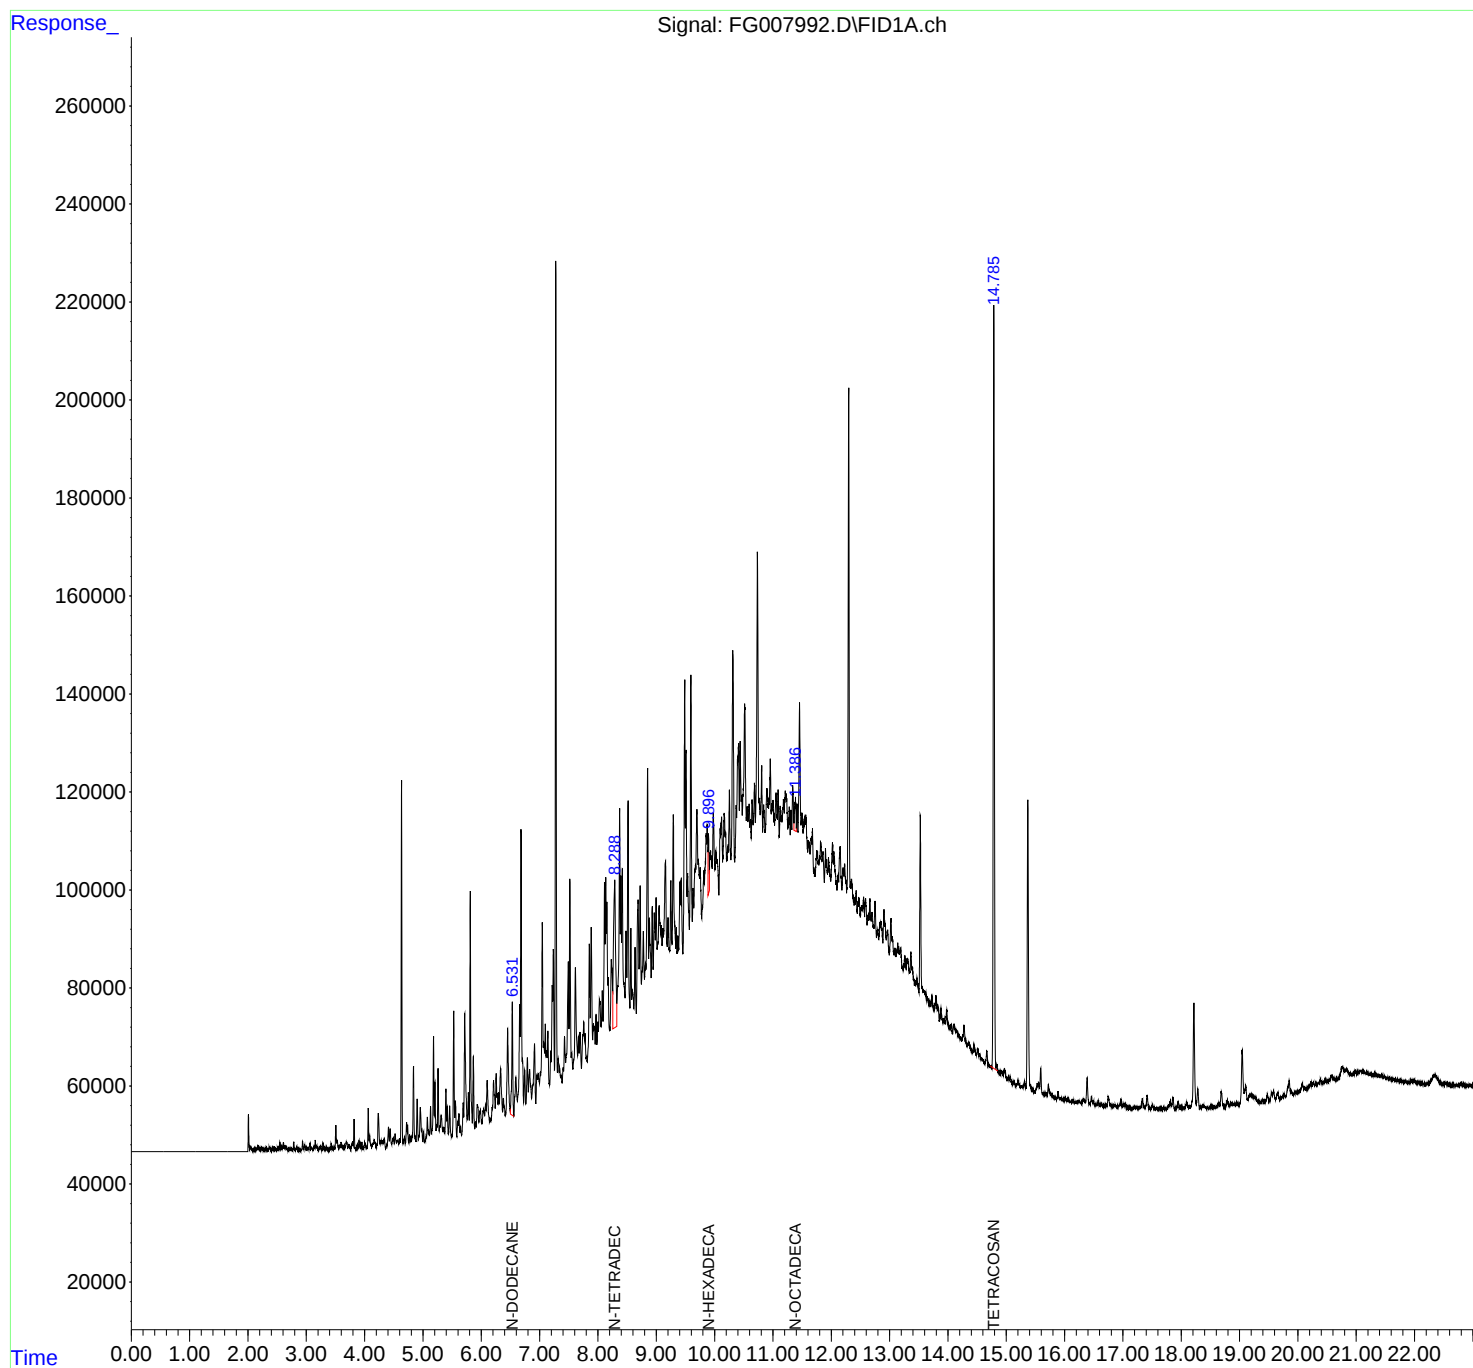


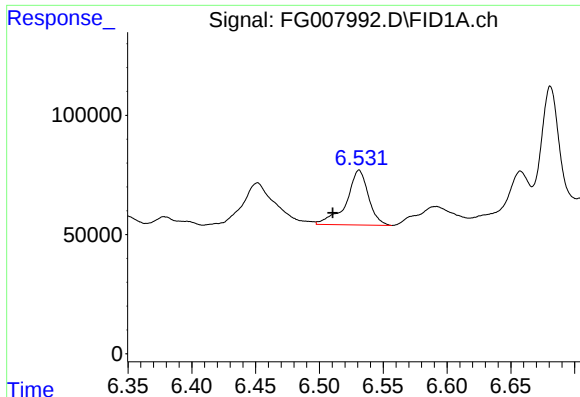

#3 N-DODECANE


R.T.: 6.531 min
Delta R.T.: 0.021 min
Response: 277052
Conc: 1.81 ug/ml

Instrument :
FID_G
ClientSampleId :

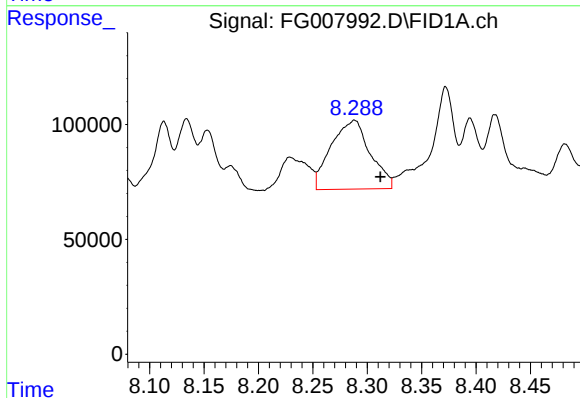


#4 N-TETRADECANE

R.T.: 8.288 min
Delta R.T.: -0.024 min
Response: 749108
Conc: 4.80 ug/ml

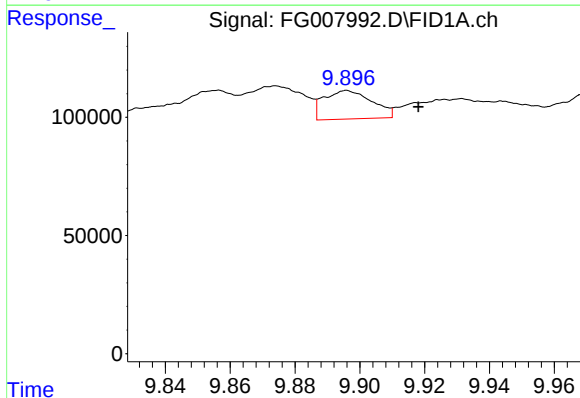


#5 N-HEXADECANE

R.T.: 9.896 min
Delta R.T.: -0.022 min
Response: 125071
Conc: 0.81 ug/ml

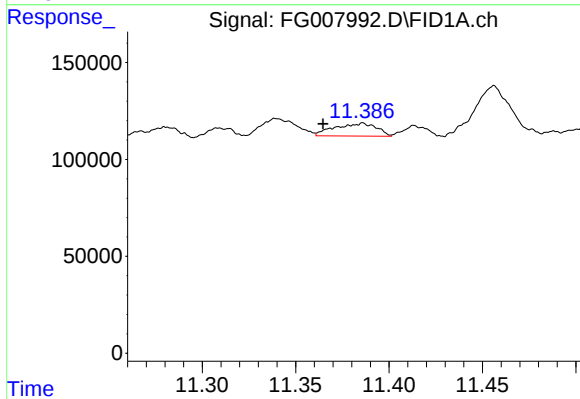

#6 N-OCTADECANE

R.T.: 11.386 min
Delta R.T.: 0.021 min
Response: 103315
Conc: 0.66 ug/ml

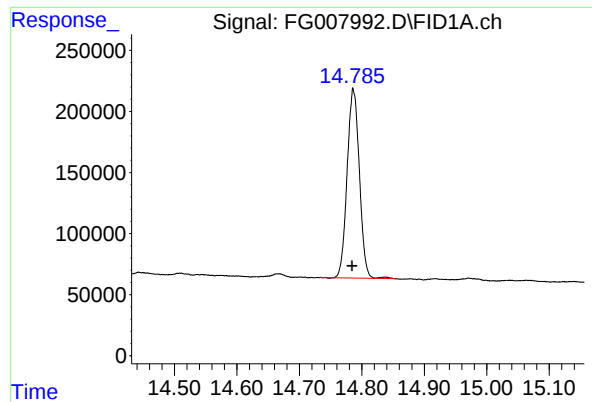

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.786 min
Delta R.T.: 0.002 min
Response: 2115666
Conc: 15.89 ug/ml

Instrument :
FID_G
ClientSampleId :